

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071223\
 Data File : BM040841.D
 Acq On : 12 Jul 2023 18:00
 Operator : MA/JU
 Sample : PB153963BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK963

Quant Time: Jul 13 00:13:22 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 12 05:37:29 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.878	152	2329	0.400	ng/ul	0.00
4) Naphthalene-d8	10.680	136	8974	0.400	ng/ul	#-0.01
9) Acenaphthene-d10	14.523	164	4522	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.274	188	8060	0.400	ng/ul	-0.02
17) Chrysene-d12	21.480	240	6118	0.400	ng/ul	0.00
23) Perylene-d12	0.000	264	0	0.000	ng/ul	-23.87
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.292	96	25230	6.896	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.275	152	4892	0.389	ng/ul	-0.01
18) Fluoranthene-d10	19.306	212	6383	0.325	ng/ul	-0.01
Target Compounds						
					Qvalue	
12) Fluorene	15.517	166	1910	0.105	ng/ul#	18
16) Anthracene	17.375	178	470	0.022	ng/ul#	1
20) Pyrene	19.673	202	1424	0.051	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071223\
Data File : BM040841.D
Acq On : 12 Jul 2023 18:00
Operator : MA/JU
Sample : PB153963BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK963

Quant Time: Jul 13 00:13:22 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 12 05:37:29 2023
Response via : Initial Calibration




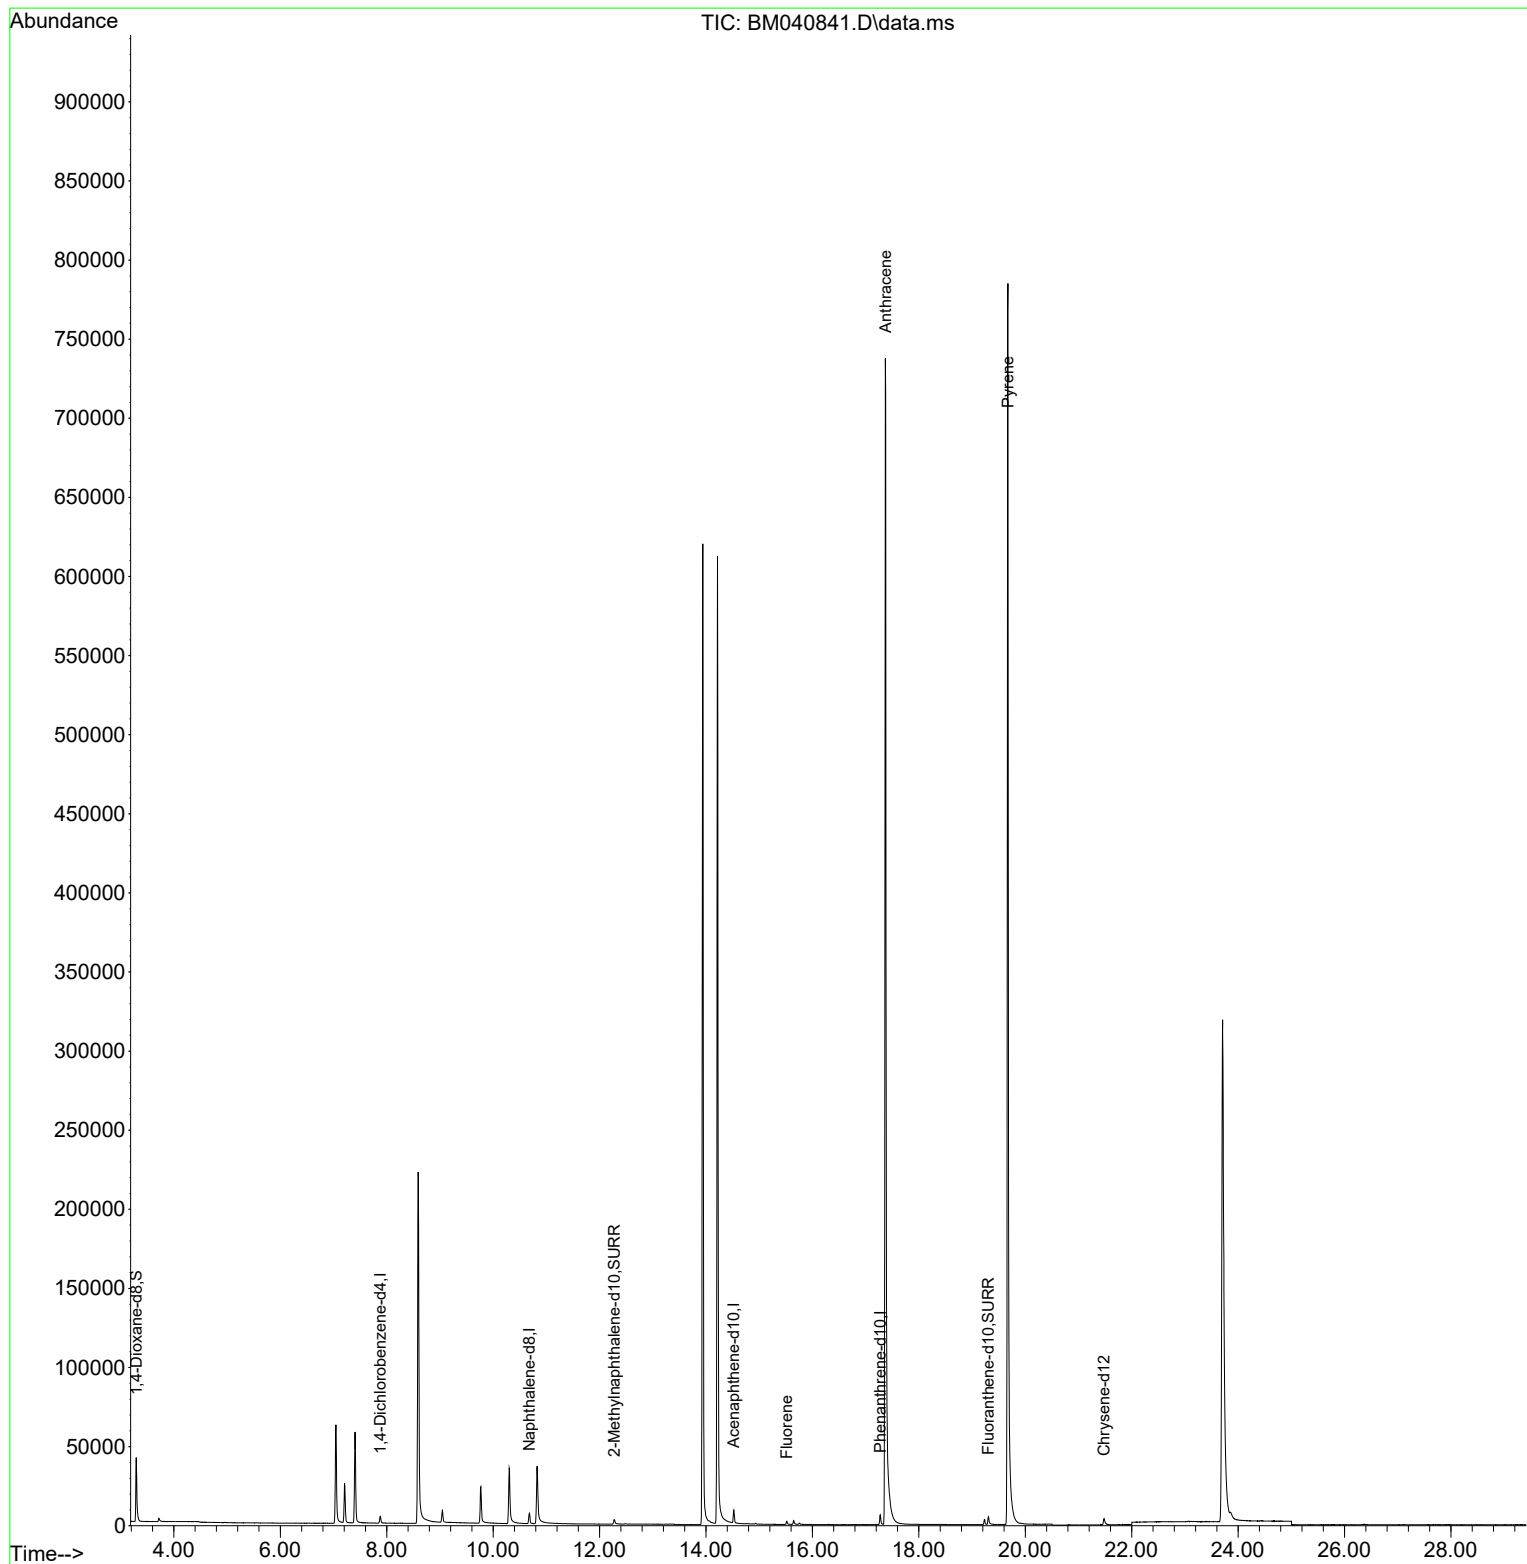


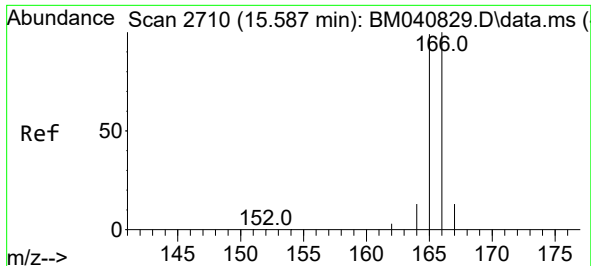

#12
 Fluorene
 Concen: 0.105 ng/ul
 RT: 15.517 min Scan# 21
 Delta R.T. -0.074 min
 Lab File: BM040841.D
 Acq: 12 Jul 2023 18:00




Instrument :
 BNA_M
 ClientSampleId :
 SBLK963


Tgt Ion:166 Resp: 1910
 Ion Ratio Lower Upper
 166 100
 165 12.9 79.6 119.4#
 167 34.0 11.4 17.0#

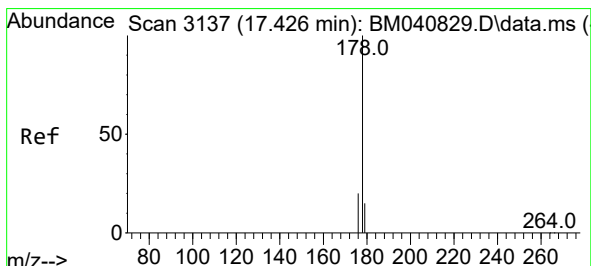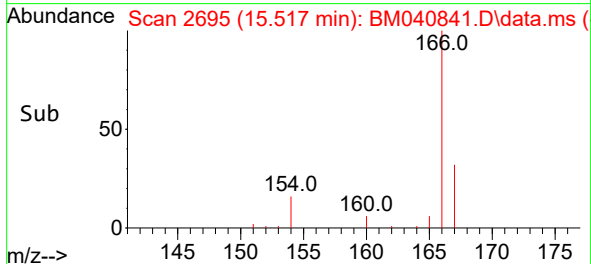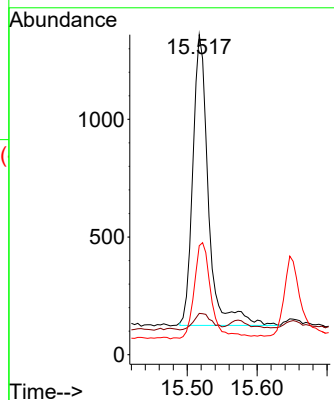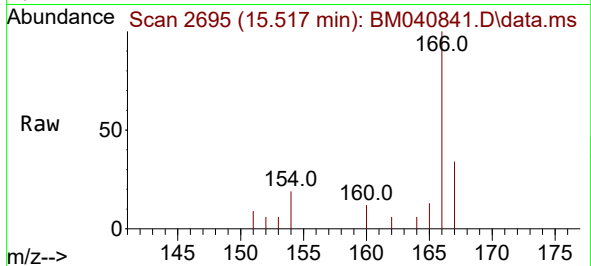

#16
 Anthracene
 Concen: 0.022 ng/ul
 RT: 17.375 min Scan# 3125
 Delta R.T. -0.055 min
 Lab File: BM040841.D
 Acq: 12 Jul 2023 18:00

Tgt Ion:178 Resp: 470
 Ion Ratio Lower Upper
 178 100
 179 204.7 12.9 19.3#
 176 31.9 15.8 23.6#

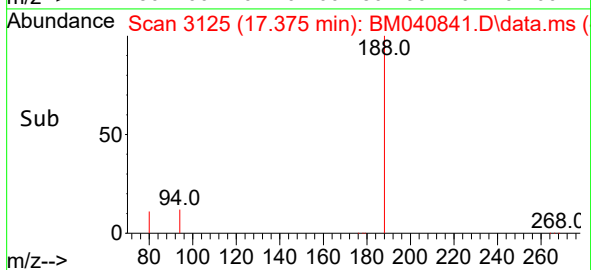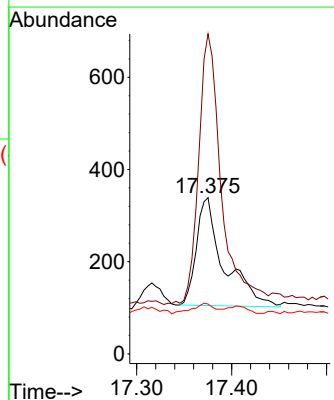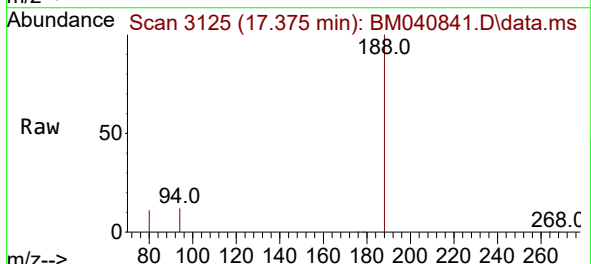

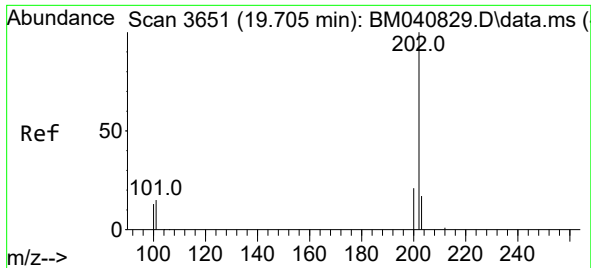

#20

Pyrene

Concen: 0.051 ng/ul

RT: 19.673 min Scan# 30

Delta R.T. -0.037 min

Lab File: BM040841.D


Acq: 12 Jul 2023 18:00

Instrument :

BNA_M

ClientSampleId :

SBLK963

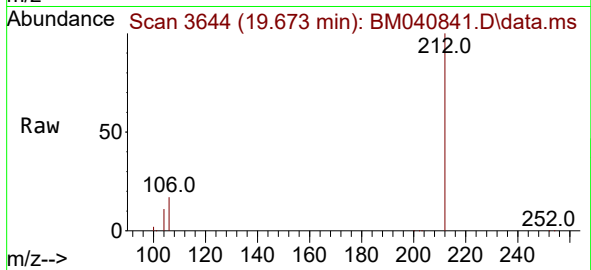

Tgt Ion:202 Resp: 1424

Ion Ratio Lower Upper

202 100

101 188.4 12.6 18.8#

100 1372.3 9.8 14.6#

