




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071223\
 Data File : BM040829.D
 Acq On : 12 Jul 2023 09:32
 Operator : MA/JU
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_M
 LabSampleId :
 SSTDCCC0.4

Manual IntegrationsAPPROVED

Quant Time: Jul 13 00:11:50 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 12 05:37:29 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/13/2023
 Supervised By :mohammad ahmed 07/13/2023

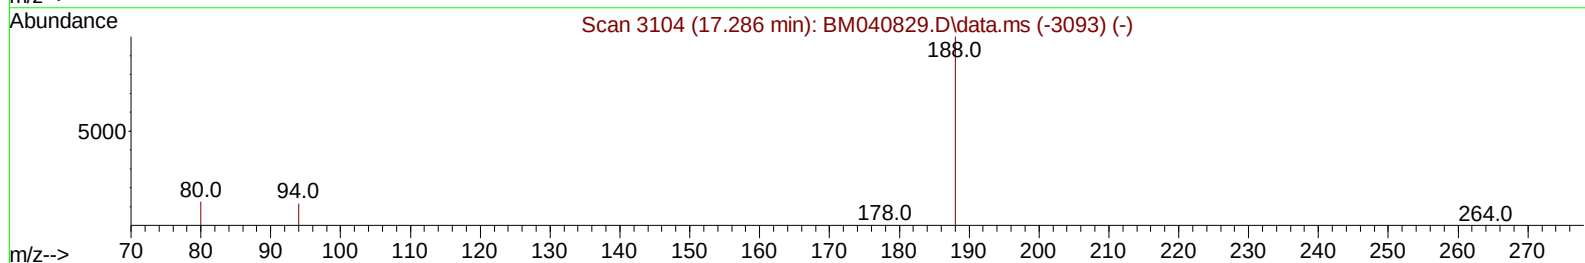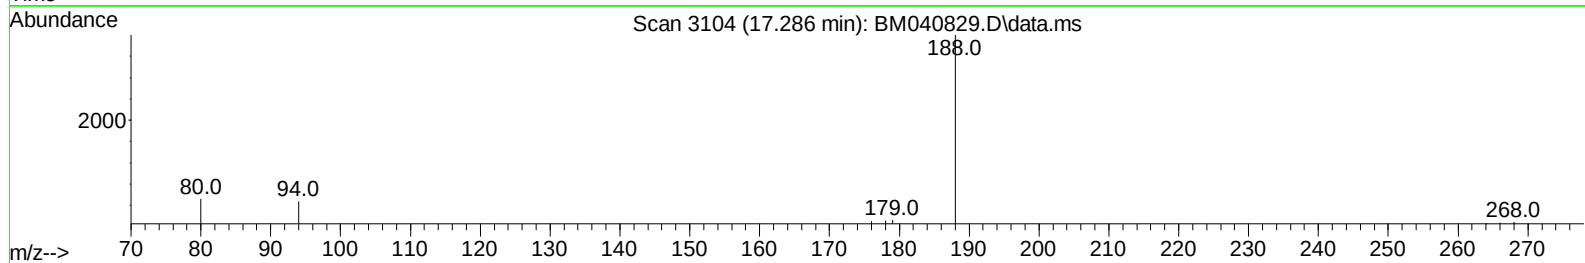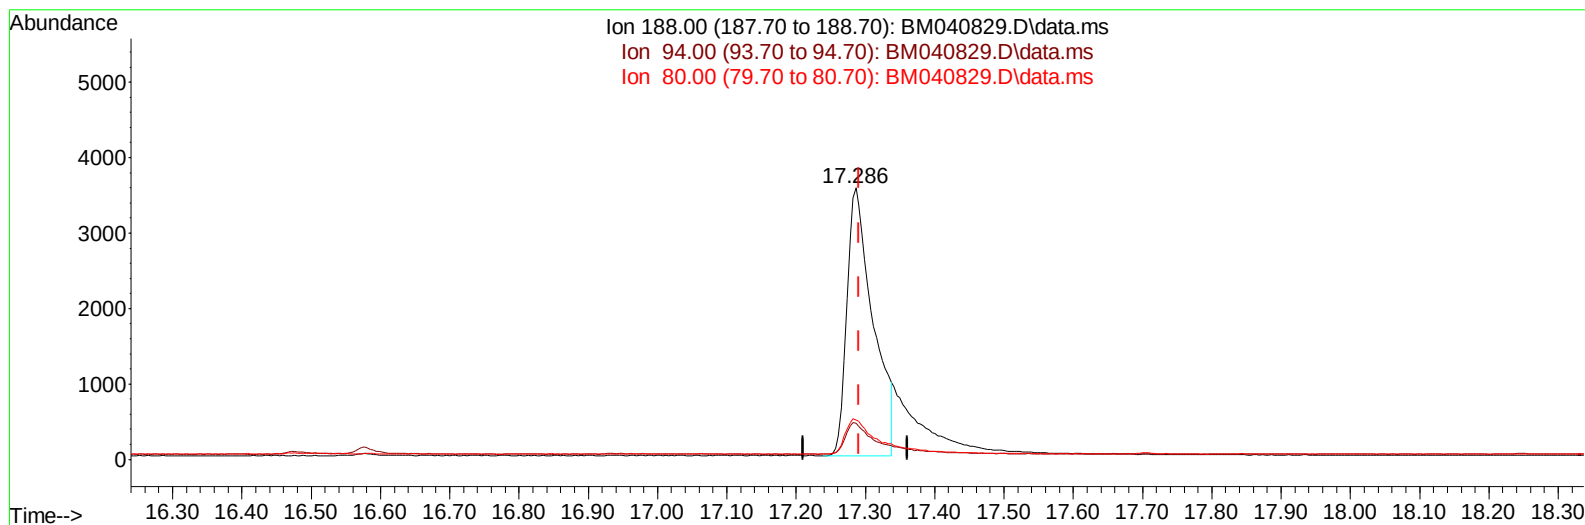

TIC: BM040829.D\data.ms

(13) Phenanthrene-d10 (I)

17.286min (-0.004) 0.40 ng/u1

response 9224

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	11.80	13.36
80.00	13.00	14.59
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071223\
Data File : BM040829.D
Acq On : 12 Jul 2023 09:32
Operator : MA/JU
Sample : SSTDCCC0.4
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_M
LabSampleId :
SSTDCCC0.4

Manual IntegrationsAPPROVED

Quant Time: Jul 13 00:11:50 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 12 05:37:29 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/13/2023
Supervised By :mohammad ahmed 07/13/2023

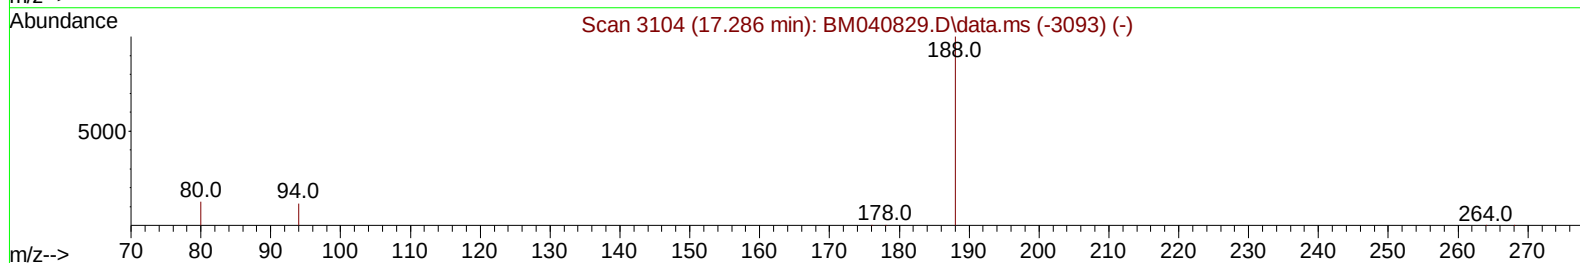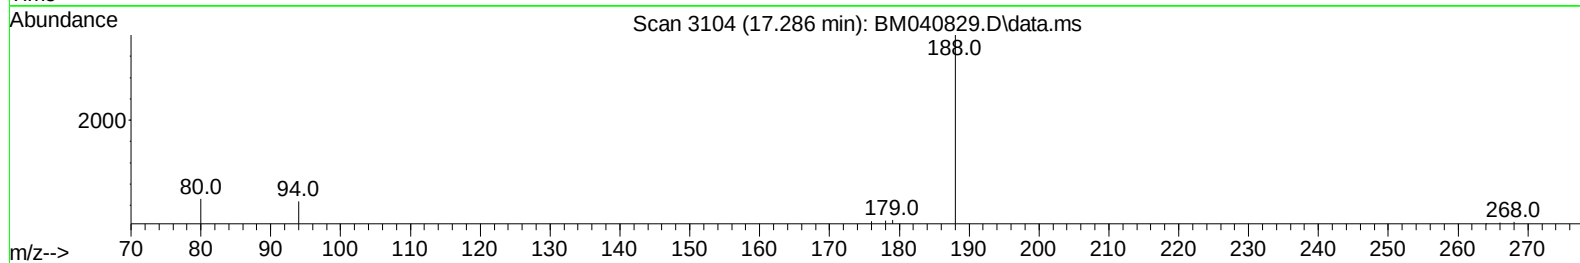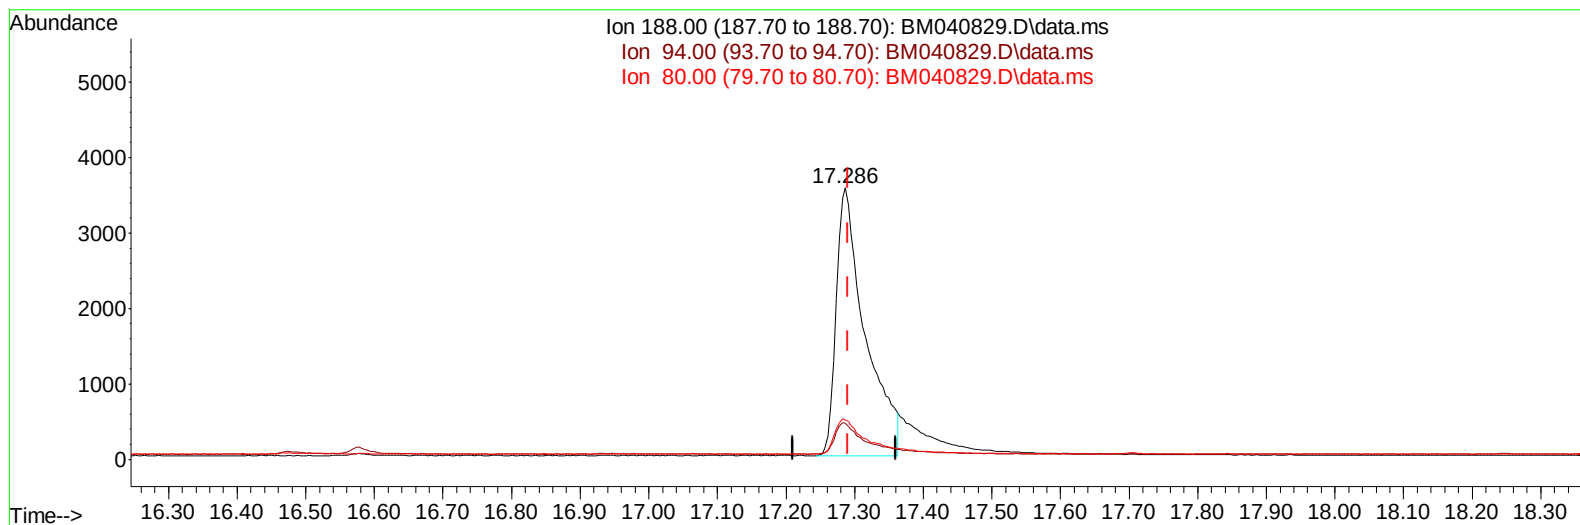

TIC: BM040829.D\data.ms

(13) Phenanthrene-d10 (I)

17.286min (-0.004) 0.40 ng/ul m

response 10332

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	11.80	13.36
80.00	13.00	14.59
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071223\
 Data File : BM040829.D
 Acq On : 12 Jul 2023 09:32
 Operator : MA/JU
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_M
 LabSampleId :
 SSTDCCC0.4

Manual IntegrationsAPPROVED

Quant Time: Jul 13 00:11:50 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 12 05:37:29 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/13/2023
 Supervised By :mohammad ahmed 07/13/2023

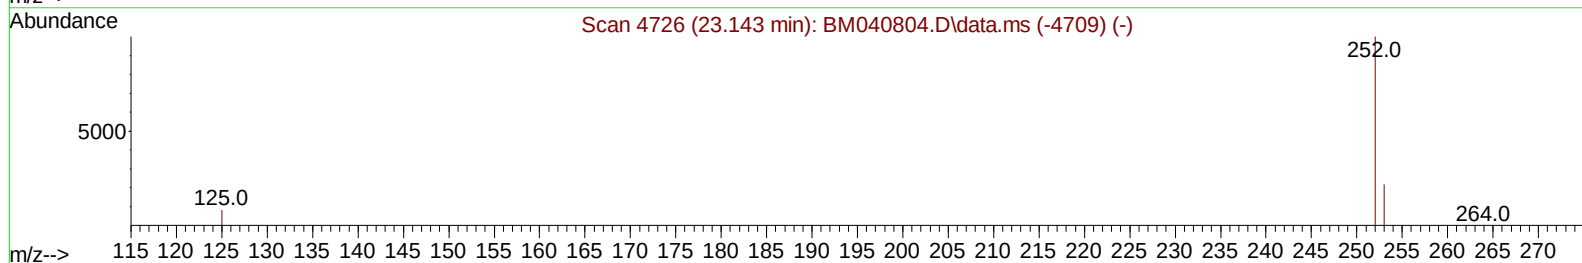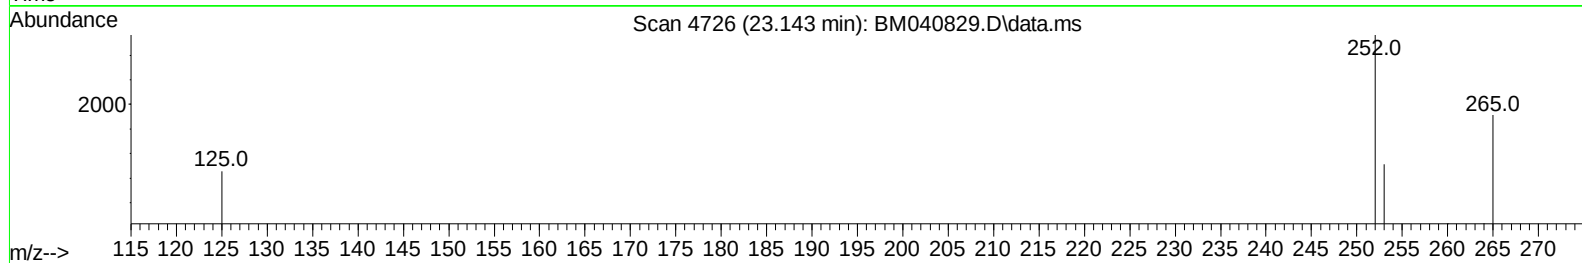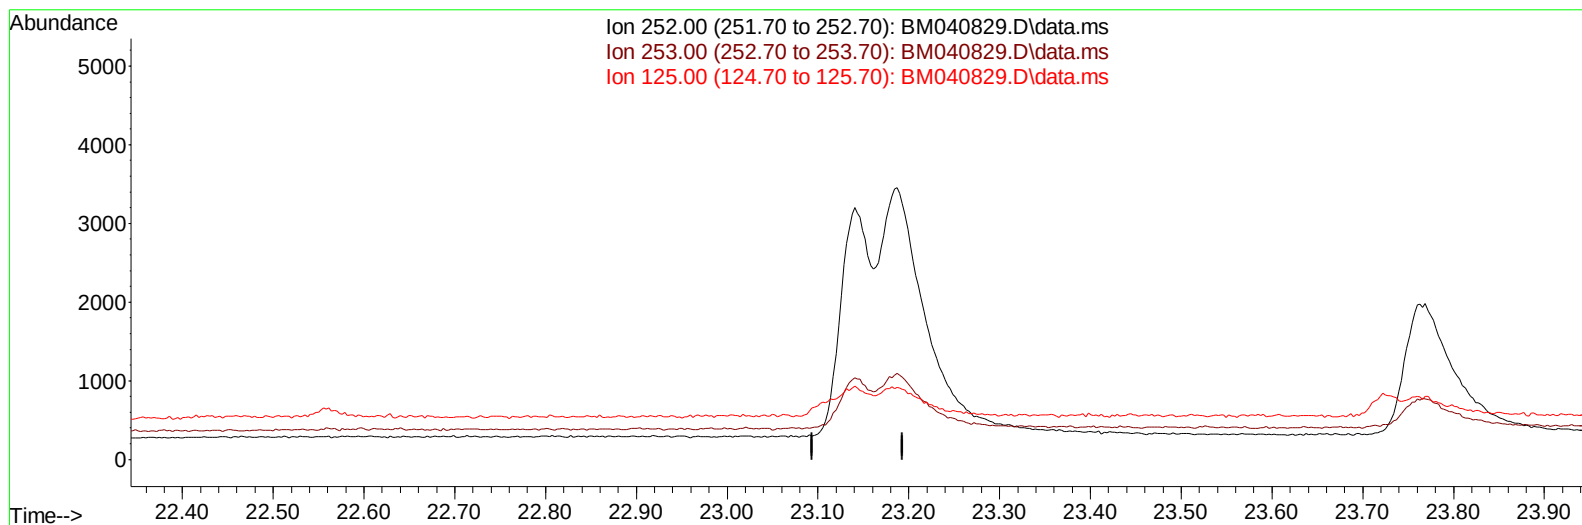

TIC: BM040829.D\data.ms

(24) Benzo(b)fluoranthene

23.143min (-23.143) 0.00 ng/ul

response 0

Ion	Exp%	Act%
252.00	100.00	0.00
253.00	26.40	0.00
125.00	21.50	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071223\
 Data File : BM040829.D
 Acq On : 12 Jul 2023 09:32
 Operator : MA/JU
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_M
 LabSampleId :
 SSTDCCC0.4

Manual IntegrationsAPPROVED

Quant Time: Jul 13 00:11:50 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 12 05:37:29 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/13/2023
 Supervised By :mohammad ahmed 07/13/2023

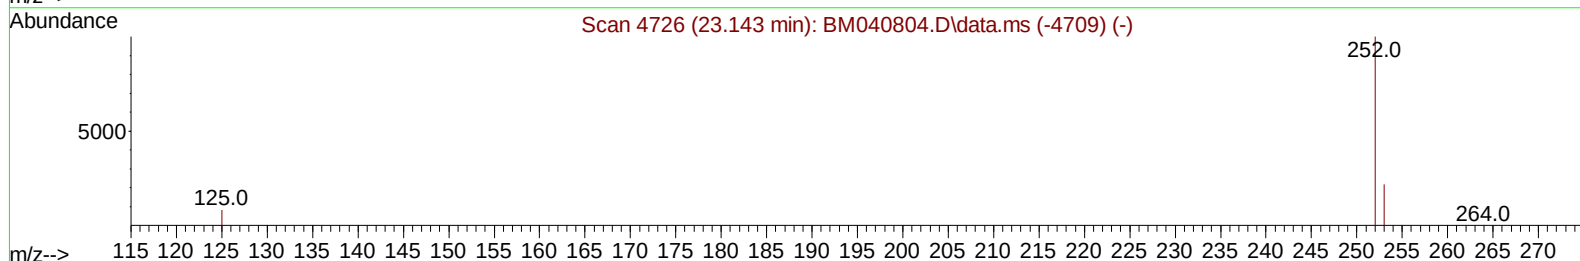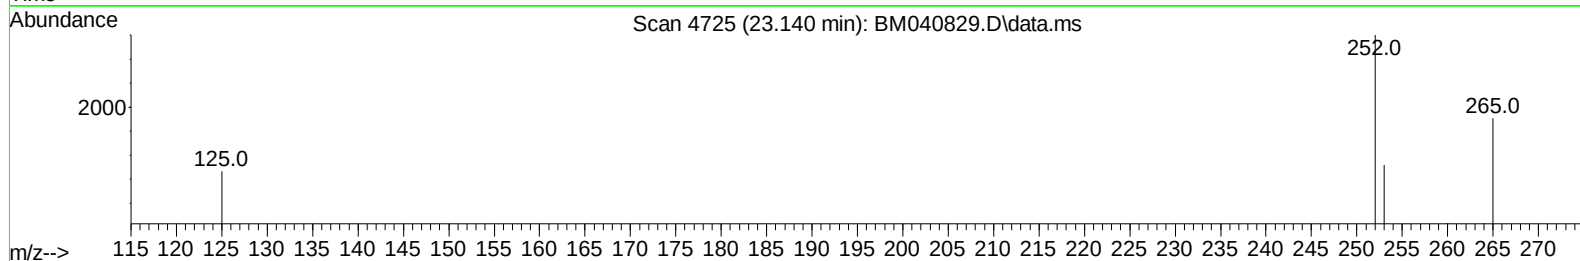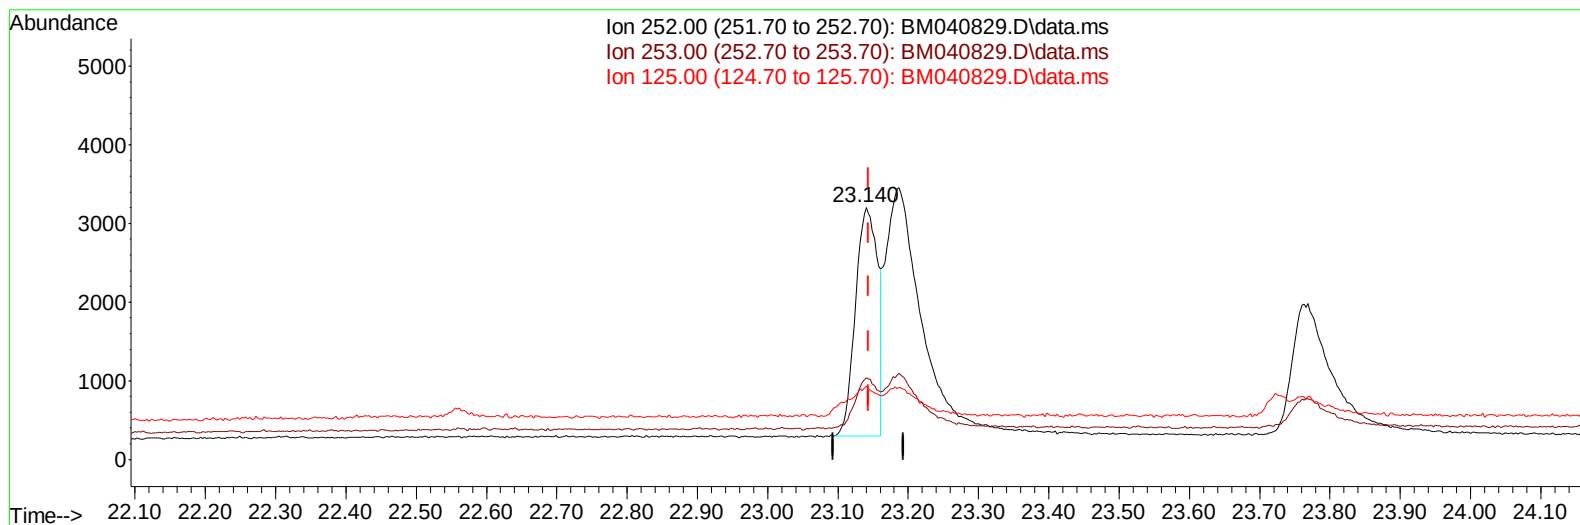

TIC: BM040829.D\data.ms

(24) Benzo(b)fluoranthene

23.140min (-0.003) 0.32 ng/ul m

response 6408

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	26.40	32.47
125.00	21.50	29.04
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071223\
Data File : BM040829.D
Acq On : 12 Jul 2023 09:32
Operator : MA/JU
Sample : SSTDCCC0.4
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_M
LabSampleId :
SSTDCCC0.4

Manual IntegrationsAPPROVED

Quant Time: Jul 13 00:11:50 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 12 05:37:29 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/13/2023
Supervised By :mohammad ahmed 07/13/2023

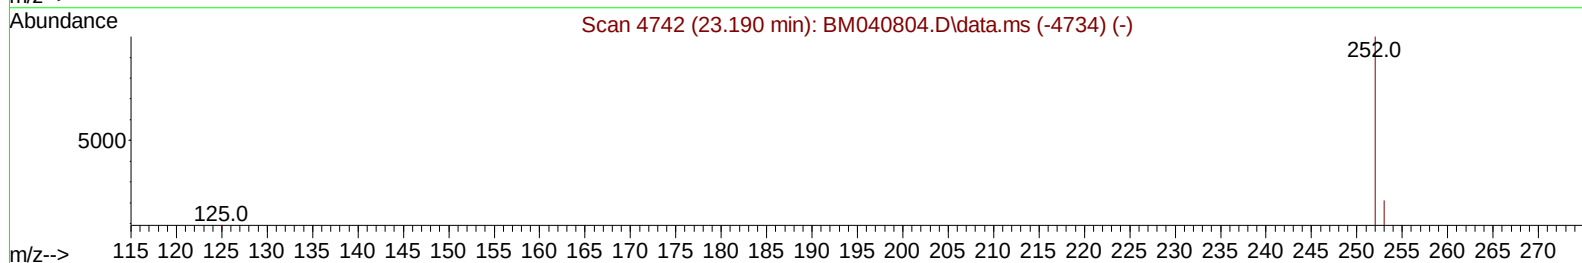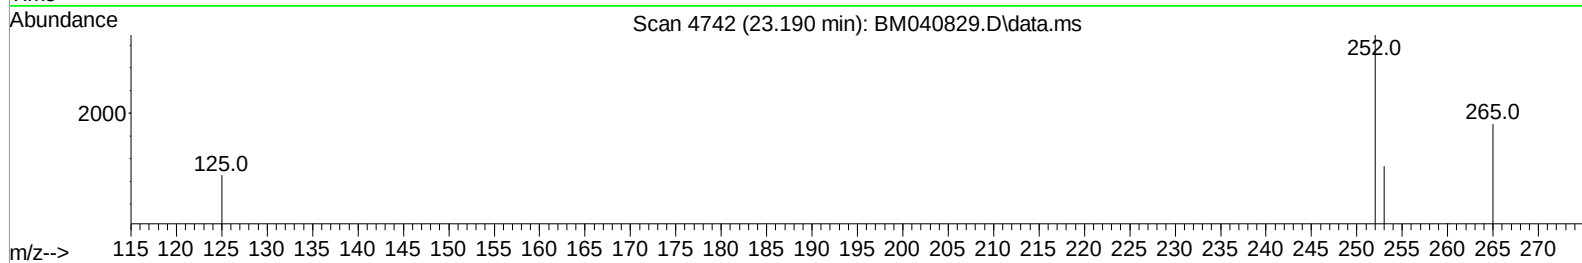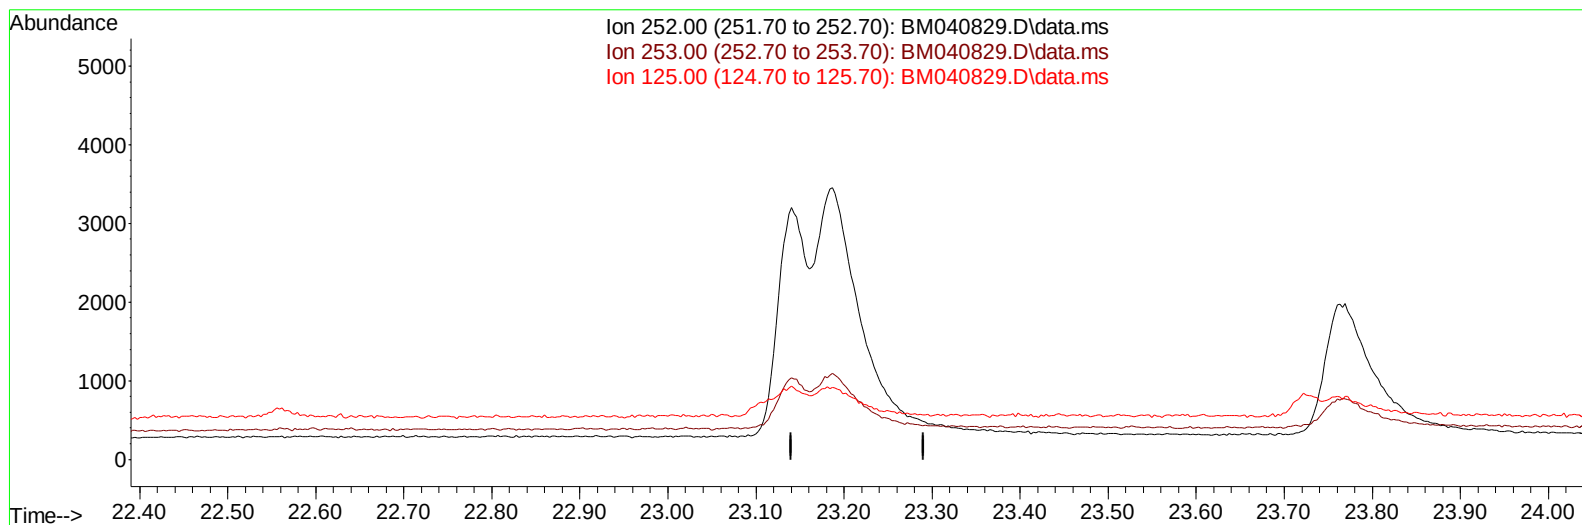

TIC: BM040829.D\data.ms

(25) Benzo(k)fluoranthene

23.190min (-23.190) 0.00 ng/ul

response 0

Ion	Exp%	Act%
252.00	100.00	0.00
253.00	26.50	0.00#
125.00	20.50	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071223\
 Data File : BM040829.D
 Acq On : 12 Jul 2023 09:32
 Operator : MA/JU
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_M
 LabSampleId :
 SSTDCCC0.4

Manual IntegrationsAPPROVED

Quant Time: Jul 13 00:11:50 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 12 05:37:29 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/13/2023
 Supervised By :mohammad ahmed 07/13/2023

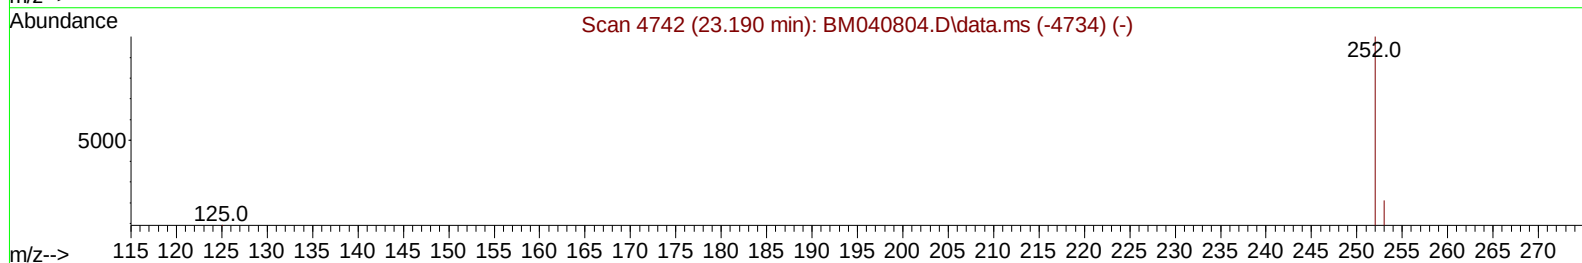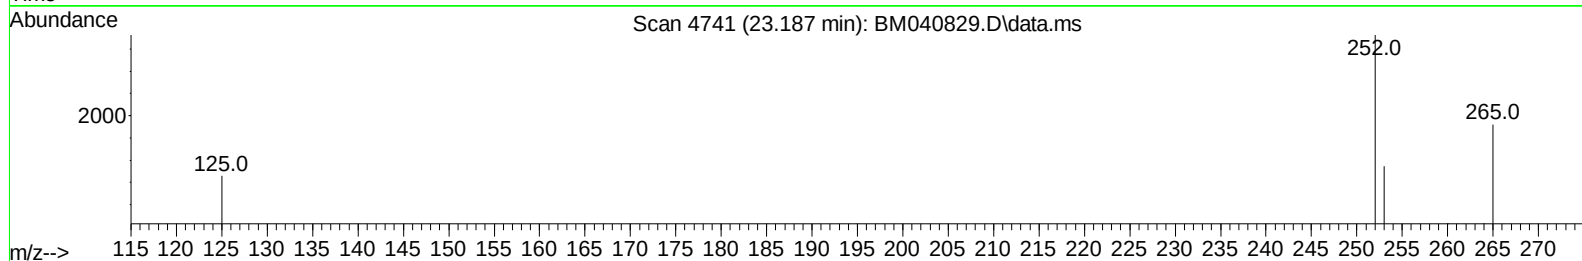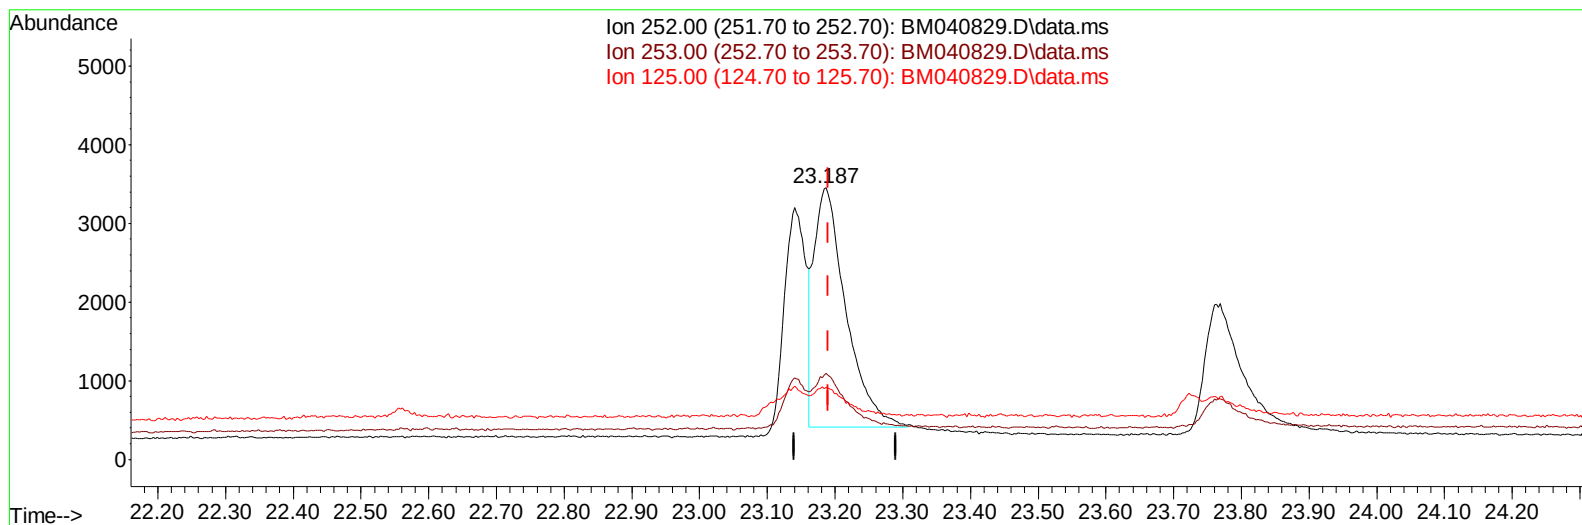

TIC: BM040829.D\data.ms

(25) Benzo(k)fluoranthene

23.187min (-0.003) 0.50 ng/ul m

response 10038

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	26.50	31.61
125.00	20.50	26.66#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071223\
 Data File : BM040829.D
 Acq On : 12 Jul 2023 09:32
 Operator : MA/JU
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_M
 LabSampleId :
 SSTDCCC0.4

Manual IntegrationsAPPROVED

Quant Time: Jul 13 00:11:50 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 12 05:37:29 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/13/2023
 Supervised By :mohammad ahmed 07/13/2023

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.882	152		3545	0.400	ng/ul	0.00
4) Naphthalene-d8	10.685	136		14254	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.527	164		6199	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.286	188		10332m	0.400	ng/ul	0.00
17) Chrysene-d12	21.483	240		6100	0.400	ng/ul	0.00
23) Perylene-d12	23.874	264		5233	0.400	ng/ul	# 0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.296	96		2463	0.442	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.280	152		7523	0.376	ng/ul	0.00
18) Fluoranthene-d10	19.315	212		8391	0.429	ng/ul	0.00
Target Compounds							
							Qvalue
2) 1,4-Dioxane	3.330	88		1963	0.346	ng/ul	90
5) Naphthalene	10.735	128		14914	0.379	ng/ul	99
7) 2-Methylnaphthalene	12.352	142		8553	0.370	ng/ul	98
8) 1-Methylnaphthalene	12.572	142		8097	0.351	ng/ul	98
10) Acenaphthylene	14.250	152		10092	0.364	ng/ul	97
11) Acenaphthene	14.587	153		8794	0.376	ng/ul	97
12) Fluorene	15.587	166		8974	0.359	ng/ul	99
14) Pentachlorophenol	16.944	266		573	0.288	ng/ul	94
15) Phenanthrene	17.328	178		10873	0.339	ng/ul	97
16) Anthracene	17.426	178		9823	0.364	ng/ul	93
19) Fluoranthene	19.348	202		10600	0.409	ng/ul	98
20) Pyrene	19.705	202		11429	0.411	ng/ul	96
21) Benzo(a)anthracene	21.466	228		6921	0.335	ng/ul	98
22) Chrysene	21.515	228		8408	0.357	ng/ul	99
24) Benzo(b)fluoranthene	23.140	252		6408m	0.316	ng/ul	
25) Benzo(k)fluoranthene	23.187	252		10038m	0.503	ng/ul	
26) Benzo(a)pyrene	23.769	252		6705	0.368	ng/ul#	77
27) Indeno(1,2,3-cd)pyrene	26.350	276		7842	0.309	ng/ul#	94
28) Dibenzo(a,h)anthracene	26.360	278		5872	0.295	ng/ul#	86
29) Benzo(g,h,i)perylene	27.105	276		7356	0.330	ng/ul	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071223\
Data File : BM040829.D
Acq On : 12 Jul 2023 09:32
Operator : MA/JU
Sample : SSTDCCC0.4
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_M
LabSampleId :
SSTDCCC0.4

Manual IntegrationsAPPROVED

Quant Time: Jul 13 00:11:50 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 12 05:37:29 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/13/2023
Supervised By :mohammad ahmed 07/13/2023

