




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071223\
 Data File : BM040841.D
 Acq On : 12 Jul 2023 18:00
 Operator : MA/JU
 Sample : PB153963BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK963

Manual IntegrationsAPPROVED

Quant Time: Jul 13 00:13:22 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 12 05:37:29 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/13/2023
 Supervised By :mohammad ahmed 07/13/2023

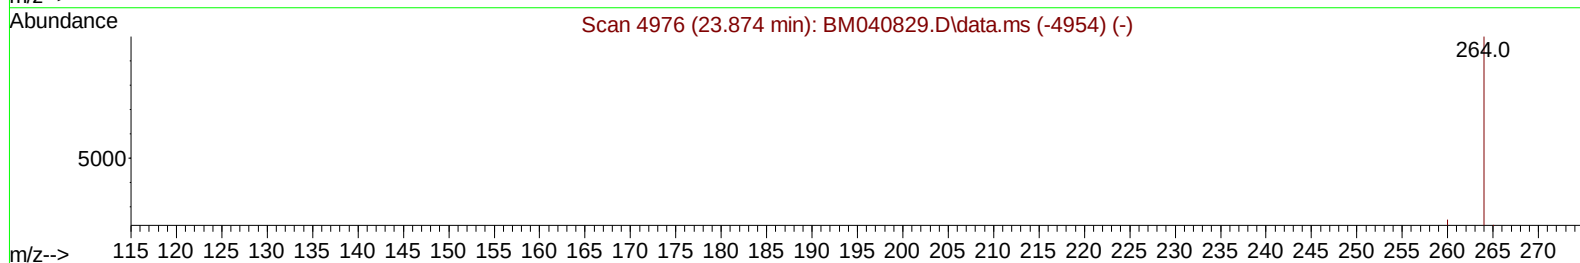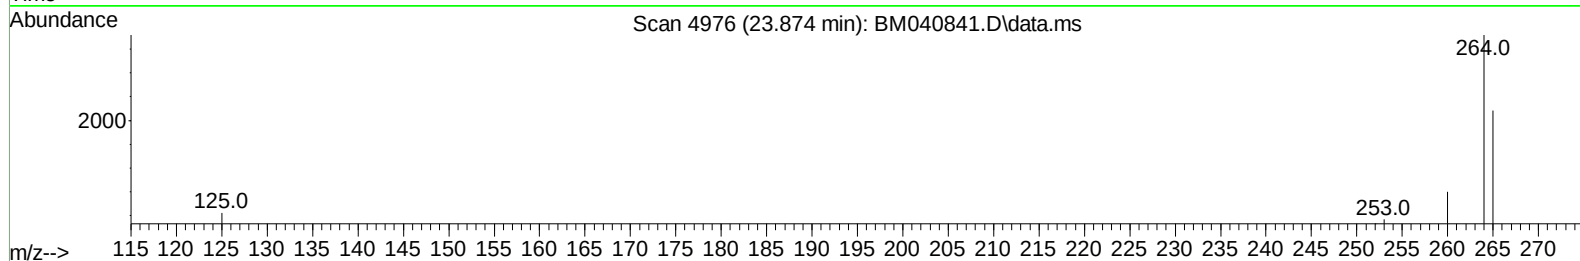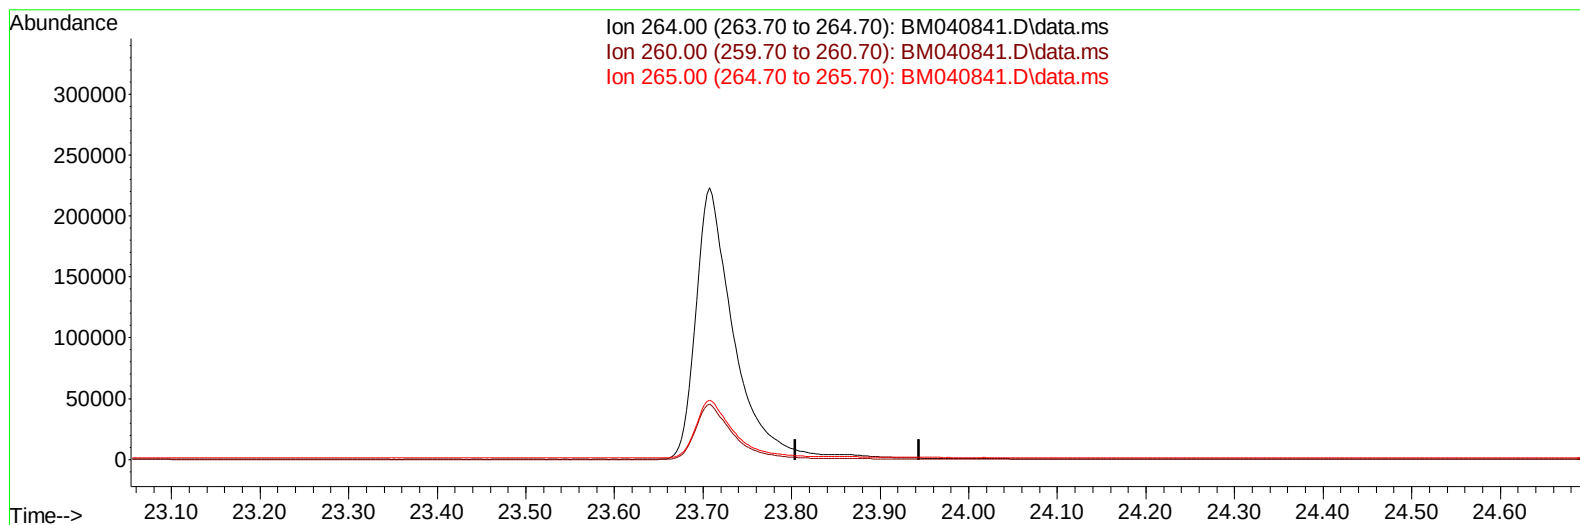

TIC: BM040841.D\data.ms

(23) Perylene-d12 (I)

23.874min (-23.874) 0.00 ng/ul

response 0

Ion	Exp%	Act%
264.00	100.00	0.00
260.00	25.70	0.00#
265.00	79.20	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071223\
 Data File : BM040841.D
 Acq On : 12 Jul 2023 18:00
 Operator : MA/JU
 Sample : PB153963BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK963

Manual IntegrationsAPPROVED

Quant Time: Jul 13 00:13:22 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 12 05:37:29 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/13/2023
 Supervised By :mohammad ahmed 07/13/2023

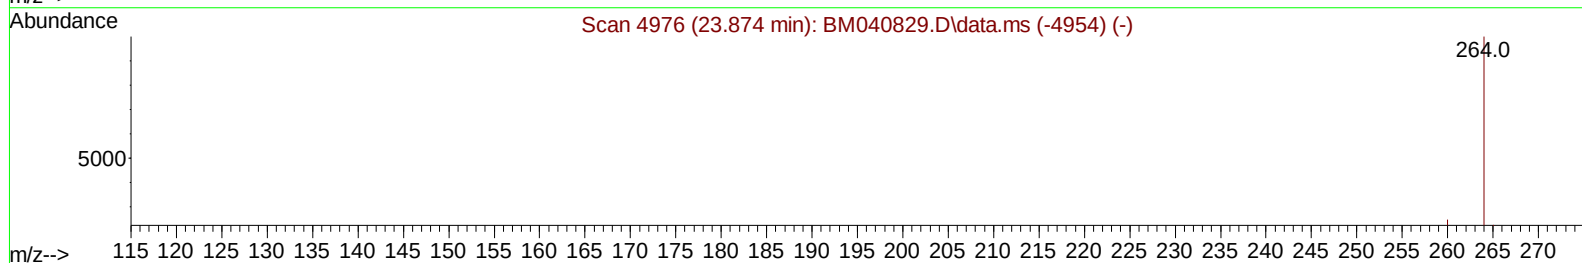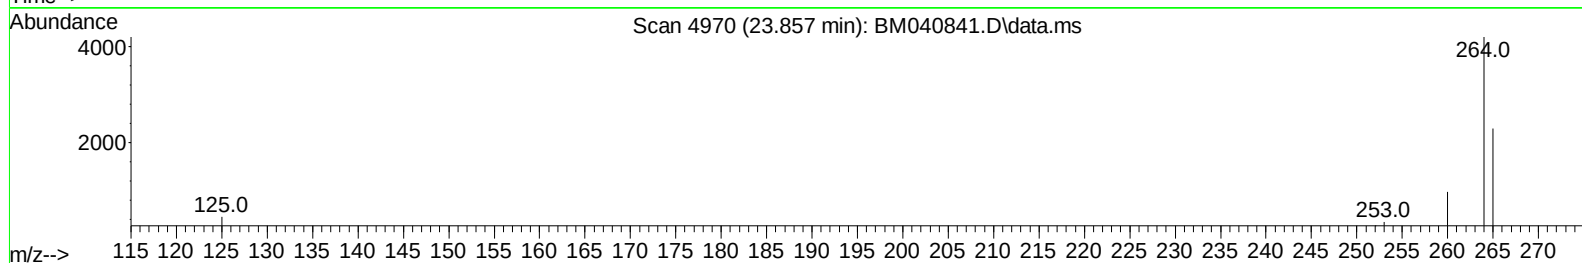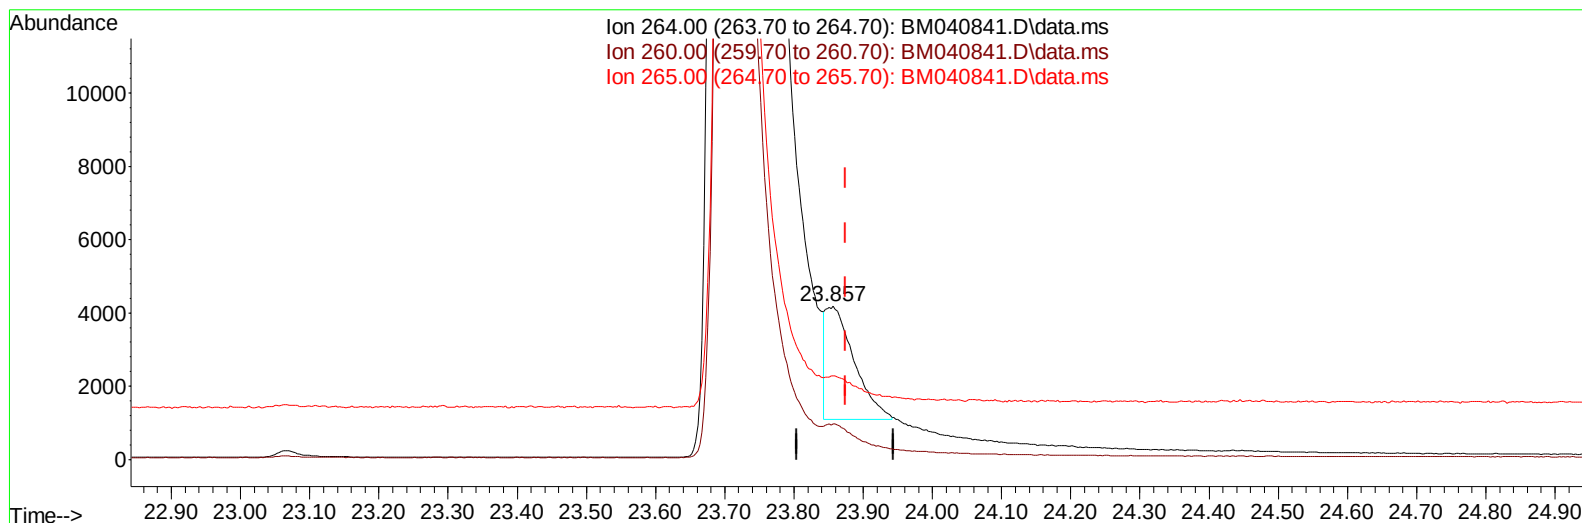

TIC: BM040841.D\data.ms

(23) Perylene-d12 (I)

23.857min (-0.018) 0.40 ng/ul m

response 8897

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	25.70	23.10
265.00	79.20	54.55#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071223\
 Data File : BM040841.D
 Acq On : 12 Jul 2023 18:00
 Operator : MA/JU
 Sample : PB153963BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK963

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/13/2023
 Supervised By :mohammad ahmed 07/13/2023

Quant Time: Jul 13 00:13:22 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 12 05:37:29 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.878	152	2329	0.400	ng/ul	0.00
4) Naphthalene-d8	10.680	136	8974	0.400	ng/ul	#-0.01
9) Acenaphthene-d10	14.523	164	4522	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.274	188	8060	0.400	ng/ul	-0.02
17) Chrysene-d12	21.480	240	6118	0.400	ng/ul	0.00
23) Perylene-d12	23.857	264	8897m	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.292	96	25230	6.896	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.275	152	4892	0.389	ng/ul	-0.01
18) Fluoranthene-d10	19.306	212	6383	0.325	ng/ul	-0.01

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071223\
Data File : BM040841.D
Acq On : 12 Jul 2023 18:00
Operator : MA/JU
Sample : PB153963BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK963

Manual IntegrationsAPPROVED

Quant Time: Jul 13 00:13:22 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 12 05:37:29 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/13/2023
Supervised By :mohammad ahmed 07/13/2023

