

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071223\
 Data File : BM040835.D
 Acq On : 12 Jul 2023 13:33
 Operator : MA/JU
 Sample : 03491-02DL 25X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GWOW-BR-05-167-187-062923DL

Quant Time: Jul 13 00:12:32 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 12 05:37:29 2023
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/13/2023
 Supervised By :mohammad ahmed 07/13/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.887	152	2654	0.400	ng/ul	0.00
4) Naphthalene-d8	10.697	136	9776	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.537	164	4018	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.295	188	6182m	0.400	ng/ul	0.00
17) Chrysene-d12	21.489	240	3987	0.400	ng/ul	# 0.00
23) Perylene-d12	23.877	264	3194	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	0.000	96	0d	0.000	ng/ul	
6) 2-Methylnaphthalene-d10	12.319	152	196	0.014	ng/ul	0.03
18) Fluoranthene-d10	19.329	212	221	0.017	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.330	88	5951	1.402	ng/ul#	81

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071223\
Data File : BM040835.D
Acq On : 12 Jul 2023 13:33
Operator : MA/JU
Sample : 03491-02DL 25X
Misc :
ALS Vial : 8 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
GWOW-BR-05-167-187-062923DL

Quant Time: Jul 13 00:12:32 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 12 05:37:29 2023
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 07/13/2023
Supervised By :mohammad ahmed 07/13/2023

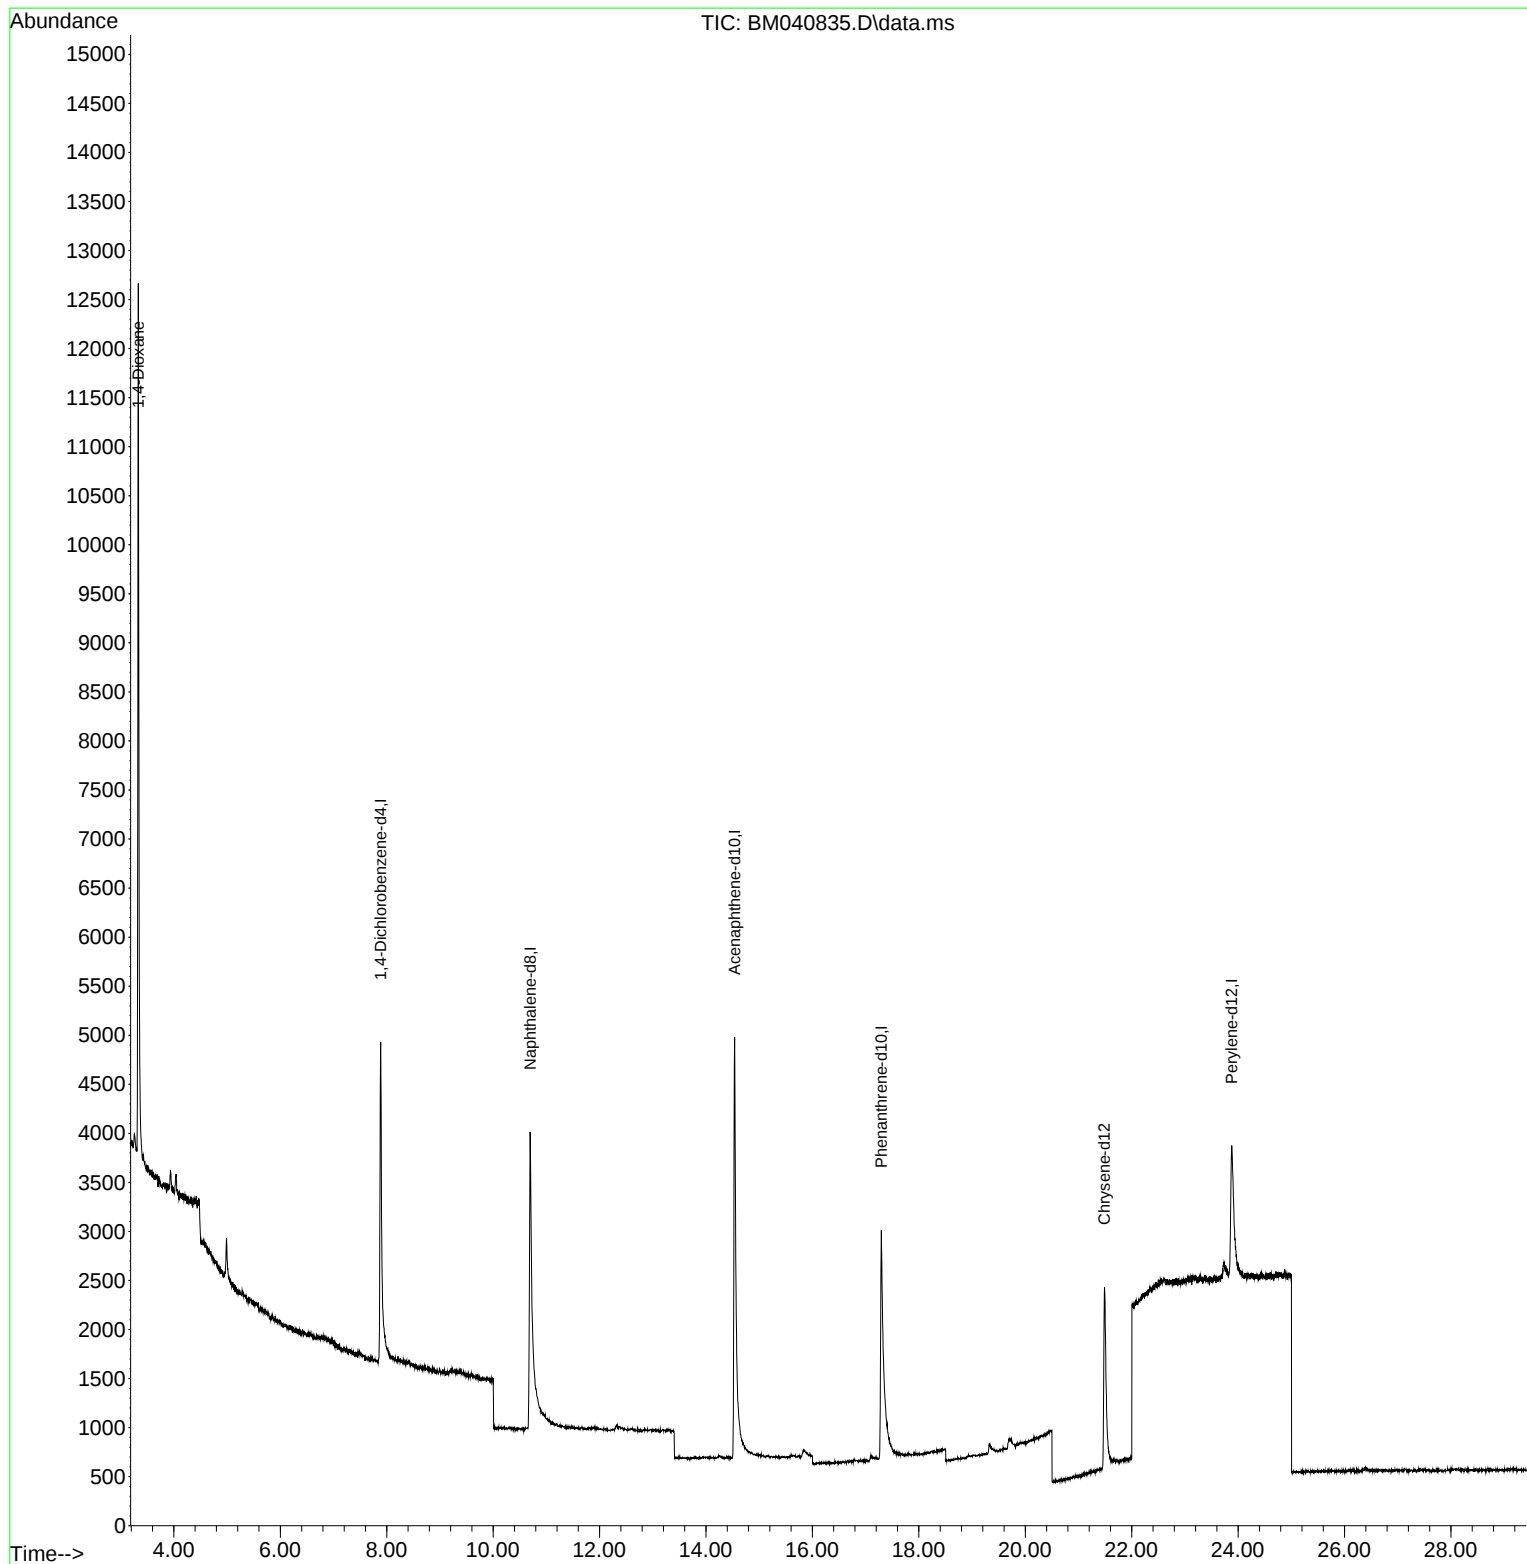

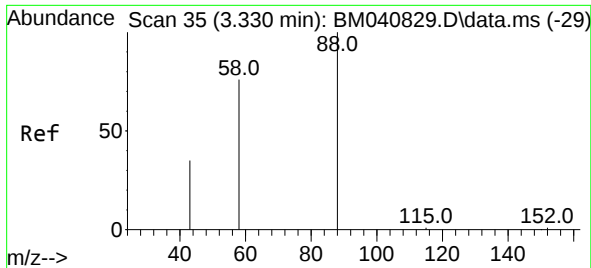

#2
 1,4-Dioxane
 Concen: 1.402 ng/ul
 RT: 3.330 min Scan# 30
 Delta R.T. -0.004 min
 Lab File: BM040835.D
 Acq: 12 Jul 2023 13:33

Instrument :
 BNA_M
 ClientSampleId :
 GWOW-BR-05-167-187-062923DL

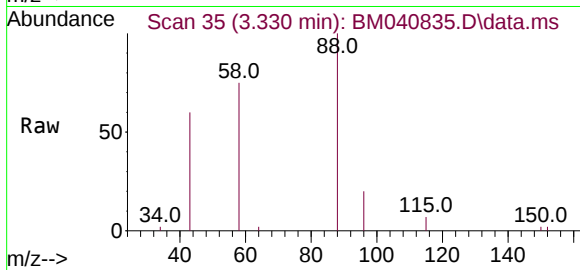

Tgt Ion: 88 Resp: 595
 Ion Ratio Lower Upper
 88 100
 43 60.5 36.1 54.1
 58 74.8 49.8 74.8

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/13/2023
 Supervised By :mohammad ahmed 07/13/2023

