




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071224\
Data File : BM046552.D
Acq On : 12 Jul 2024 19:28
Operator : MA/JU
Sample : PB161866BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK866

Manual IntegrationsAPPROVED

Quant Time: Jul 13 00:35:41 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM071024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 12 05:09:19 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/13/2024
Supervised By :mohammad ahmed 07/16/2024

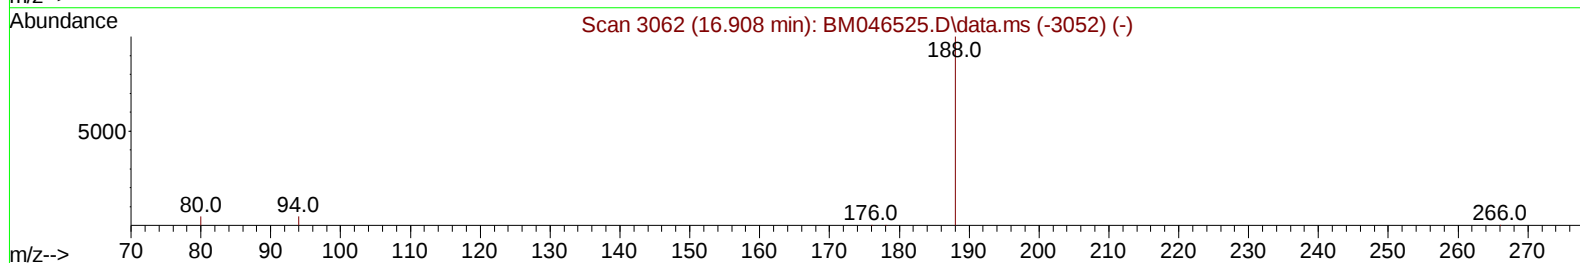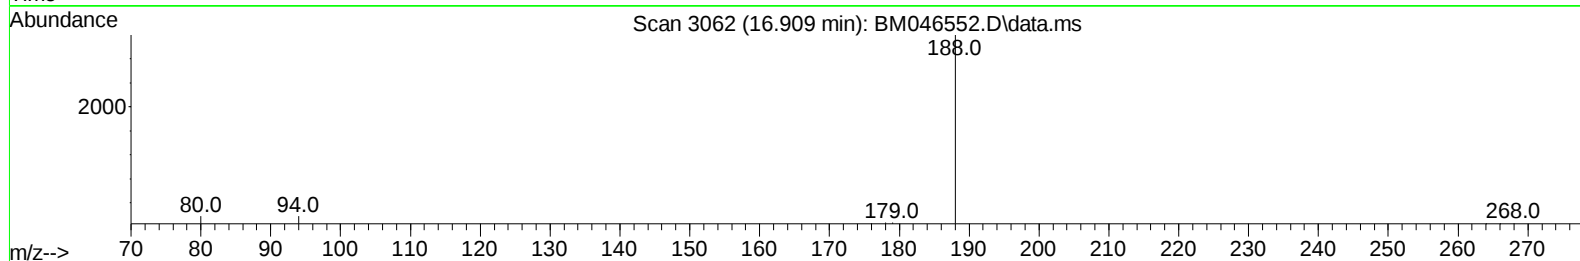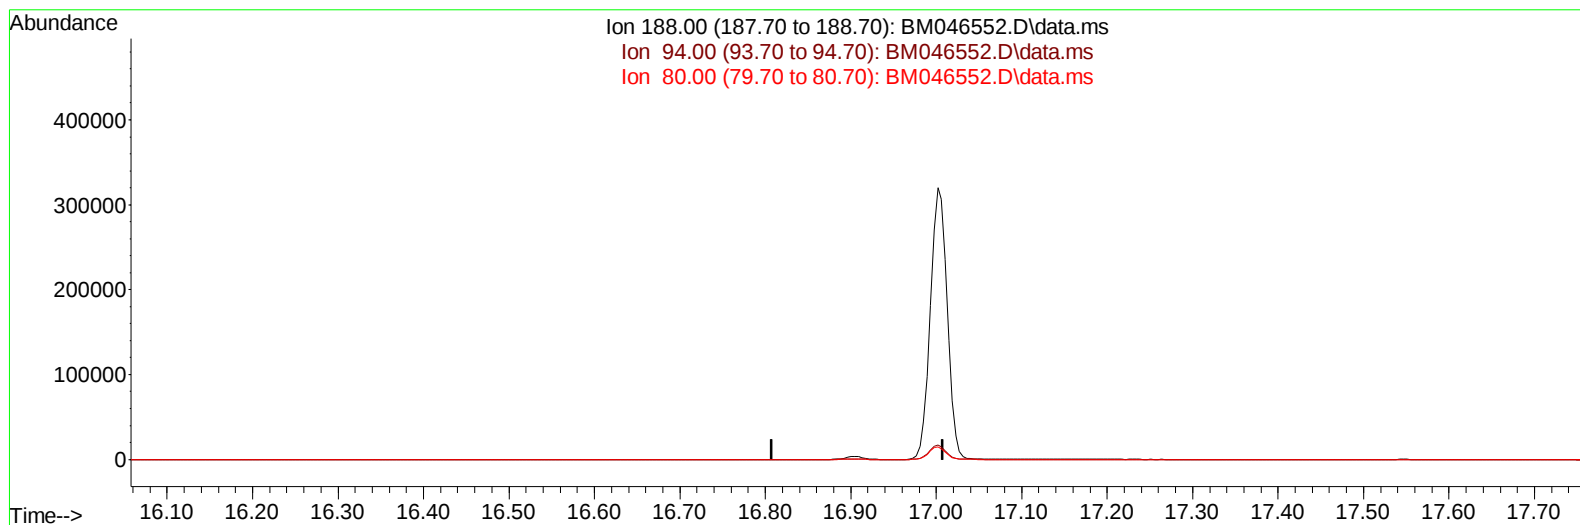

TIC: BM046552.D\data.ms

(13) Phenanthrene-d10 (I)

16.908min (-16.908) 0.00 ng/u1

response 0

Ion	Exp%	Act%
188.00	100.00	0.00
94.00	6.40	0.00#
80.00	6.60	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071224\
Data File : BM046552.D
Acq On : 12 Jul 2024 19:28
Operator : MA/JU
Sample : PB161866BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK866

Manual IntegrationsAPPROVED

Quant Time: Jul 13 00:35:41 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM071024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 12 05:09:19 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/13/2024
Supervised By :mohammad ahmed 07/16/2024

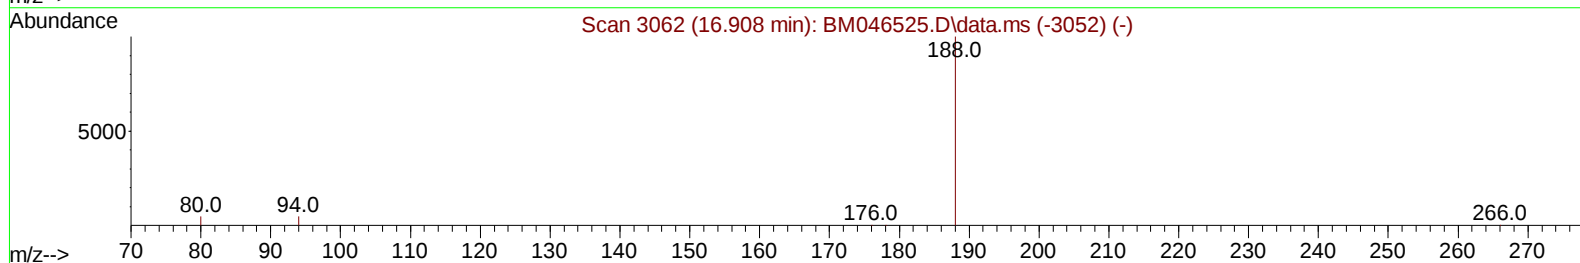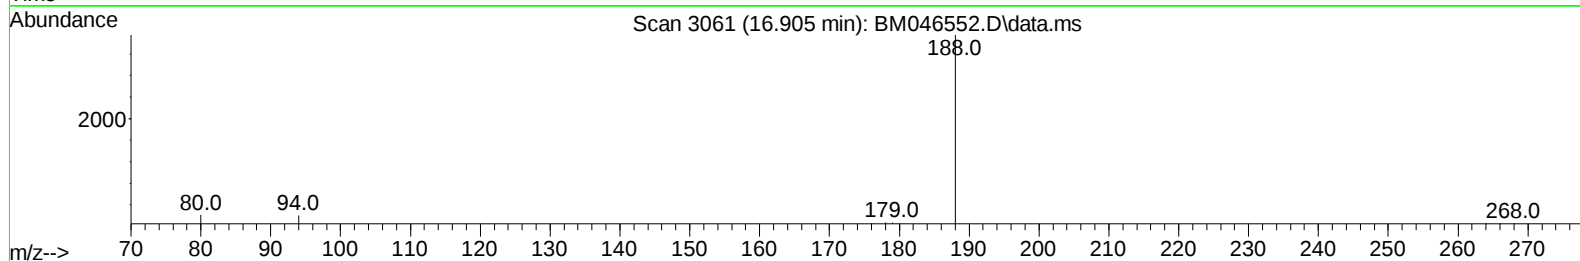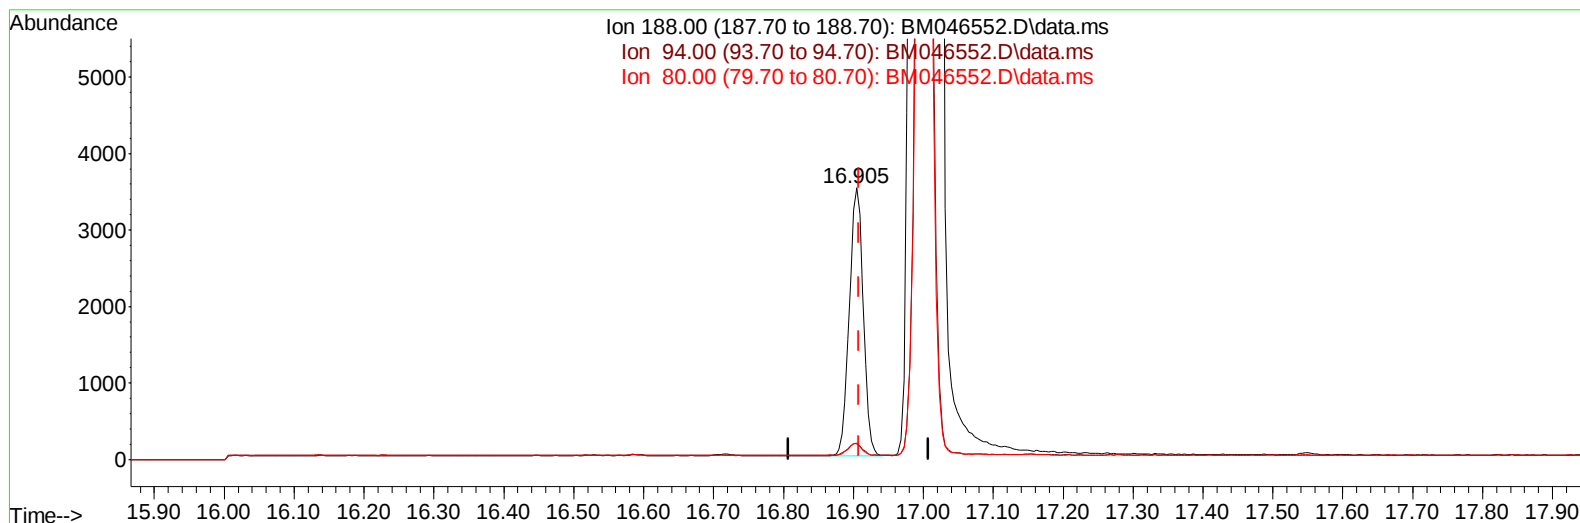

TIC: BM046552.D\data.ms

(13) Phenanthrene-d10 (I)

16.905min (-0.003) 0.40 ng/ul m

response 4839

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	6.40	5.75
80.00	6.60	6.14
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071224\
Data File : BM046552.D
Acq On : 12 Jul 2024 19:28
Operator : MA/JU
Sample : PB161866BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK866

Manual IntegrationsAPPROVED

Quant Time: Jul 13 00:35:41 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM071024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 12 05:09:19 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/13/2024
Supervised By :mohammad ahmed 07/16/2024

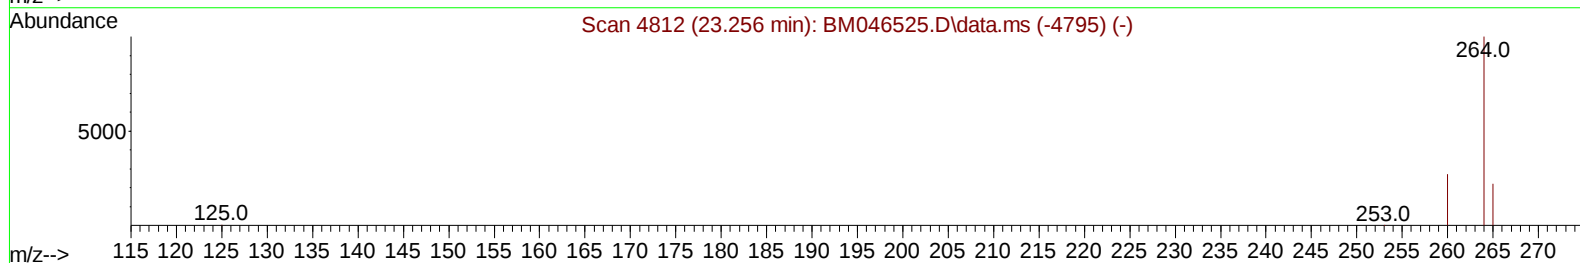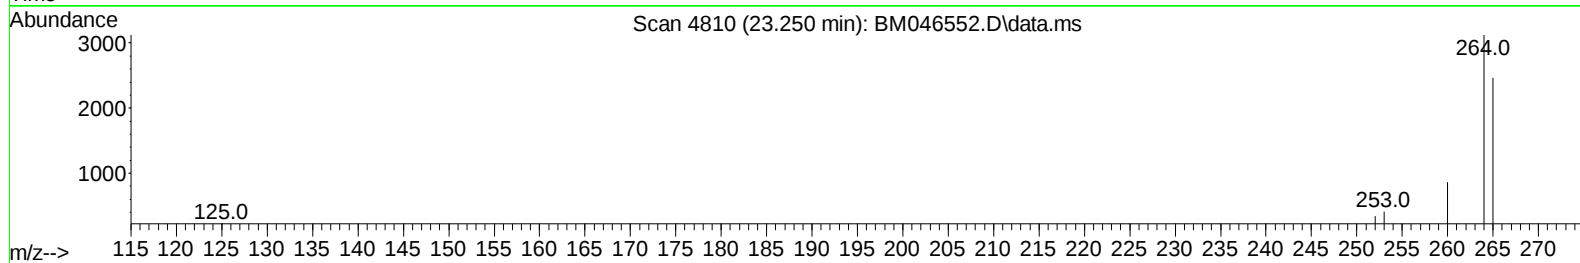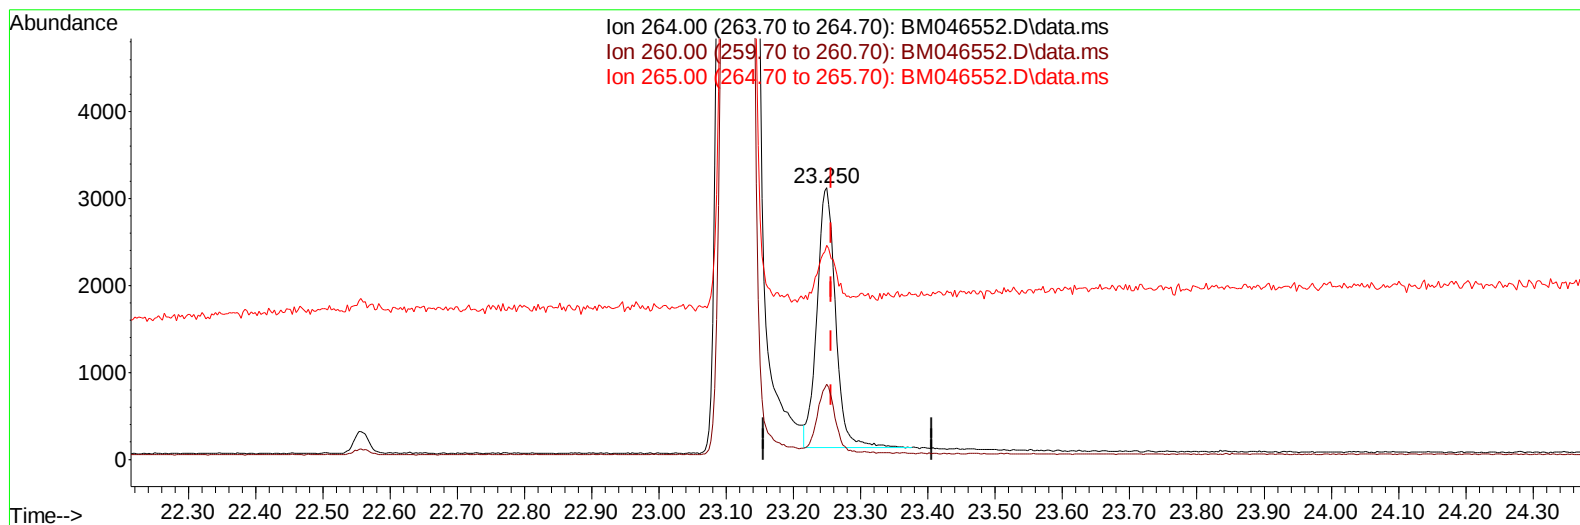

TIC: BM046552.D\data.ms

(23) Perylene-d12 (I)

23.250min (-0.006) 0.40 ng/u1

response 5740

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.80	27.74
265.00	88.90	78.86
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071224\
Data File : BM046552.D
Acq On : 12 Jul 2024 19:28
Operator : MA/JU
Sample : PB161866BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK866

Manual IntegrationsAPPROVED

Quant Time: Jul 13 00:35:41 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM071024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 12 05:09:19 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/13/2024
Supervised By :mohammad ahmed 07/16/2024

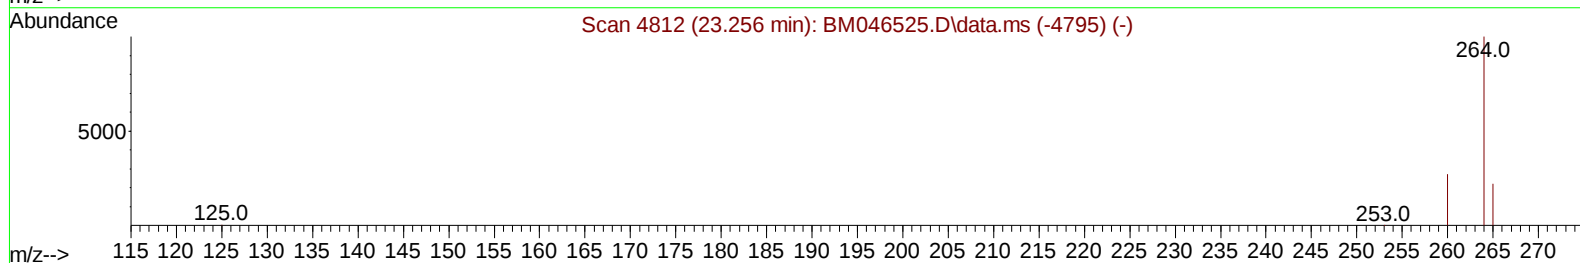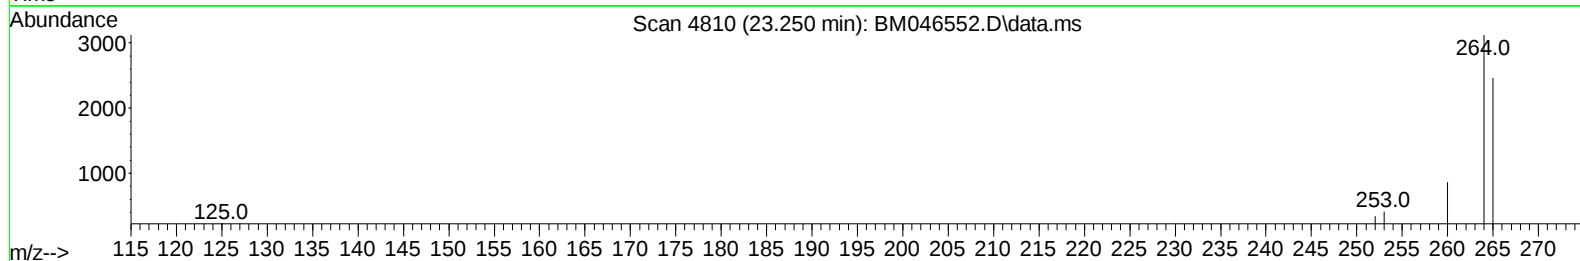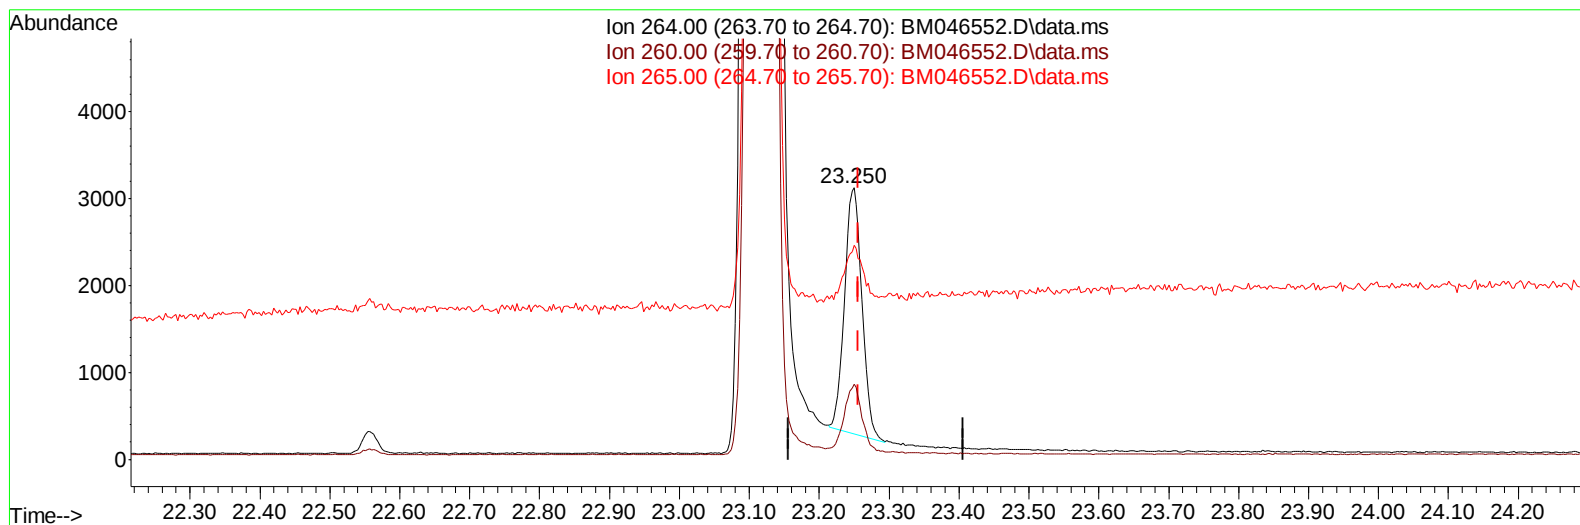

TIC: BM046552.D\data.ms

(23) Perylene-d12 (I)

23.250min (-0.006) 0.40 ng/ul m

response 4880

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.80	27.74
265.00	88.90	78.86
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071224\
 Data File : BM046552.D
 Acq On : 12 Jul 2024 19:28
 Operator : MA/JU
 Sample : PB161866BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK866

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/13/2024
 Supervised By :mohammad ahmed 07/16/2024

Quant Time: Jul 13 00:35:41 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM071024.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 12 05:09:19 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.510	152	1228	0.400	ng/ul	0.00
4) Naphthalene-d8	10.271	136	3092	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.155	164	2264	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.905	188	4839m	0.400	ng/ul	0.00
17) Chrysene-d12	21.108	240	4088	0.400	ng/ul	0.00
23) Perylene-d12	23.250	264	4880m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.117	96	7172	7.108	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.871	152	1956	0.392	ng/ul	0.00
18) Fluoranthene-d10	18.942	212	4861	0.391	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071224\
Data File : BM046552.D
Acq On : 12 Jul 2024 19:28
Operator : MA/JU
Sample : PB161866BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK866

Manual IntegrationsAPPROVED

Quant Time: Jul 13 00:35:41 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM071024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 12 05:09:19 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/13/2024
Supervised By :mohammad ahmed 07/16/2024

