

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071224\
 Data File : BM046589.D
 Acq On : 13 Jul 2024 19:21
 Operator : MA/JU
 Sample : P3084-03
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E1GE2

Quant Time: Jul 15 09:57:40 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM071024.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 15 08:57:27 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.510	152	3852	0.400	ng/ul	0.00
4) Naphthalene-d8	10.271	136	10403	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	0.000	164	0	0.000	ng/ul	-14.15
13) Phenanthrene-d10	0.000	188	0	0.000	ng/ul	-16.90
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.11
23) Perylene-d12	0.000	264	0	0.000	ng/ul	-23.24
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.117	96	10398	3.285	ng/ul	0.00
6) 2-Methylnaphthalene-d10	0.000	152	0	0.000	ng/ul	
18) Fluoranthene-d10	0.000	212	0	0.000	ng/ul	
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.143	88	71	0.021	ng/ul#	16
5) Naphthalene	10.315	128	5065	0.191	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071224\
Data File : BM046589.D
Acq On : 13 Jul 2024 19:21
Operator : MA/JU
Sample : P3084-03
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E1GE2

Quant Time: Jul 15 09:57:40 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM071024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 15 08:57:27 2024
Response via : Initial Calibration




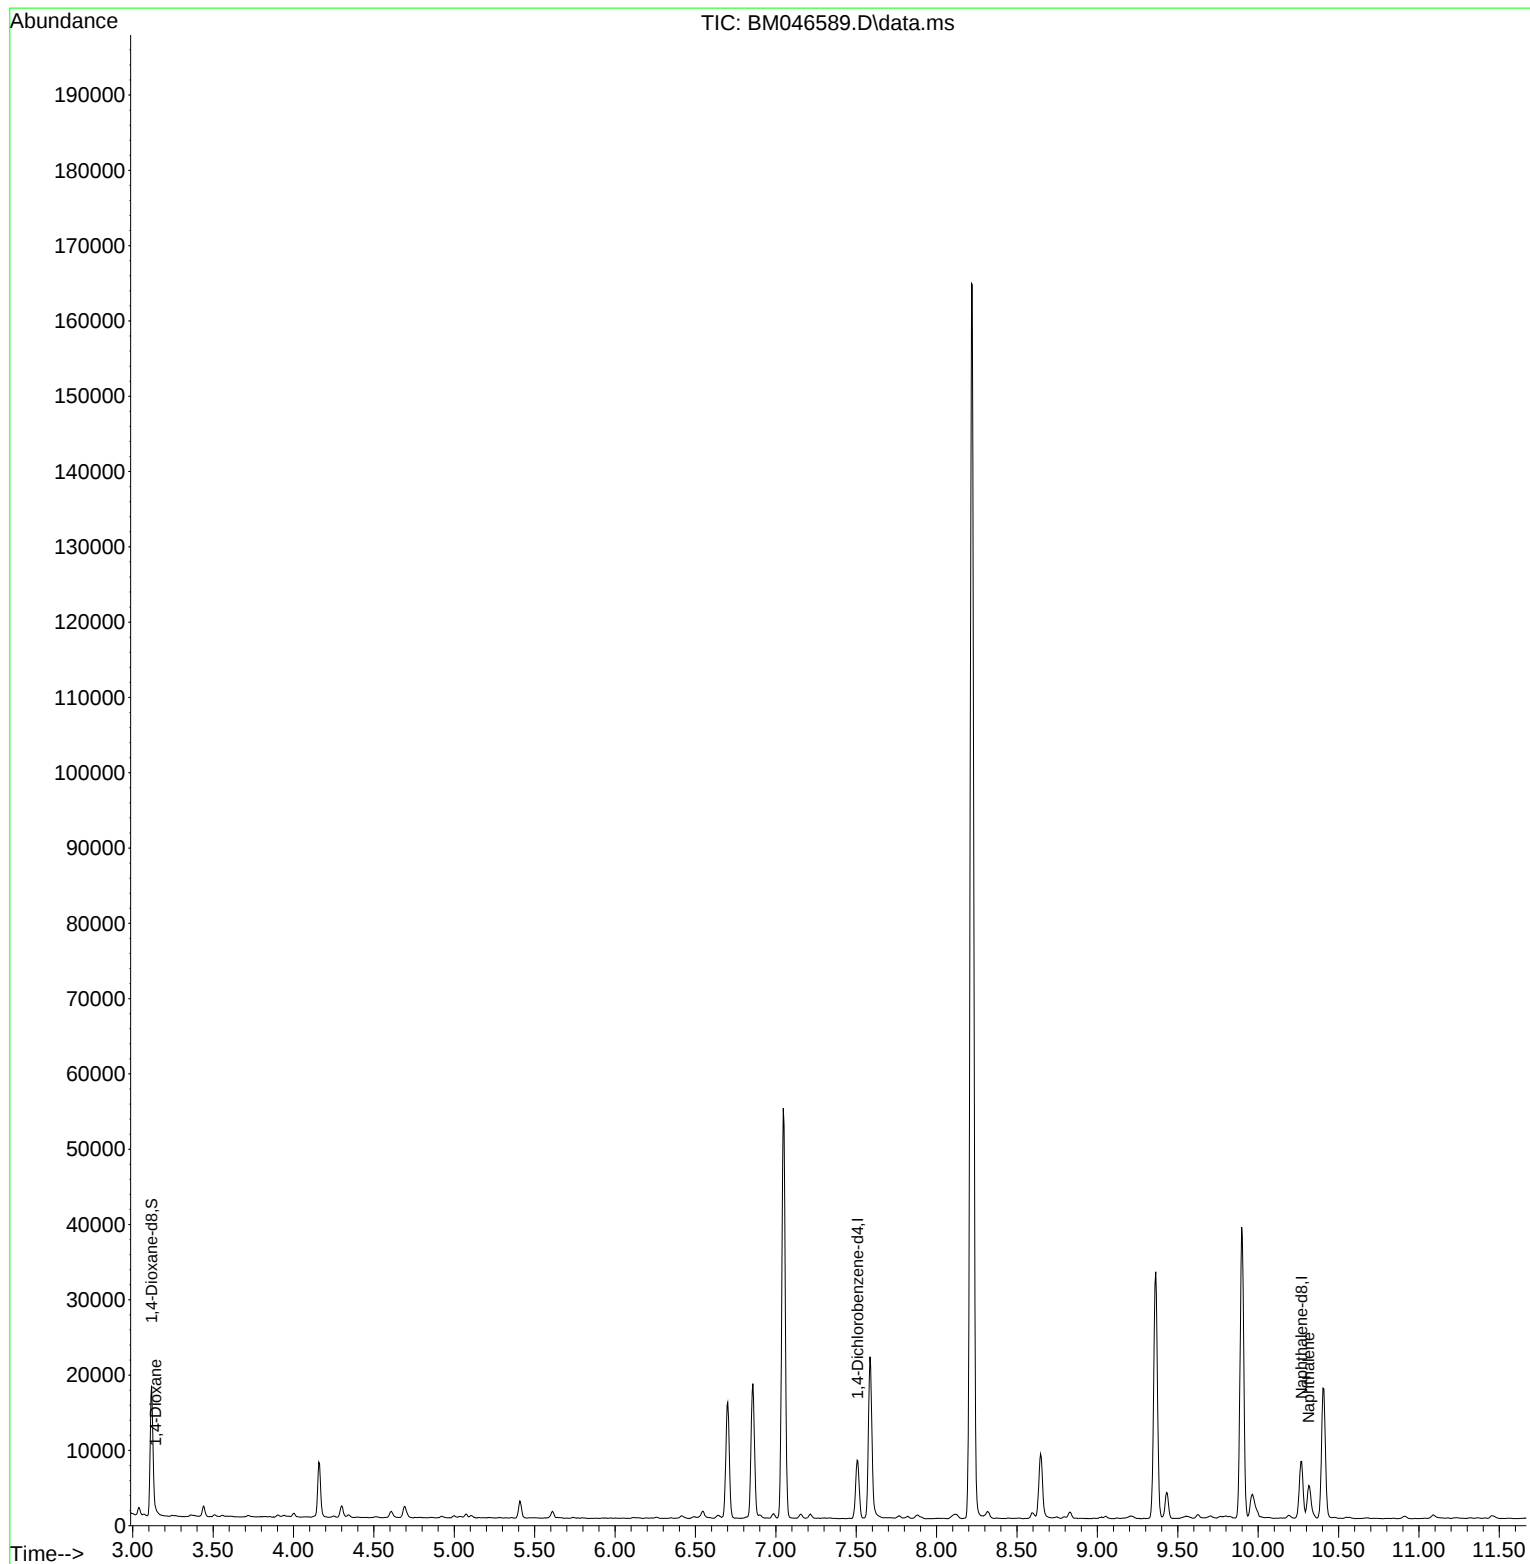


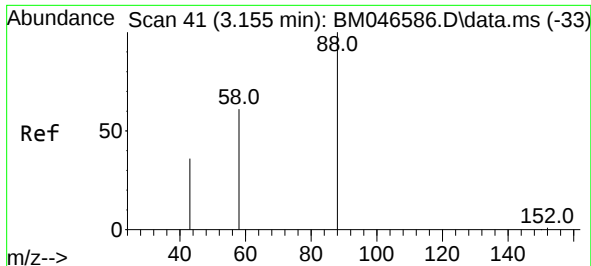

#2
1,4-Dioxane
Concen: 0.021 ng/ul
RT: 3.143 min Scan# 31
Delta R.T. -0.009 min
Lab File: BM046589.D
Acq: 13 Jul 2024 19:21

Instrument :
BNA_M
ClientSampleId :
E1GE2

Tgt Ion: 88 Resp: 71
Ion Ratio Lower Upper
88 100
43 201.4 70.2 105.4#
58 38.5 48.2 72.4#

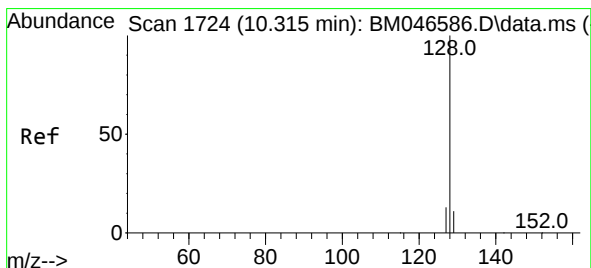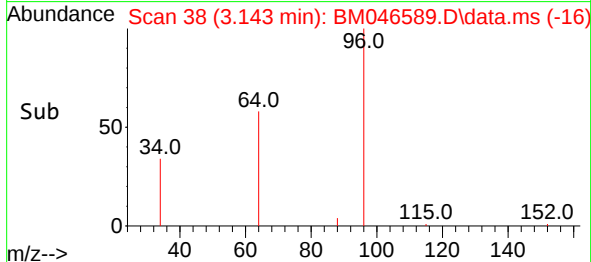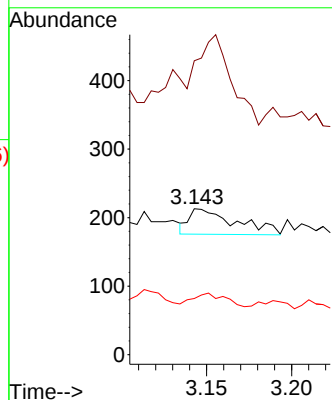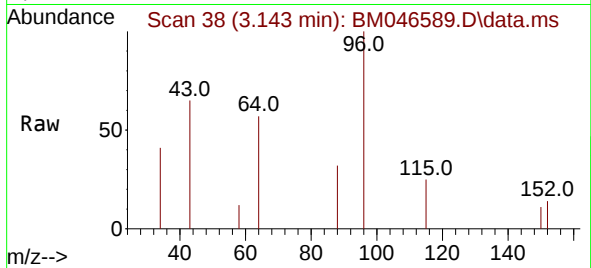

#5
Naphthalene
Concen: 0.191 ng/ul
RT: 10.315 min Scan# 1724
Delta R.T. -0.000 min
Lab File: BM046589.D
Acq: 13 Jul 2024 19:21

Tgt Ion: 128 Resp: 5065
Ion Ratio Lower Upper
128 100
129 13.4 10.3 15.5
127 13.7 12.2 18.4

