


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM071321\
Data File : BM030930.D
Acq On : 13 Jul 2021 14:45
Operator : CG/JU
Sample : PB137523BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK523

Quant Time: Jul 13 15:16:56 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM071321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 13 14:01:01 2021
Response via : Initial Calibration

Manual Integrations
APPROVED

mohammad
7/14/2021 12:16:24 PM

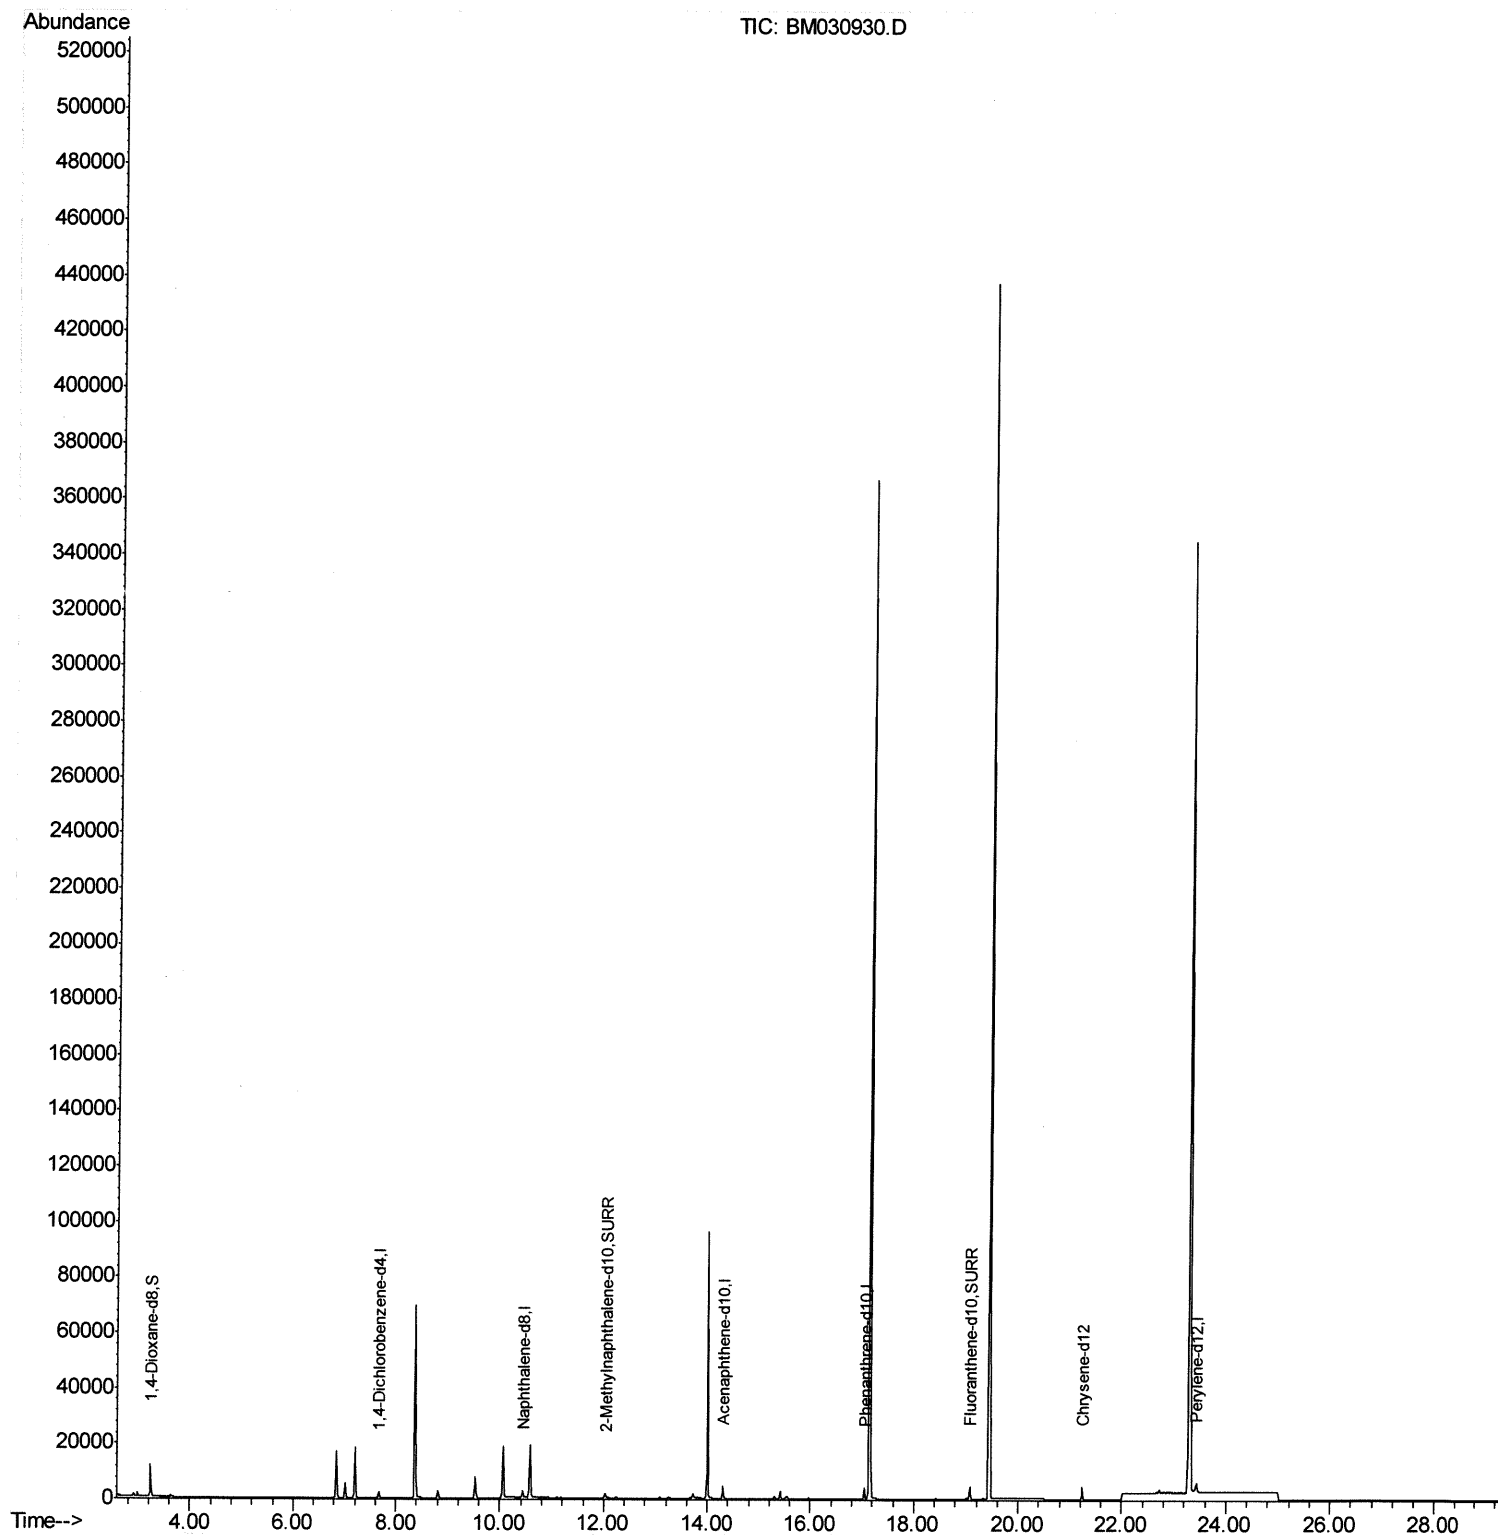




Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM071321\
 Data File : BM030930.D
 Acq On : 13 Jul 2021 14:45
 Operator : CG/JU
 Sample : PB137523BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK523

Manual Integrations
 APPROVED

mohammad
 7/14/2021 12:16:24 PM

Quant Time: Jul 13 15:15:46 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM071321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 13 14:01:01 2021
 Response via : Initial Calibration

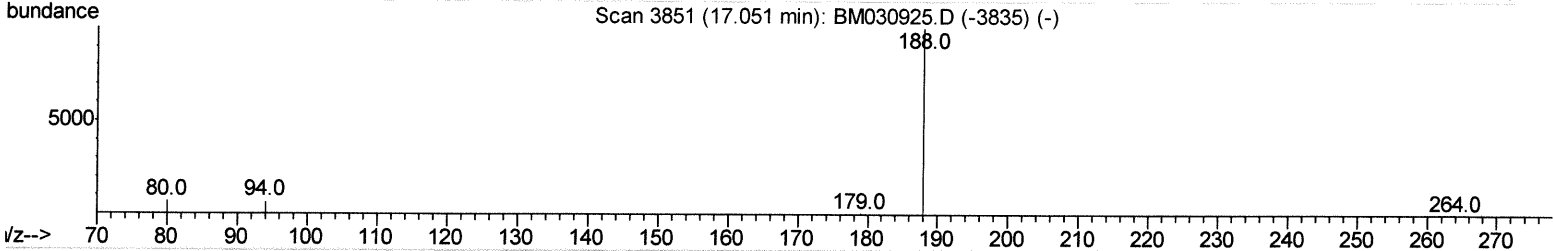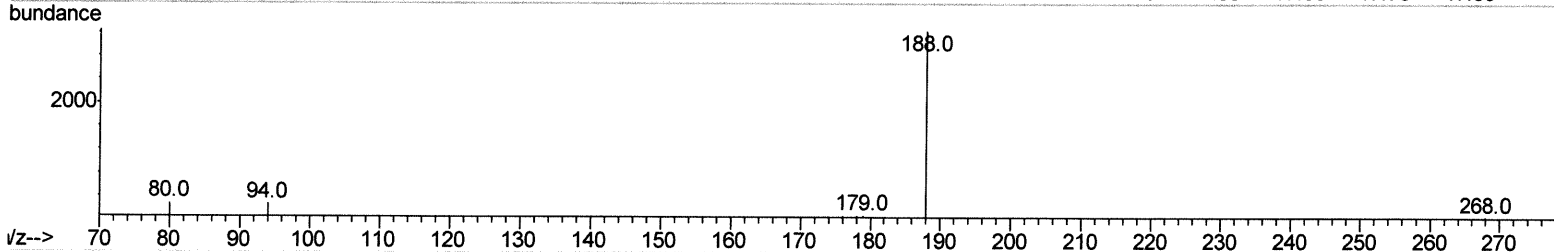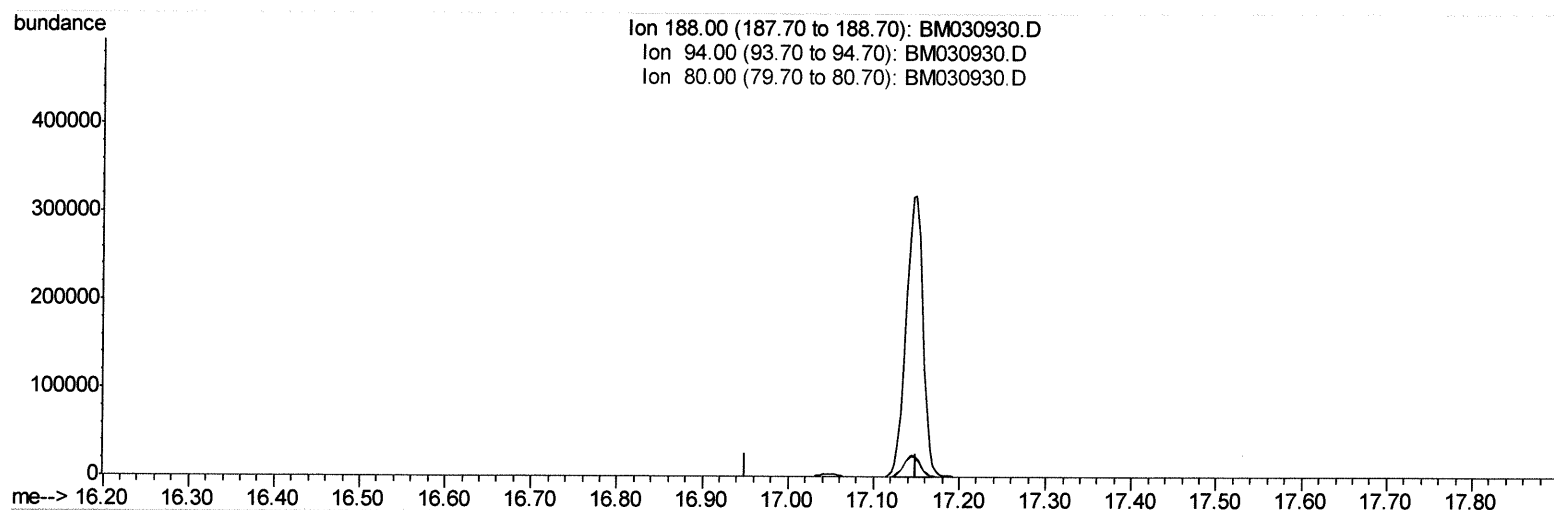

TIC: BM030930.D

(13) Phenanthrene-d10 (I)

17.051min (-17.051) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	8.70	0.00#
80.00	8.50	0.00#
0.00	0.00	0.00




Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM071321\
 Data File : BM030930.D
 Acq On : 13 Jul 2021 14:45
 Operator : CG/JU
 Sample : PB137523BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK523

Manual Integrations
 APPROVED

mohammad
 7/14/2021 12:16:24 PM

Quant Time: Jul 13 15:15:46 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM071321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 13 14:01:01 2021
 Response via : Initial Calibration

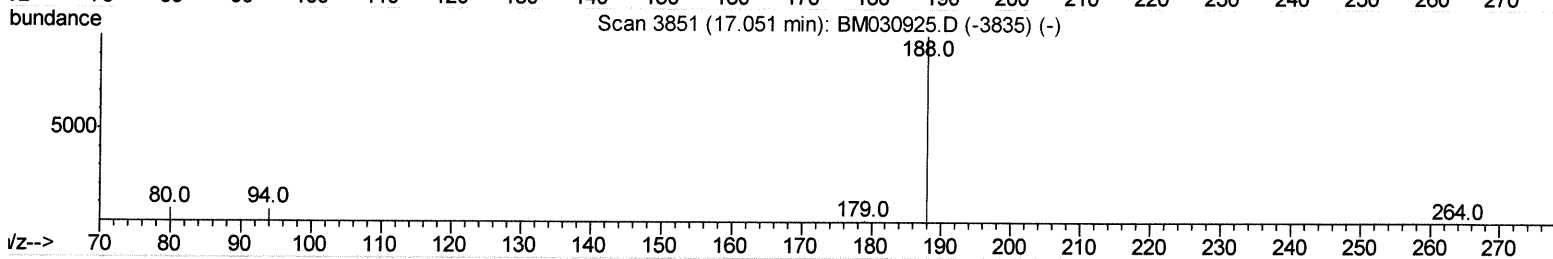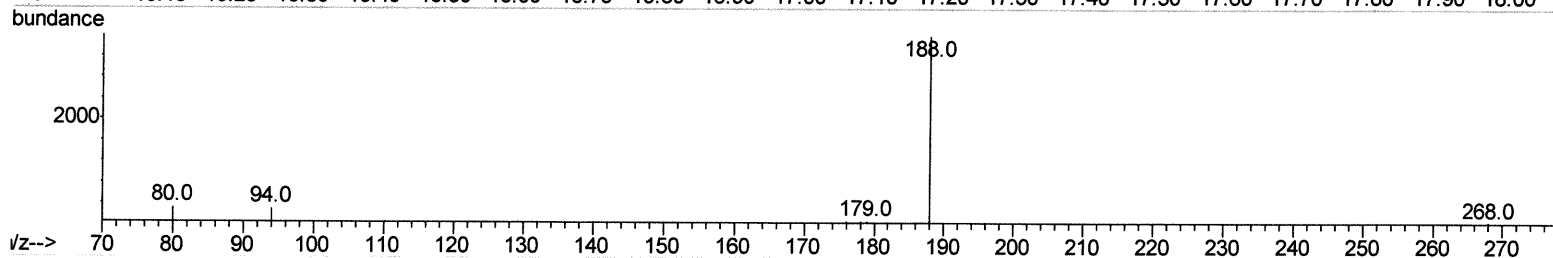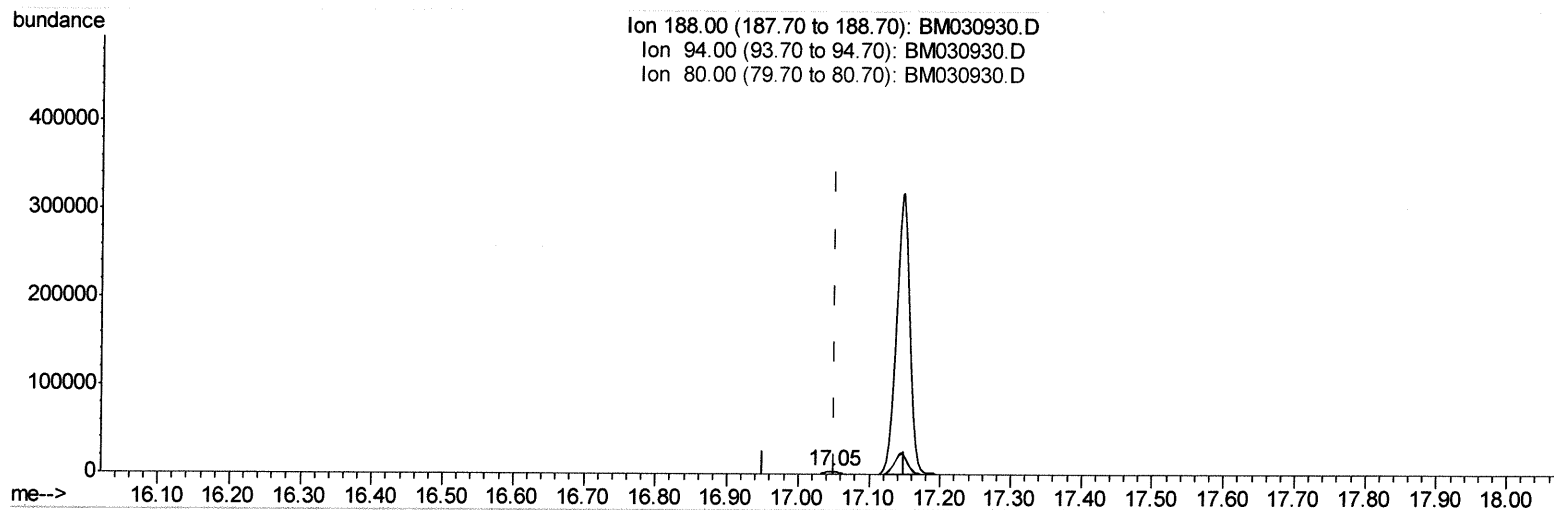

TIC: BM030930.D

(13) Phenanthrene-d10 (I)

17.048min (-0.003) 0.40ng/ul m

response 4894

Ion	Exp%	Act%
188.00	100	100
94.00	8.70	8.30
80.00	8.50	8.97
0.00	0.00	0.00

JU 7/15/21

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM071321\
 Data File : BM030930.D
 Acq On : 13 Jul 2021 14:45
 Operator : CG/JU
 Sample : PB137523BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK523

Manual Integrations
 APPROVED

mohammad
 7/14/2021 12:16:24 PM

Quant Time: Jul 13 15:16:56 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM071321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 13 14:01:01 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.67	152	944	0.40	ng/ul	0.00
4) Naphthalene-d8	10.44	136	3308	0.40	ng/ul	0.00
9) Acenaphthene-d10	14.30	164	2363	0.40	ng/ul	0.00
13) Phenanthrene-d10	17.05	188	4894m	0.40	ng/ul	0.00
17) Chrysene-d12	21.24	240	3863	0.40	ng/ul	0.00
23) Perylene-d12	23.43	264	4313	0.40	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.24	96	6552	6.75	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.03	152	2092	0.36	ng/ul	0.00
18) Fluoranthene-d10	19.08	212	5012	0.39	ng/ul	0.00

Target Compounds

Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed