


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM071321\
Data File : BM030937.D
Acq On : 13 Jul 2021 19:03
Operator : CG/JU
Sample : PB137523BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK523

Manual Integrations
APPROVED

mohammad
7/14/2021 12:16:38 PM

Quant Time: Jul 14 04:02:56 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM071321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 13 14:01:01 2021
Response via : Initial Calibration

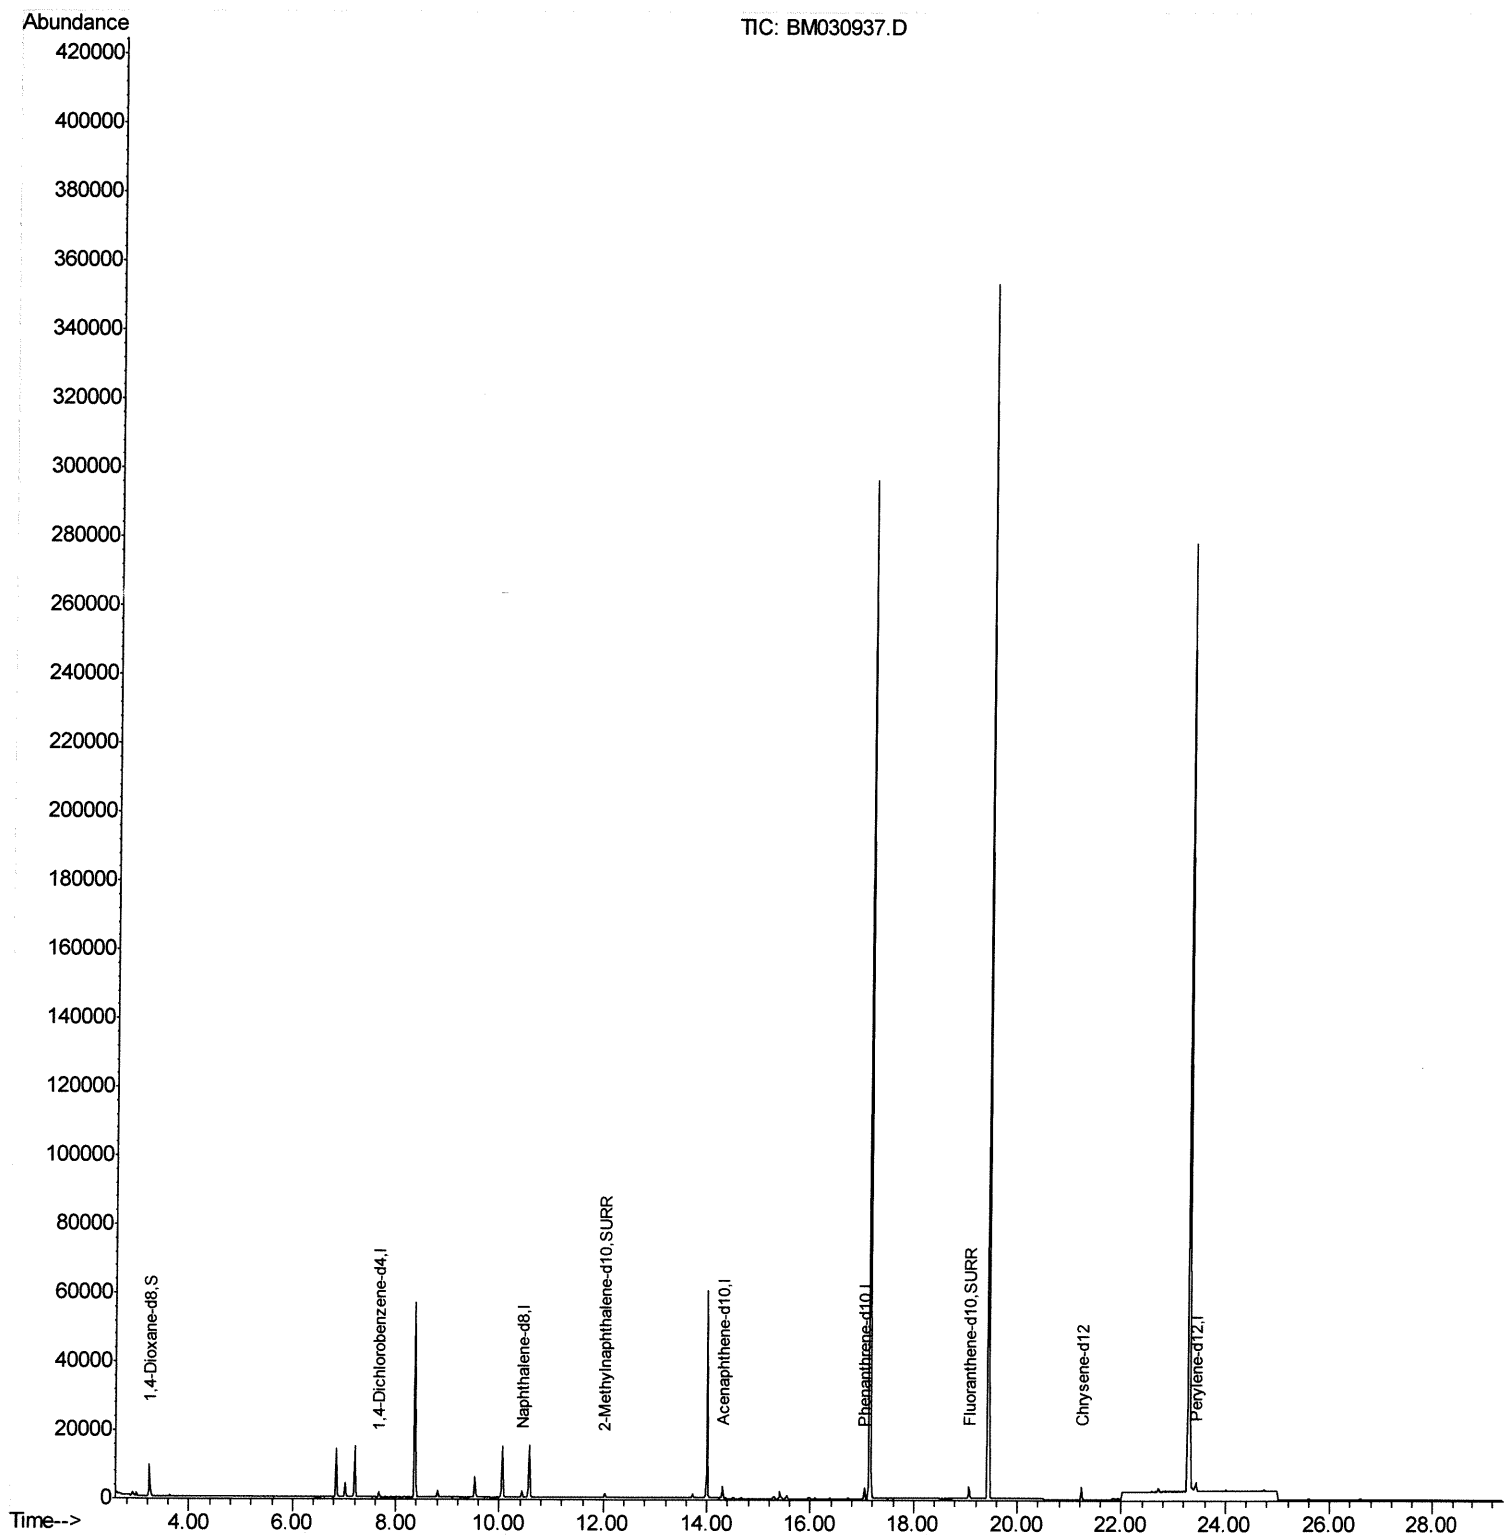


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM071321\
Data File : BM030937.D
Acq On : 13 Jul 2021 19:03
Operator : CG/JU
Sample : PB137523BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK523

Manual Integrations
APPROVED

mohammad
7/14/2021 12:16:38 PM

Quant Time: Jul 14 04:01:40 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM071321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 13 14:01:01 2021
Response via : Initial Calibration

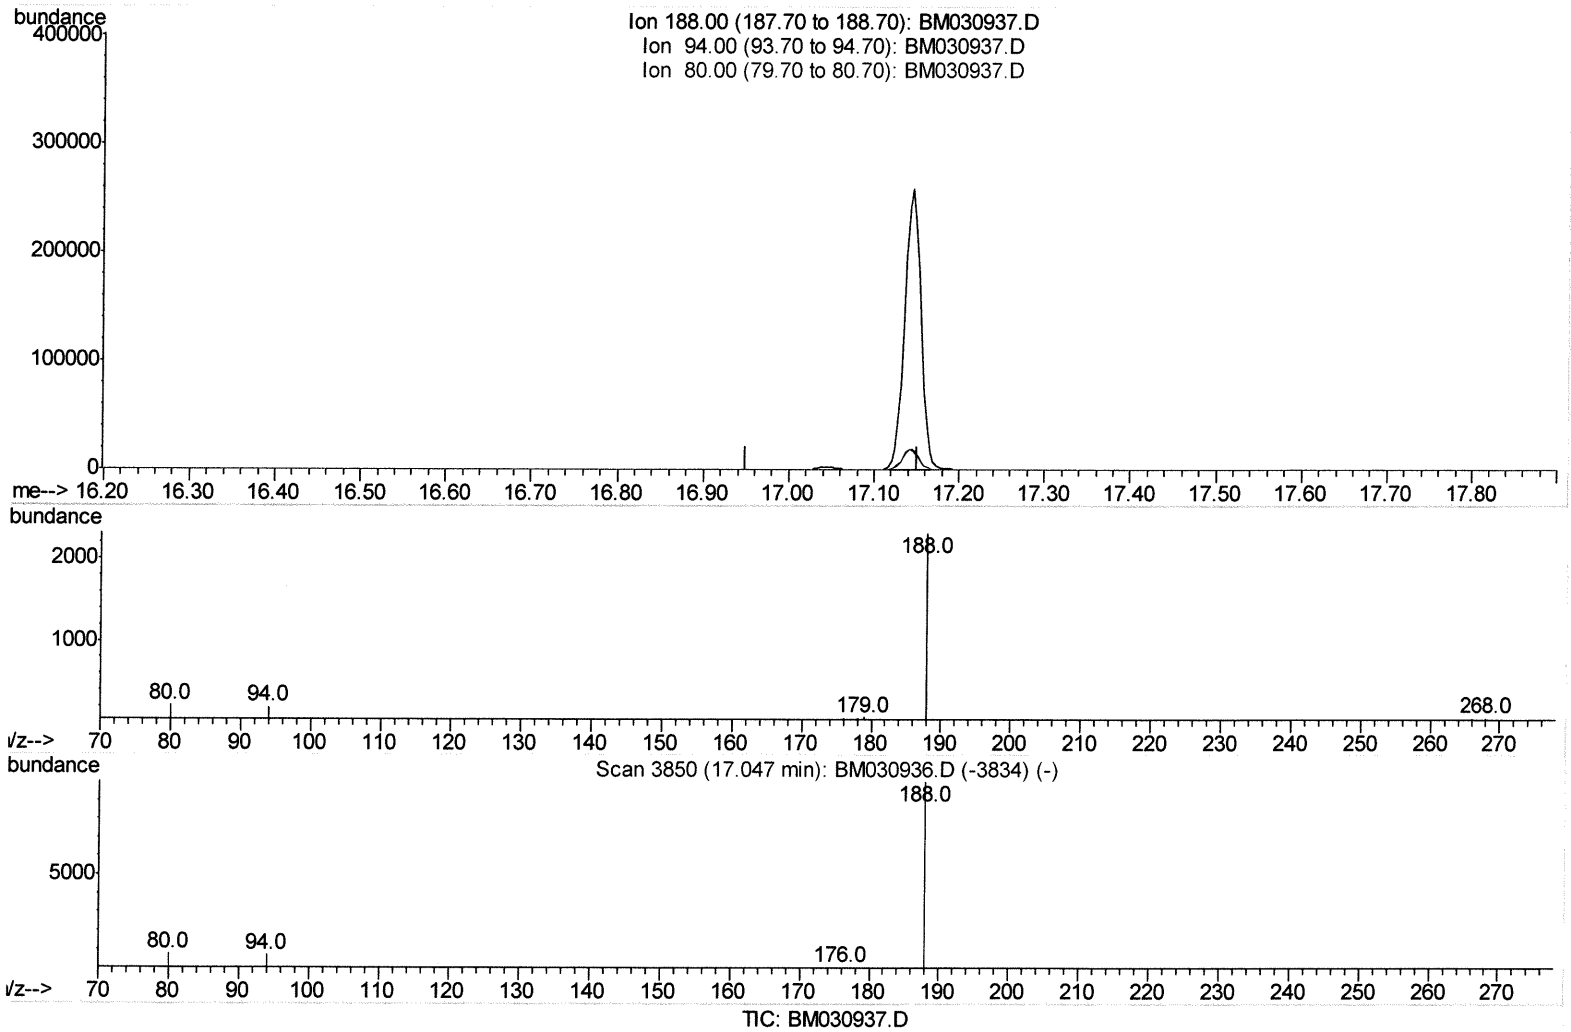

(13) Phenanthrene-d10 (I)

17.051min (-17.051) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	8.70	0.00#
80.00	8.50	0.00#
0.00	0.00	0.00


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM071321\
 Data File : BM030937.D
 Acq On : 13 Jul 2021 19:03
 Operator : CG/JU
 Sample : PB137523BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK523

Manual Integrations
 APPROVED

mohammad
 7/14/2021 12:16:38 PM

Quant Time: Jul 14 04:01:40 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM071321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 13 14:01:01 2021
 Response via : Initial Calibration

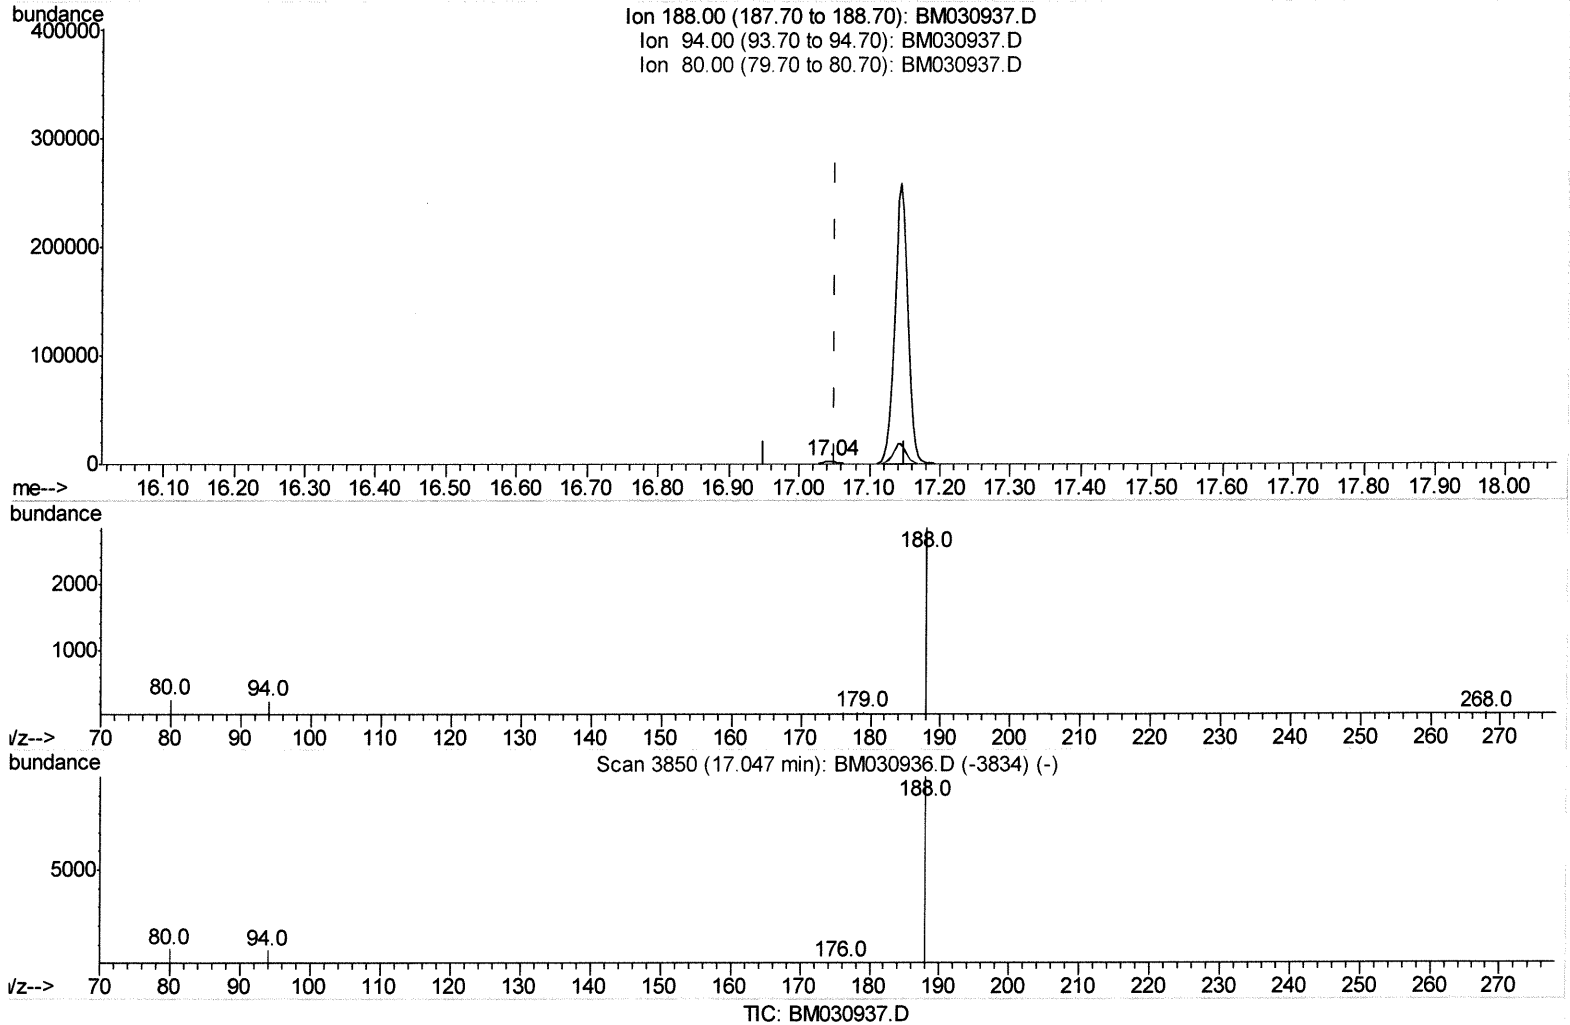

(13) Phenanthrene-d10 (I)

17.044min (-0.007) 0.40ng/ul m

response 3905

Ion	Exp%	Act%
188.00	100	100
94.00	8.70	8.53
80.00	8.50	9.20
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM071321\
 Data File : BM030937.D
 Acq On : 13 Jul 2021 19:03
 Operator : CG/JU
 Sample : PB137523BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK523

Manual Integrations
 APPROVED

mohammad
 7/14/2021 12:16:38 PM

Quant Time: Jul 14 04:02:56 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM071321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 13 14:01:01 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.67	152	794	0.40	ng/ul	0.00
4) Naphthalene-d8	10.44	136	2695	0.40	ng/ul	0.00
9) Acenaphthene-d10	14.30	164	1933	0.40	ng/ul	0.00
13) Phenanthrene-d10	17.04	188	3905m	0.40	ng/ul	0.00
17) Chrysene-d12	21.23	240	3126	0.40	ng/ul	0.00
23) Perylene-d12	23.43	264	3297	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.24	96	5478	6.71	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.03	152	1674	0.36	ng/ul	0.00
18) Fluoranthene-d10	19.07	212	4035	0.38	ng/ul	0.00

Target Compounds	Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

7/14/21