

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM071321\  
 Data File : BM030945.D  
 Acq On : 13 Jul 2021 23:57  
 Operator : CG/JU  
 Sample : M2878-13  
 Misc :  
 ALS Vial : 17 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 BGE04

Quant Time: Jul 14 04:21:34 2021  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SFAM-EPA-SIM-BM071321.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Wed Jul 14 04:01:52 2021  
 Response via : Initial Calibration


| Compound                    | R.T.   | QIon | Response | Conc  | Units  | Dev(Min)  |
|-----------------------------|--------|------|----------|-------|--------|-----------|
| -----                       |        |      |          |       |        |           |
| Internal Standards          |        |      |          |       |        |           |
| 1) 1,4-Dichlorobenzene-d4   | 7.666  | 152  | 1077     | 0.400 | ng/ul  | 0.00      |
| 4) Naphthalene-d8           | 10.433 | 136  | 3744     | 0.400 | ng/ul  | 0.00      |
| 9) Acenaphthene-d10         | 14.296 | 164  | 2480     | 0.400 | ng/ul  | 0.00      |
| 13) Phenanthrene-d10        | 17.044 | 188  | 5216     | 0.400 | ng/ul  | 0.00      |
| 17) Chrysene-d12            | 21.231 | 240  | 4162     | 0.400 | ng/ul  | 0.00      |
| 23) Perylene-d12            | 23.423 | 264  | 4328     | 0.400 | ng/ul  | 0.00      |
| System Monitoring Compounds |        |      |          |       |        |           |
| 3) 1,4-Dioxane-d8           | 3.237  | 96   | 2214     | 1.999 | ng/ul  | 0.00      |
| 6) 2-Methylnaphthalene-d10  | 12.029 | 152  | 1214     | 0.186 | ng/ul  | 0.00      |
| 18) Fluoranthene-d10        | 19.073 | 212  | 2854     | 0.204 | ng/ul  | 0.00      |
| Target Compounds            |        |      |          |       |        |           |
| 19) Fluoranthene            | 19.104 | 202  | 386      | 0.021 | ng/ul# | Qvalue 58 |
| -----                       |        |      |          |       |        |           |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM071321\  
Data File : BM030945.D  
Acq On : 13 Jul 2021 23:57  
Operator : CG/JU  
Sample : M2878-13  
Misc :  
ALS Vial : 17 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
BGE04

Quant Time: Jul 14 04:21:34 2021  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SFAM-EPA-SIM-BM071321.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Jul 14 04:01:52 2021  
Response via : Initial Calibration

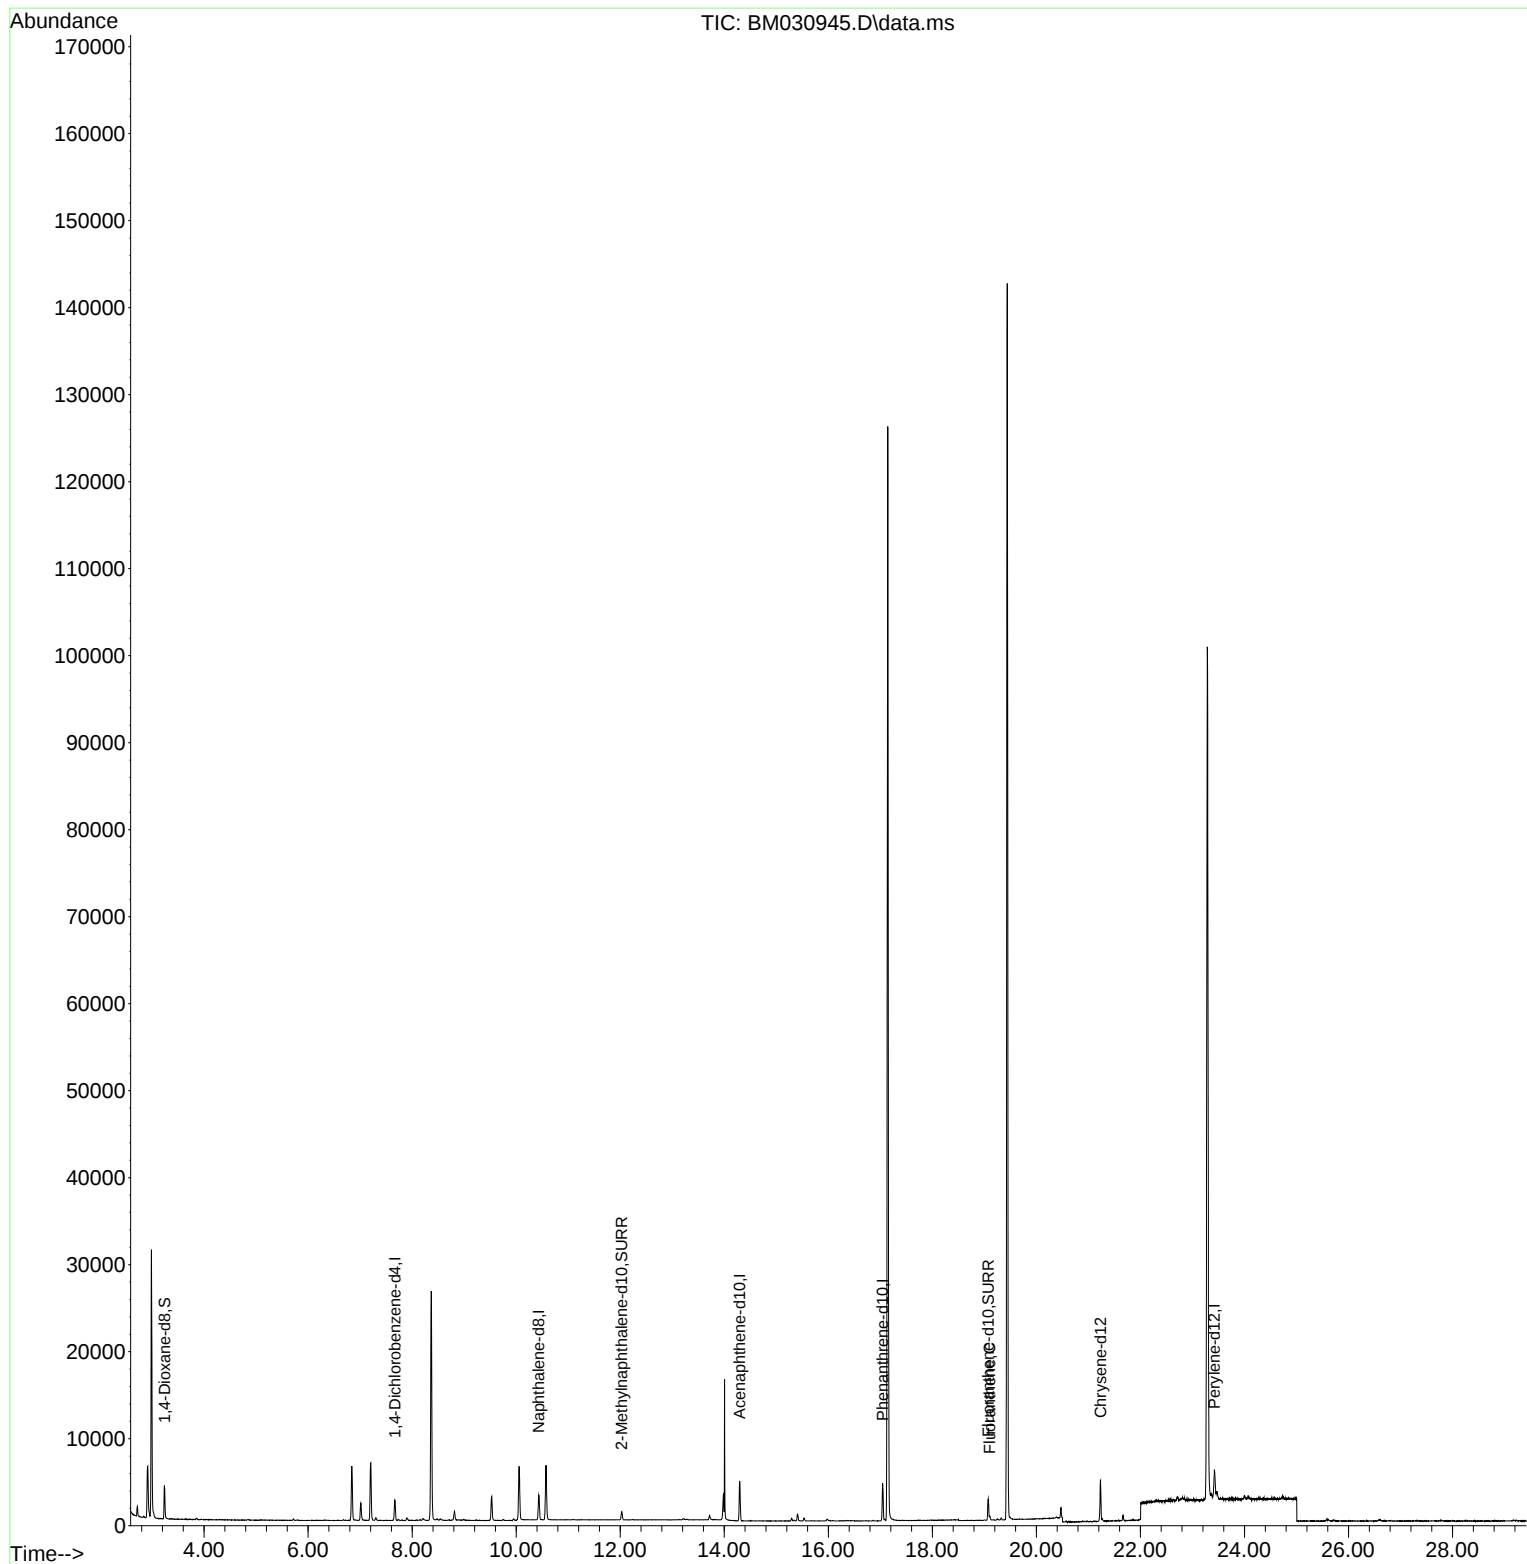

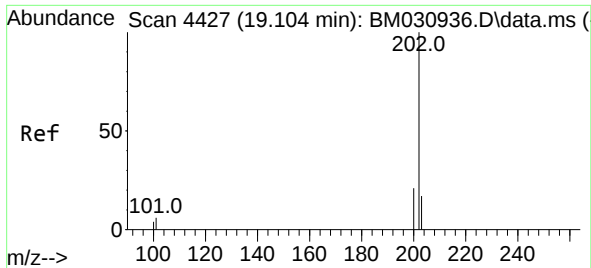

#19  
Fluoranthene  
Concen: 0.021 ng/ul  
RT: 19.104 min Scan# 4427  
Delta R.T. -0.004 min  
Lab File: BM030945.D  
Acq: 13 Jul 2021 23:57

Instrument :  
BNA\_M  
ClientSampleId :  
BGE04

Tgt Ion:202 Resp: 386  
Ion Ratio Lower Upper  
202 100  
101 23.6 6.3 9.5#  
100 19.7 5.0 7.6#

