

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071321\
 Data File : BM030954.D
 Acq On : 14 Jul 2021 09:21
 Operator : CG/JU
 Sample : M2878-02
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGDZ1

Quant Time: Jul 14 10:07:22 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM071321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 13 14:01:01 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.663	152	1157	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.433	136	3939	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.292	164	2542	0.400	ng/ul	-0.01
13) Phenanthrene-d10	17.041	188	5106	0.400	ng/ul	-0.01
17) Chrysene-d12	21.229	240	3880	0.400	ng/ul	0.00
23) Perylene-d12	23.421	264	3845	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.238	96	815	0.685	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.025	152	1850	0.270	ng/ul	0.00
18) Fluoranthene-d10	19.070	212	3866	0.296	ng/ul	0.00
Target Compounds						
19) Fluoranthene	19.100	202	370	0.022	ng/ul#	Qvalue 55


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071321\
Data File : BM030954.D
Acq On : 14 Jul 2021 09:21
Operator : CG/JU
Sample : M2878-02
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGDZ1


Quant Time: Jul 14 10:07:22 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM071321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 13 14:01:01 2021
Response via : Initial Calibration

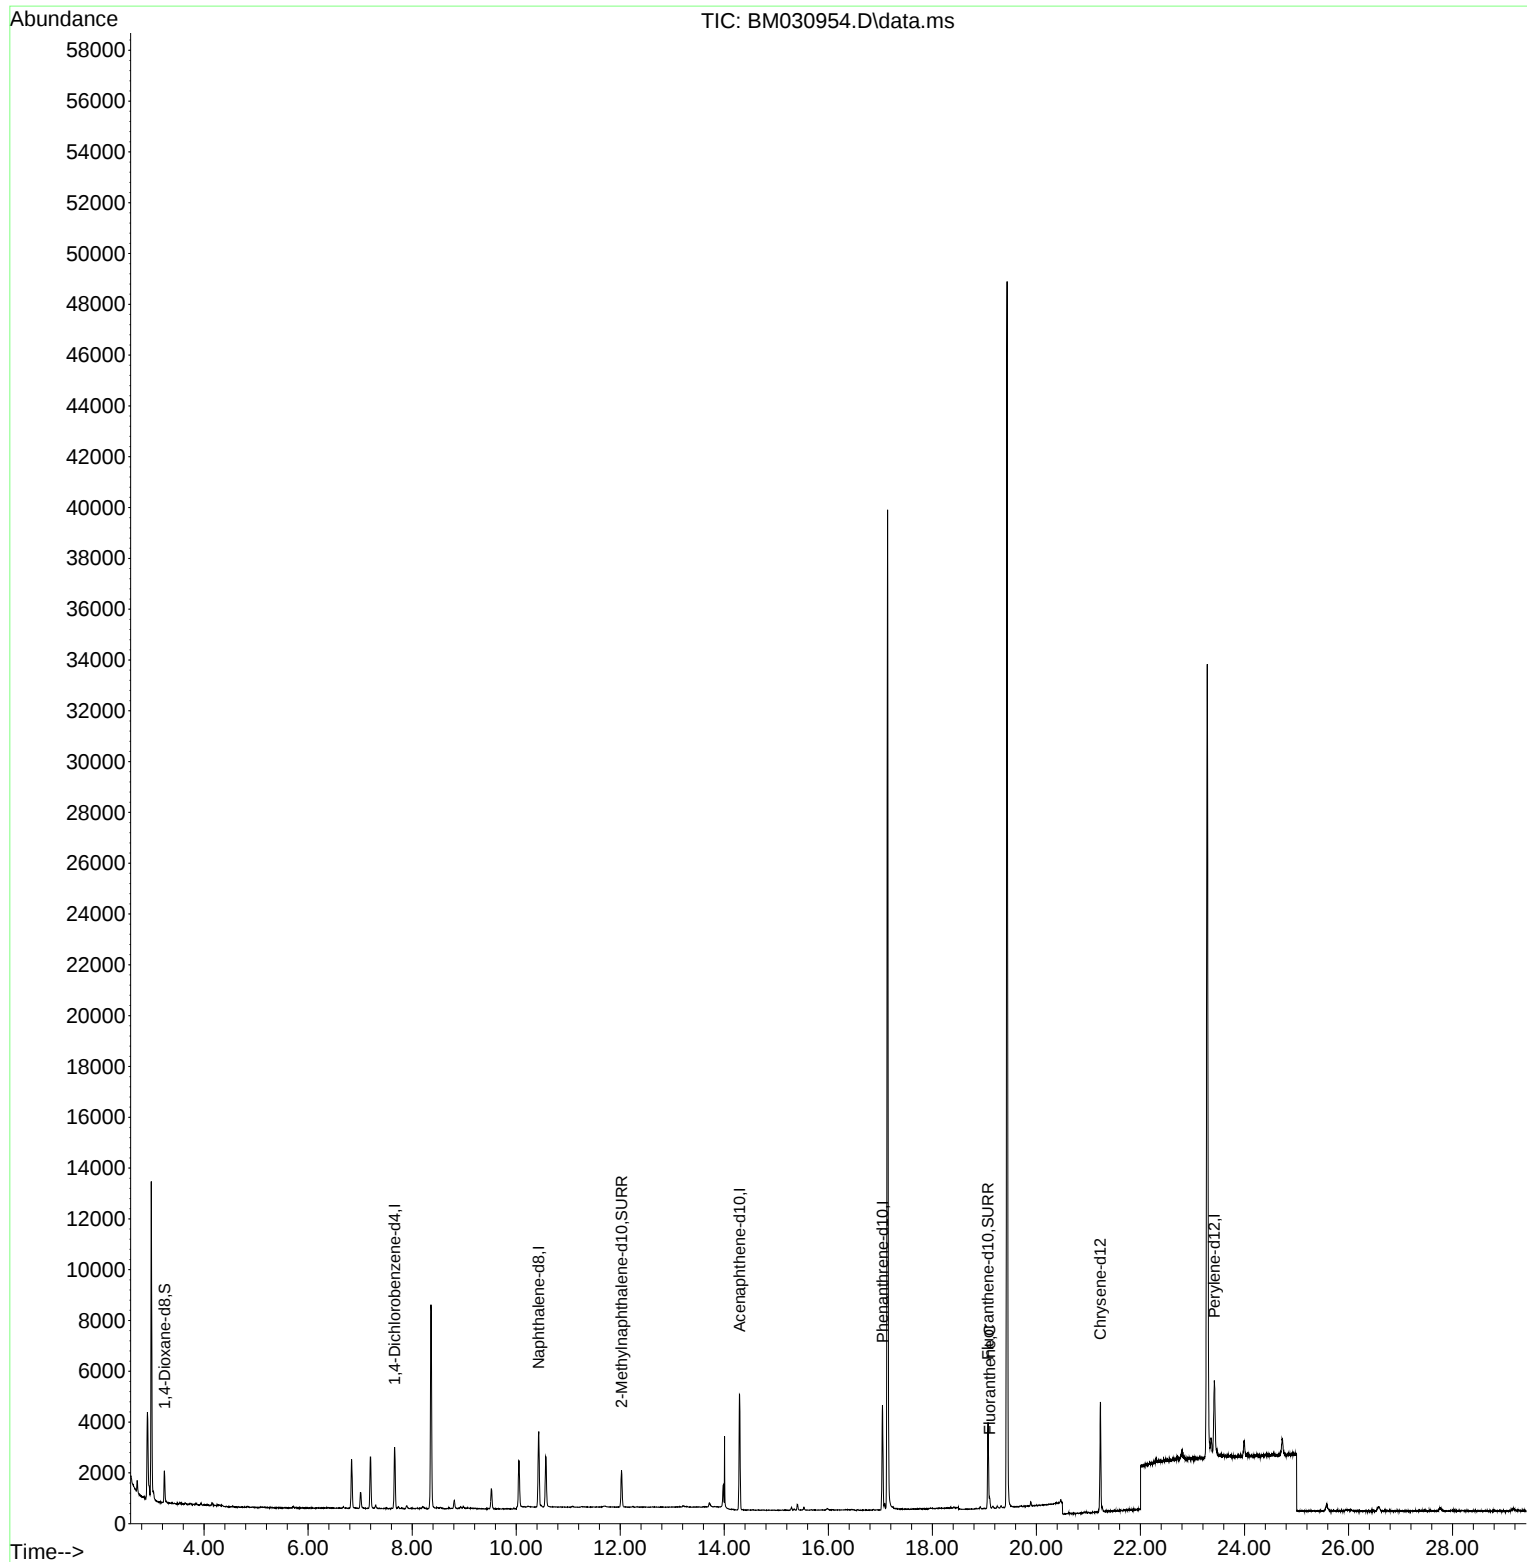

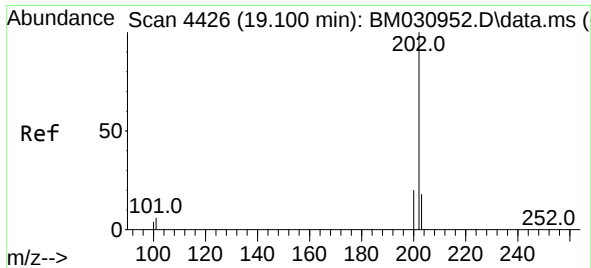

#19
 Fluoranthene
 Concen: 0.022 ng/ul
 RT: 19.100 min Scan# 4426
 Delta R.T. -0.007 min
 Lab File: BM030954.D
 Acq: 14 Jul 2021 09:21

Instrument :
 BNA_M
 ClientSampleId :
 BGDZ1

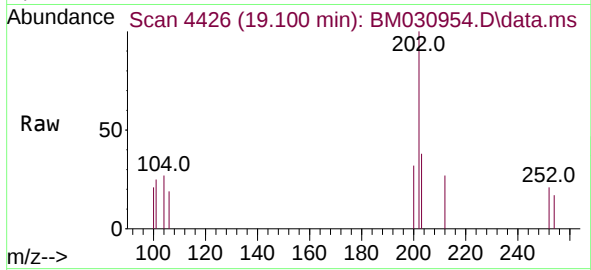

Tgt Ion:	202	Resp:	370
Ion	Ratio	Lower	Upper
202	100		
101	24.9	6.3	9.5#
100	20.5	5.0	7.6#

