

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071423\
 Data File : BM040871.D
 Acq On : 14 Jul 2023 09:42
 Operator : MA/JU
 Sample : PB153998BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK998

Quant Time: Jul 15 03:13:59 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 14 03:14:53 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.857	152	4210	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.658	136	14290	0.400	ng/ul	#-0.01
9) Acenaphthene-d10	14.509	164	6885	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.261	188	13287	0.400	ng/ul	0.00
17) Chrysene-d12	21.457	240	8924	0.400	ng/ul	0.00
23) Perylene-d12	23.836	264	10245	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.275	96	33630	5.085	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.258	152	5654	0.282	ng/ul	0.00
18) Fluoranthene-d10	19.292	212	8715	0.305	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.659	202	1736	0.043	ng/ul#	1
26) Benzo(a)pyrene	23.681	252	3287	0.092	ng/ul#	53


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071423\
Data File : BM040871.D
Acq On : 14 Jul 2023 09:42
Operator : MA/JU
Sample : PB153998BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK998

Quant Time: Jul 15 03:13:59 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 14 03:14:53 2023
Response via : Initial Calibration




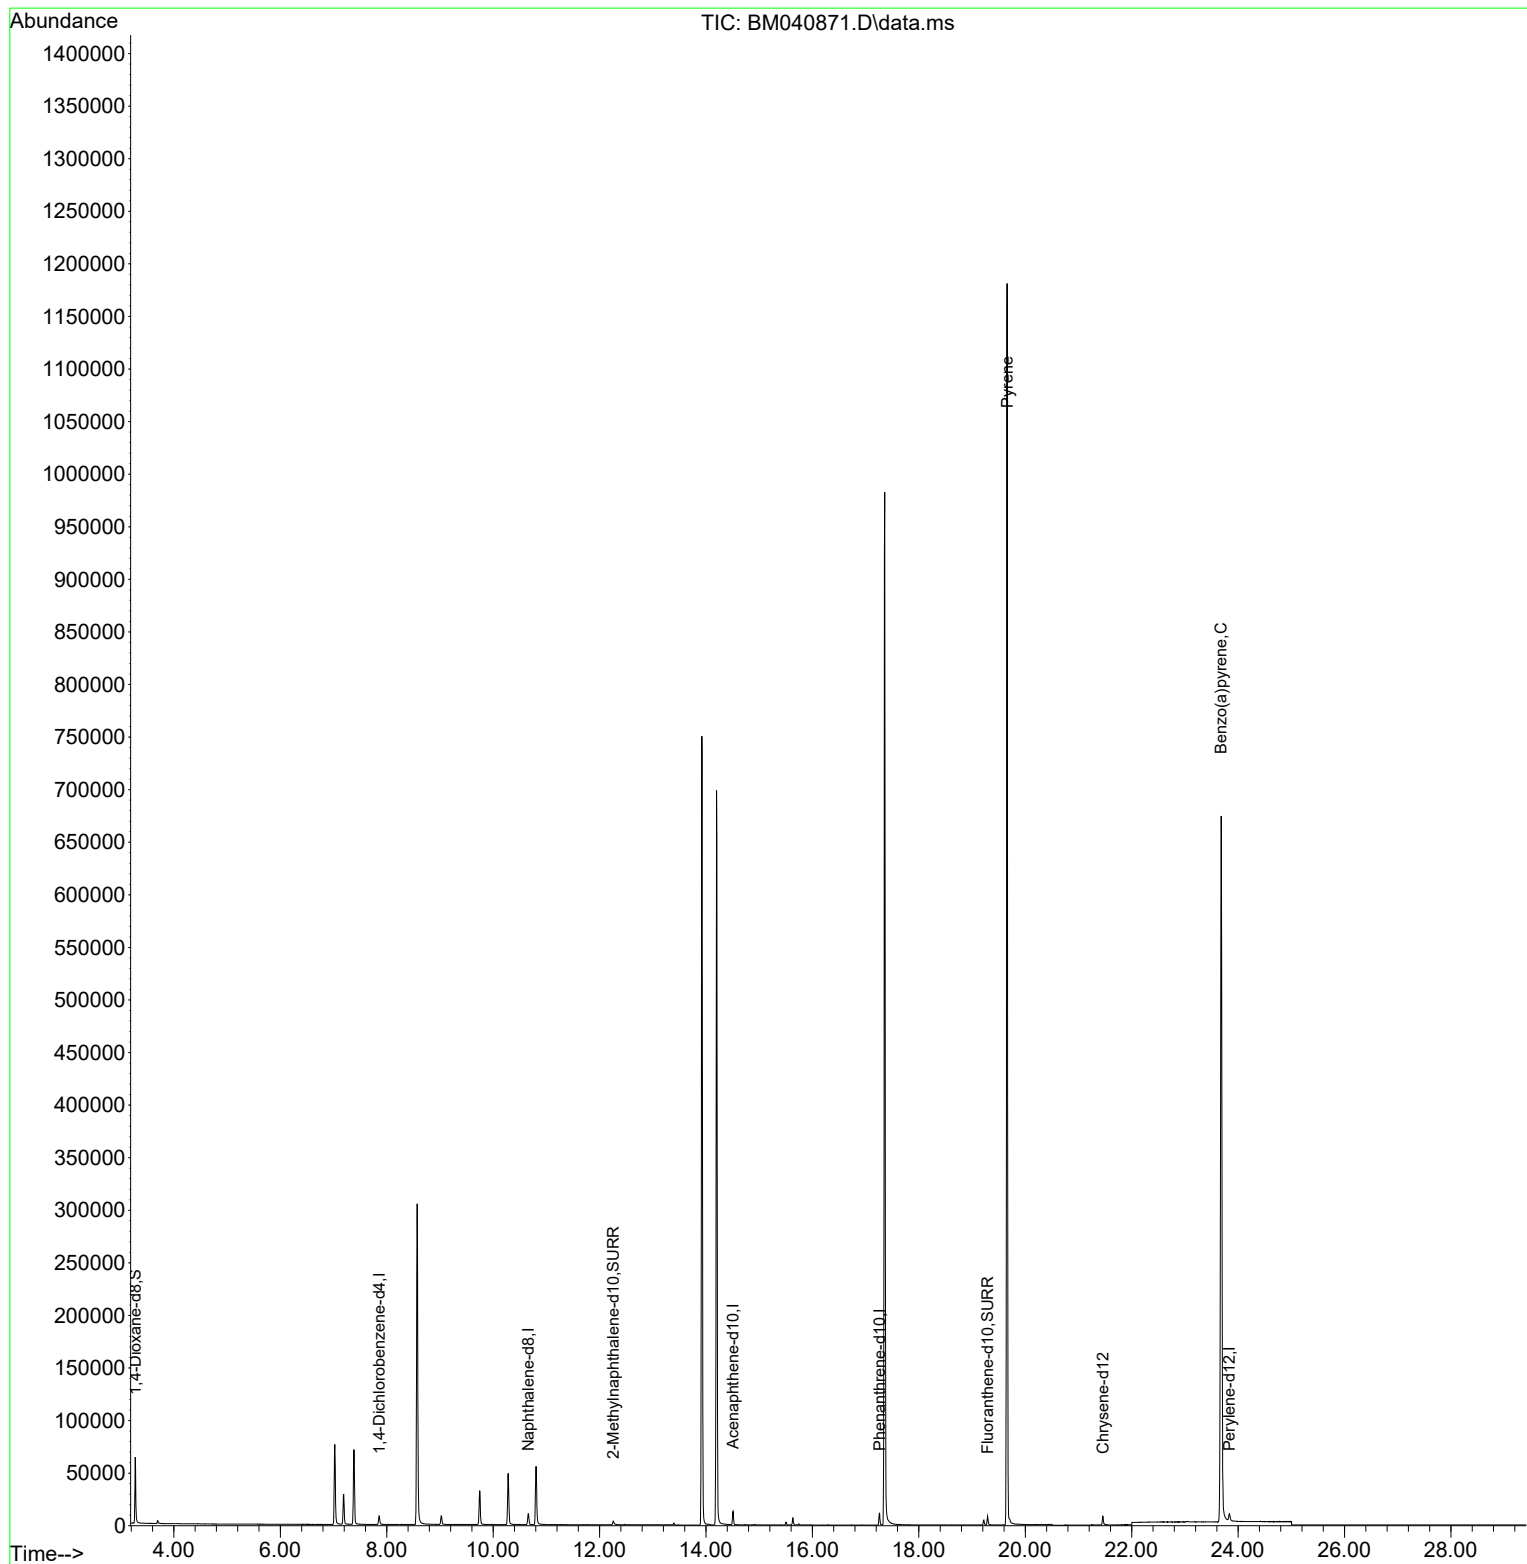


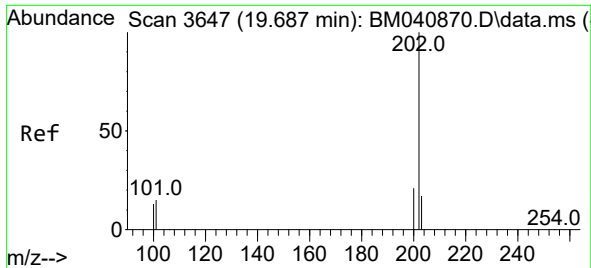

#20
Pyrene
Concen: 0.043 ng/ul
RT: 19.659 min Scan# 30
Delta R.T. -0.032 min
Lab File: BM040871.D
Acq: 14 Jul 2023 09:42

Instrument :
BNA_M
ClientSampleId :
SBLK998

Tgt Ion:202 Resp: 1736
Ion Ratio Lower Upper
202 100
101 172.7 12.6 18.8#
100 1254.6 9.8 14.6#

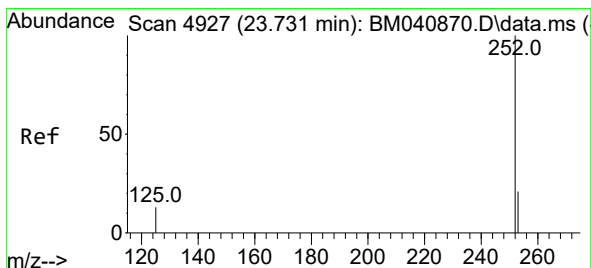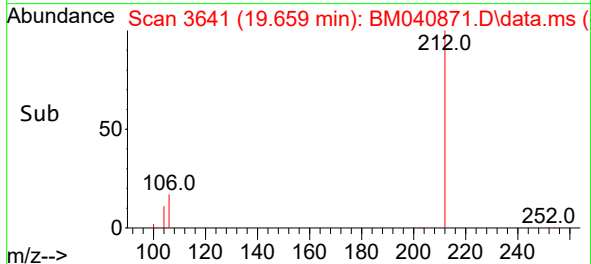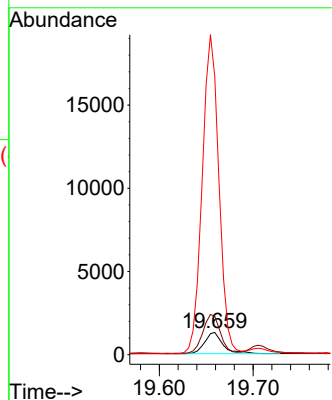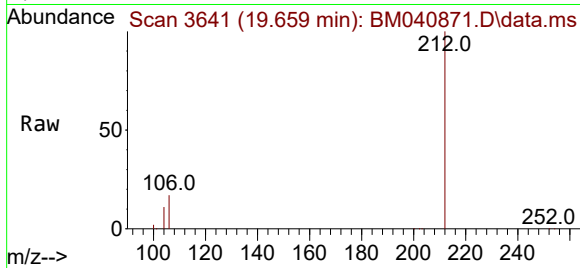

#26
Benzo(a)pyrene
Concen: 0.092 ng/ul
RT: 23.681 min Scan# 4910
Delta R.T. -0.058 min
Lab File: BM040871.D
Acq: 14 Jul 2023 09:42

Tgt Ion:252 Resp: 3287
Ion Ratio Lower Upper
252 100
253 51.8 22.9 34.3#
125 52.2 21.0 31.4#

