

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071423\
 Data File : BM040887.D
 Acq On : 14 Jul 2023 20:09
 Operator : MA/JU
 Sample : 03437-04
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A46H5

Quant Time: Jul 15 03:59:54 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jul 15 03:58:02 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.861	152	3904	0.400	ng/ul	0.00
4) Naphthalene-d8	10.664	136	13047	0.400	ng/ul #	0.00
9) Acenaphthene-d10	14.509	164	5938	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.257	188	10746	0.400	ng/ul	0.00
17) Chrysene-d12	21.451	240	7322	0.400	ng/ul	0.00
23) Perylene-d12	23.827	264	6722	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.280	96	6201	1.011	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.258	152	1234	0.067	ng/ul	0.00
18) Fluoranthene-d10	19.292	212	1906	0.081	ng/ul	0.00
Target Compounds						
					Qvalue	
5) Naphthalene	10.713	128	16179	0.450	ng/ul	99
7) 2-Methylnaphthalene	12.330	142	849	0.040	ng/ul	98
15) Phenanthrene	17.299	178	5117	0.153	ng/ul	96
19) Fluoranthene	19.320	202	14815	0.476	ng/ul	98
20) Pyrene	19.682	202	11810	0.354	ng/ul	99
21) Benzo(a)anthracene	21.434	228	4425	0.179	ng/ul	94
22) Chrysene	21.486	228	7141	0.253	ng/ul	97
24) Benzo(b)fluoranthene	23.105	252	9227	0.355	ng/ul	86
26) Benzo(a)pyrene	23.722	252	1729	0.074	ng/ul#	27
27) Indeno(1,2,3-cd)pyrene	26.287	276	4077	0.125	ng/ul#	90
28) Dibenzo(a,h)anthracene	26.300	278	1239	0.048	ng/ul#	34
29) Benzo(g,h,i)perylene	27.041	276	783	0.027	ng/ul#	43


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071423\
Data File : BM040887.D
Acq On : 14 Jul 2023 20:09
Operator : MA/JU
Sample : 03437-04
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A46H5

Quant Time: Jul 15 03:59:54 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jul 15 03:58:02 2023
Response via : Initial Calibration

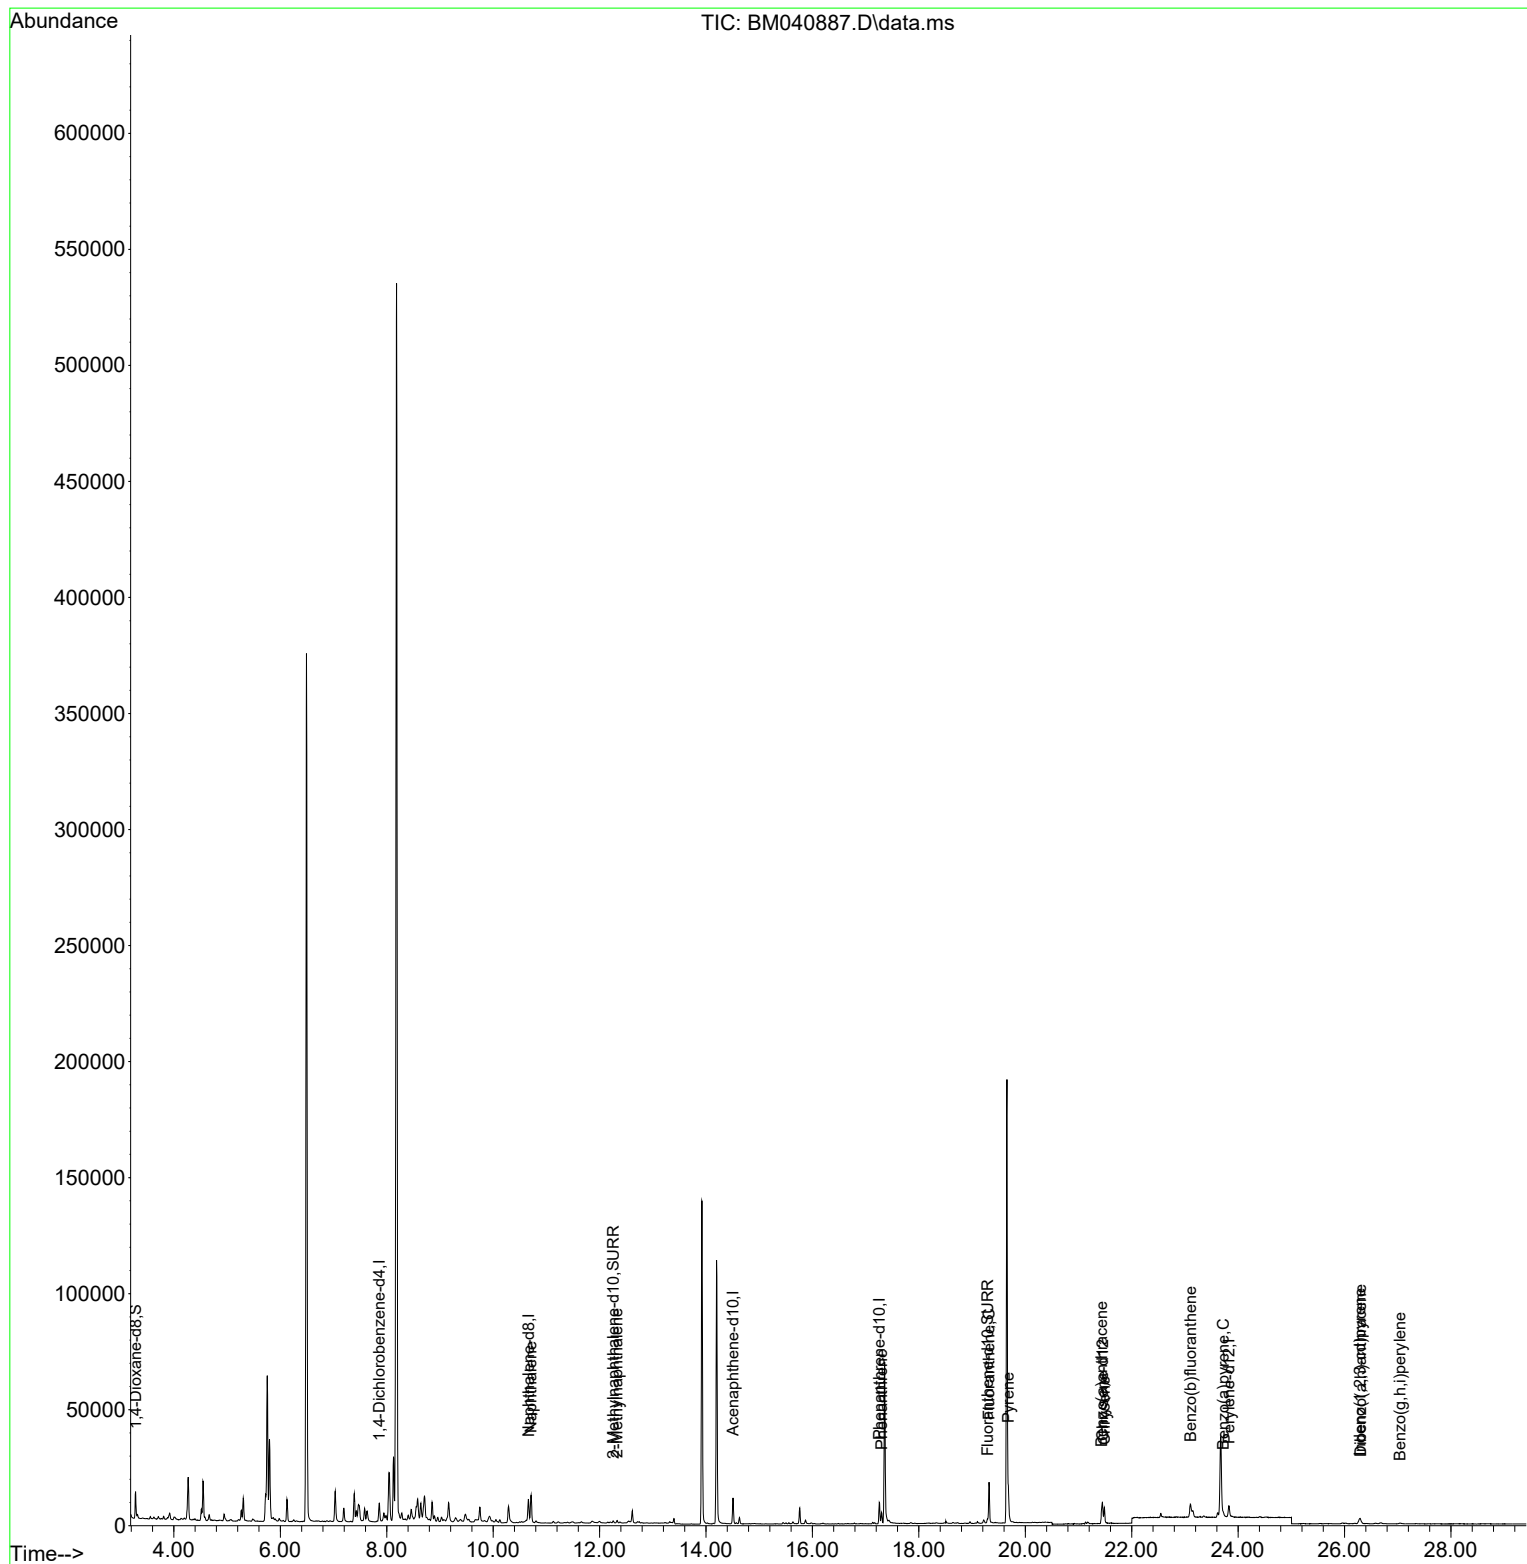



#5

Naphthalene

Concen: 0.450 ng/ul

RT: 10.713 min Scan# 1

Delta R.T. -0.000 min

Lab File: BM040887.D

Acq: 14 Jul 2023 20:09

Instrument :

BNA_M

ClientSampleId :

A46H5





Tgt Ion:128 Resp: 16179

Ion Ratio Lower Upper

128 100

129 11.7 9.2 13.8

127 13.6 10.6 15.8

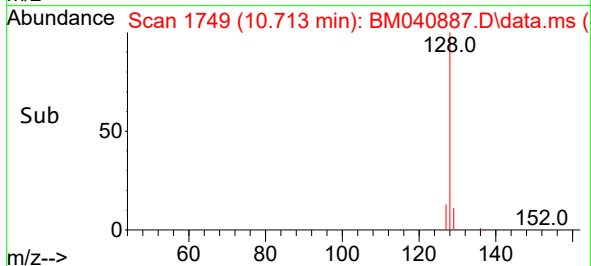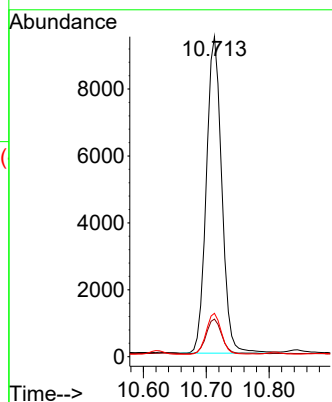

#7

2-Methylnaphthalene

Concen: 0.040 ng/ul

RT: 12.330 min Scan# 2043

Delta R.T. -0.000 min

Lab File: BM040887.D




Acq: 14 Jul 2023 20:09


Tgt Ion:142 Resp: 849

Ion Ratio Lower Upper

142 100

141 91.6 71.9 107.9


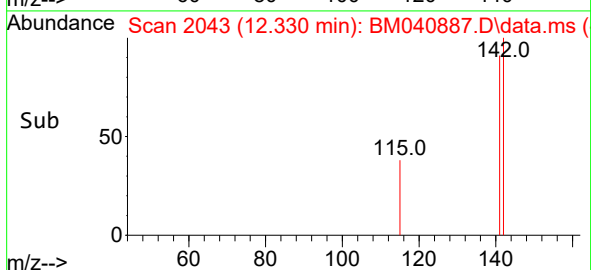
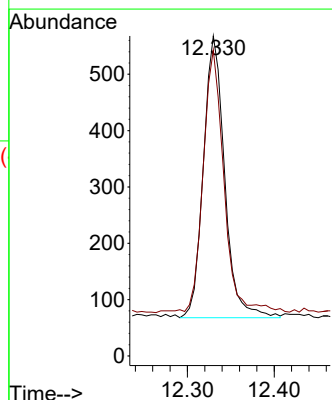
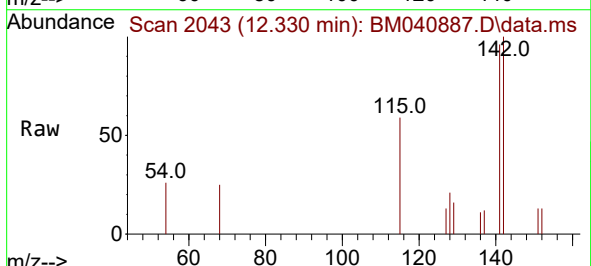


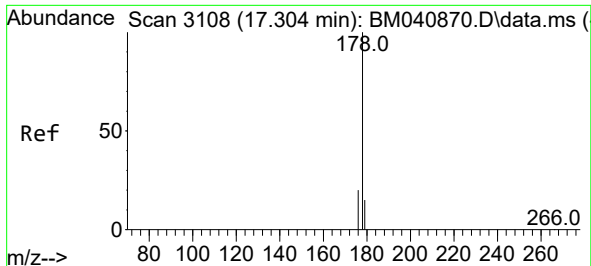

#15
Phenanthrene
Concen: 0.153 ng/ul
RT: 17.299 min Scan# 3107
Delta R.T. -0.004 min
Lab File: BM040887.D
Acq: 14 Jul 2023 20:09




Instrument :
BNA_M
ClientSampleId :
A46H5


Tgt Ion:178 Resp: 5117
Ion Ratio Lower Upper
178 100
179 18.1 12.8 19.2
176 22.0 16.4 24.6

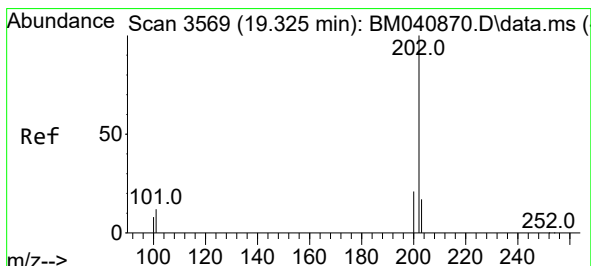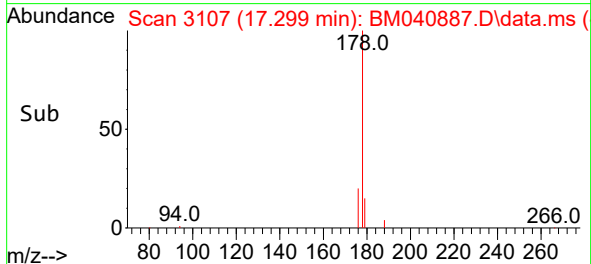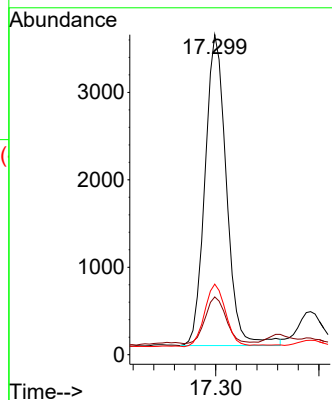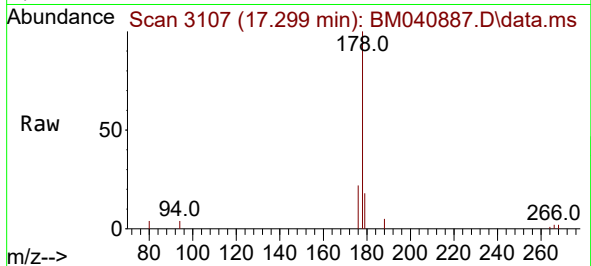

#19
Fluoranthene
Concen: 0.476 ng/ul
RT: 19.320 min Scan# 3568
Delta R.T. -0.005 min
Lab File: BM040887.D
Acq: 14 Jul 2023 20:09

Tgt Ion:202 Resp: 14815
Ion Ratio Lower Upper
202 100
101 13.2 11.4 17.0
100 10.4 8.7 13.1


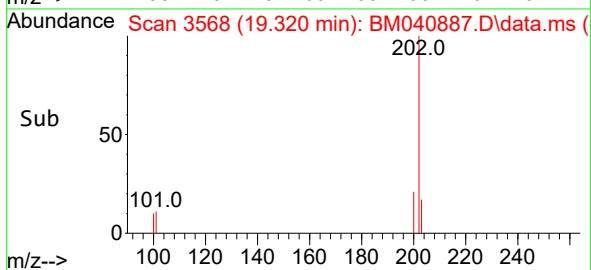
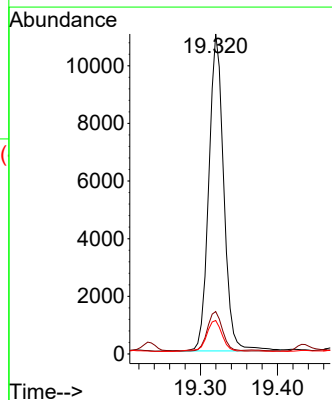
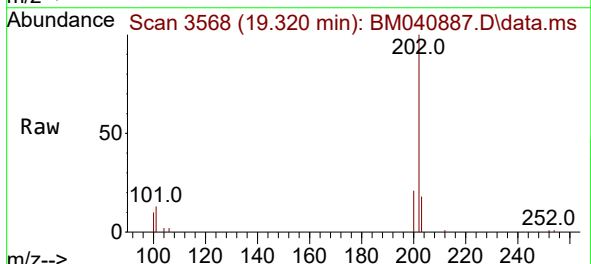


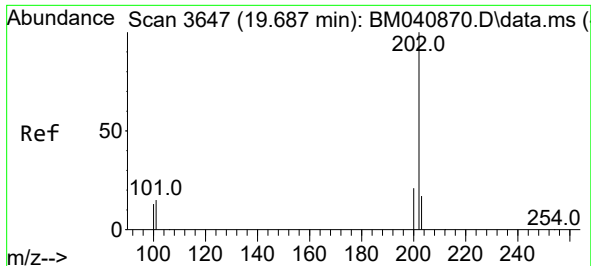

#20
 Pyrene
 Concen: 0.354 ng/ul
 RT: 19.682 min Scan# 30
 Delta R.T. -0.005 min
 Lab File: BM040887.D
 Acq: 14 Jul 2023 20:09




Instrument :
 BNA_M
 ClientSampleId :
 A46H5


Tgt Ion:202 Resp: 11810
 Ion Ratio Lower Upper
 202 100
 101 15.6 12.6 18.8
 100 13.4 9.8 14.6

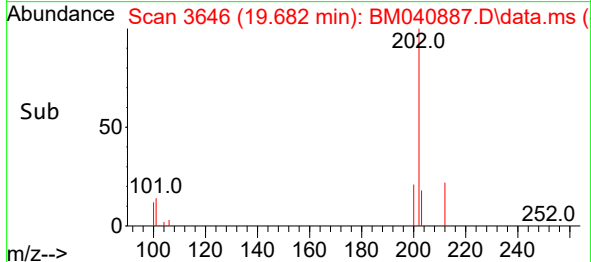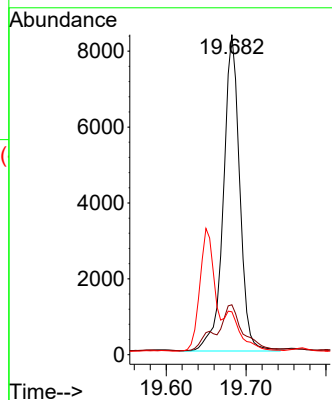

#21
 Benzo(a)anthracene
 Concen: 0.179 ng/ul
 RT: 21.434 min Scan# 4141
 Delta R.T. -0.000 min
 Lab File: BM040887.D
 Acq: 14 Jul 2023 20:09

Tgt Ion:228 Resp: 4425
 Ion Ratio Lower Upper
 228 100
 229 24.0 16.0 24.0
 226 30.0 22.3 33.5

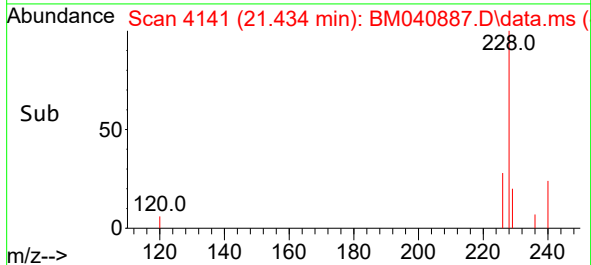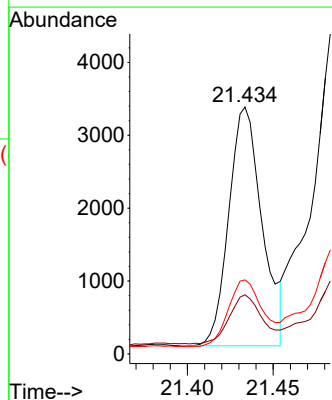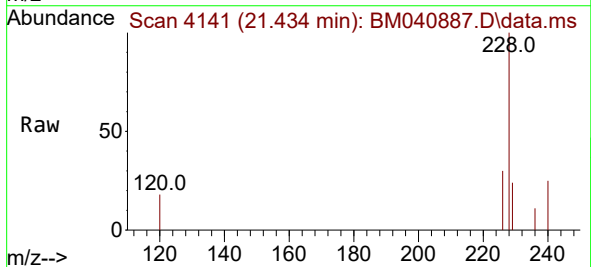

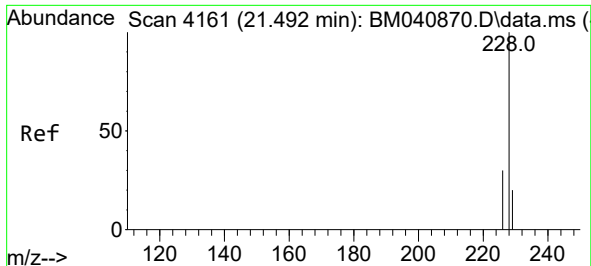

#22

Chrysene

Concen: 0.253 ng/ul

RT: 21.486 min Scan# 41

Delta R.T. -0.000 min

Lab File: BM040887.D

Acq: 14 Jul 2023 20:09

Instrument :

BNA_M

ClientSampleId :

A46H5





Tgt Ion:228 Resp: 7141

Ion Ratio Lower Upper

228 100

226 31.9 24.9 37.3

229 22.6 15.8 23.6

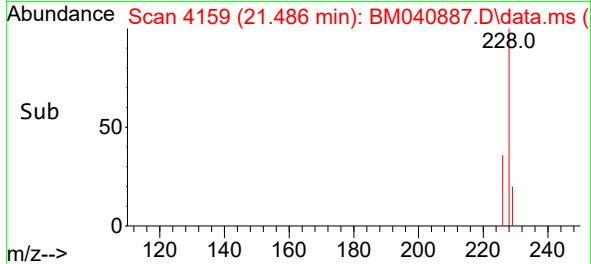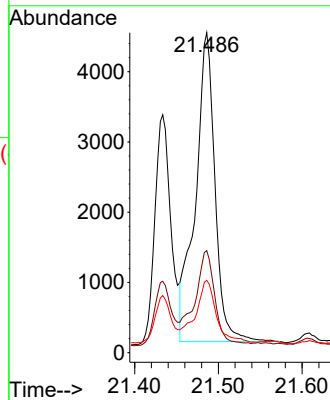

#24

Benzo(b)fluoranthene

Concen: 0.355 ng/ul

RT: 23.105 min Scan# 4713

Delta R.T. 0.003 min

Lab File: BM040887.D

Acq: 14 Jul 2023 20:09




Tgt Ion:252 Resp: 9227


Ion Ratio Lower Upper

252 100

253 31.1 0.0 52.8

125 31.2 0.0 43.0


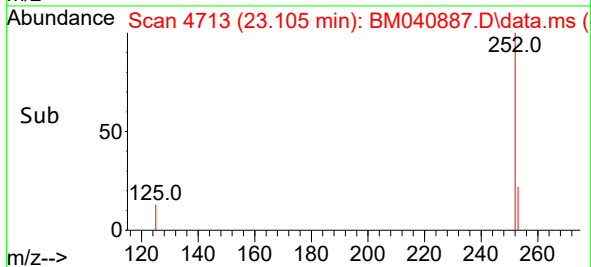
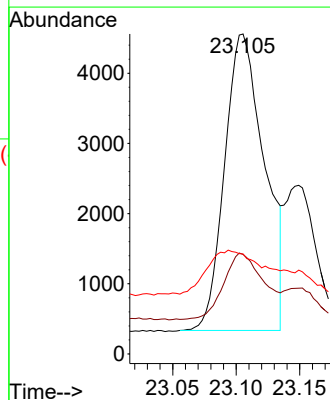
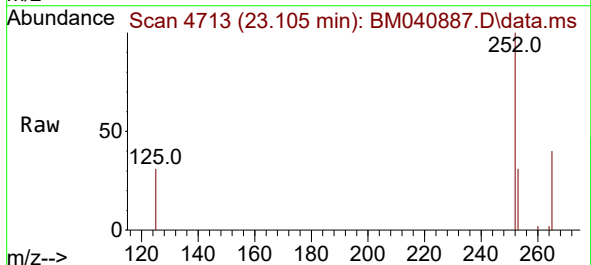


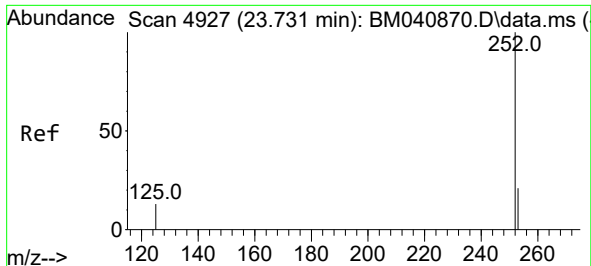

#26
Benzo(a)pyrene
Concen: 0.074 ng/ul
RT: 23.722 min Scan# 4924
Delta R.T. -0.000 min
Lab File: BM040887.D
Acq: 14 Jul 2023 20:09




Instrument :
BNA_M
ClientSampleId :
A46H5


Tgt Ion:252 Resp: 1729
Ion Ratio Lower Upper
252 100
253 56.9 22.9 34.3#
125 74.5 21.0 31.4#

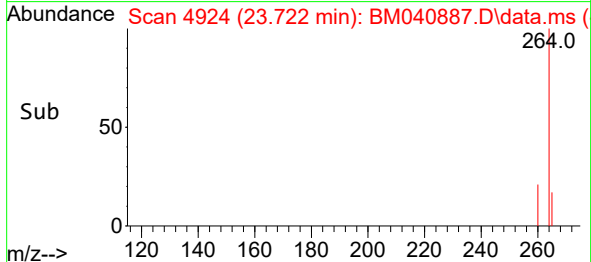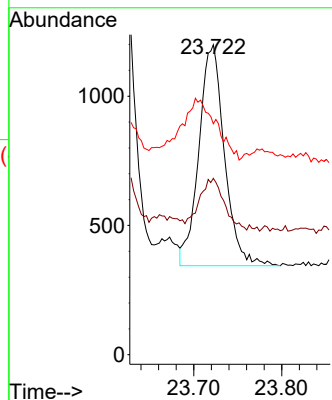

#27
Indeno(1,2,3-cd)pyrene
Concen: 0.125 ng/ul
RT: 26.287 min Scan# 5745
Delta R.T. -0.003 min
Lab File: BM040887.D
Acq: 14 Jul 2023 20:09

Tgt Ion:276 Resp: 4077
Ion Ratio Lower Upper
276 100
138 24.9 24.5 36.7
227 0.2 0.1 0.1#


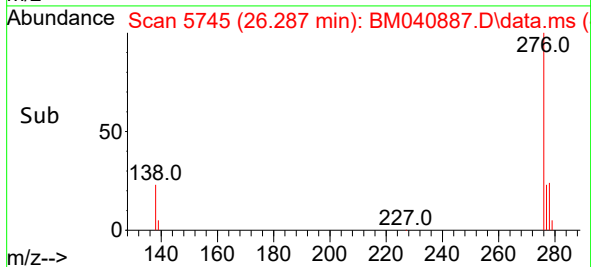
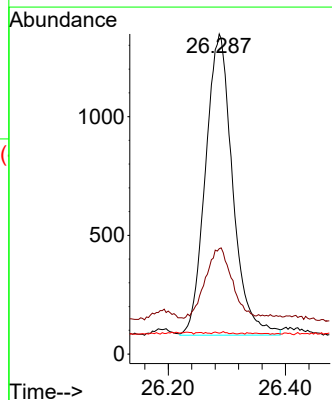
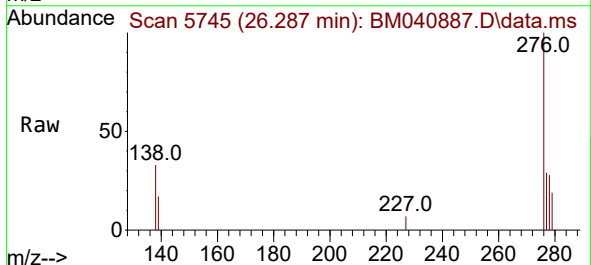


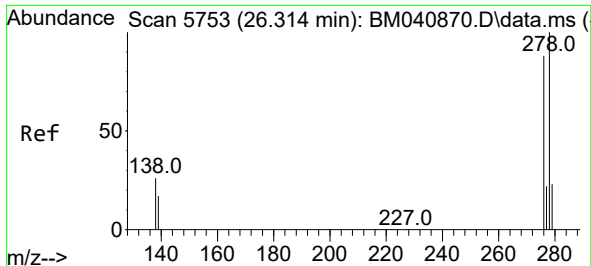

#28
Dibenzo(a,h)anthracene
Concen: 0.048 ng/ul
RT: 26.300 min Scan# 51
Delta R.T. -0.007 min
Lab File: BM040887.D
Acq: 14 Jul 2023 20:09

Instrument :
BNA_M
ClientSampleId :
A46H5

Tgt Ion:278 Resp: 1239
Ion Ratio Lower Upper
278 100
139 54.0 17.9 26.9#
279 61.9 22.0 33.0#

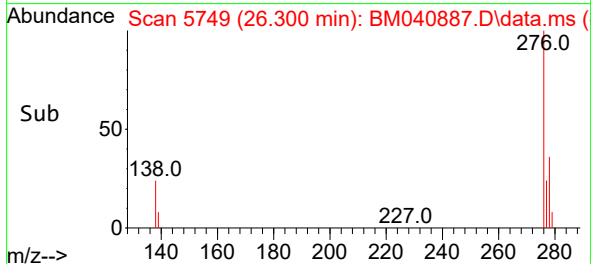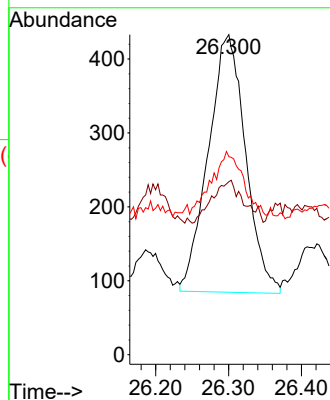

#29
Benzo(g,h,i)perylene
Concen: 0.027 ng/ul
RT: 27.041 min Scan# 5970
Delta R.T. -0.003 min
Lab File: BM040887.D
Acq: 14 Jul 2023 20:09

Tgt Ion:276 Resp: 783
Ion Ratio Lower Upper
276 100
138 63.8 23.0 34.6#
277 49.7 20.3 30.5#

