

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071423\
 Data File : BM040906.D
 Acq On : 15 Jul 2023 15:20
 Operator : MA/JU
 Sample : PB154014BL
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK014

Quant Time: Jul 16 00:29:12 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jul 15 03:58:02 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.853	152	4778	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.653	136	16242	0.400	ng/ul	#-0.01
9) Acenaphthene-d10	14.504	164	7719	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.257	188	13573	0.400	ng/ul	0.00
17) Chrysene-d12	21.451	240	7736	0.400	ng/ul	0.00
23) Perylene-d12	23.831	264	9391	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.275	96	53917	7.184	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.247	152	9090	0.399	ng/ul	-0.01
18) Fluoranthene-d10	19.287	212	11944	0.482	ng/ul	0.00
Target Compounds						Qvalue
16) Anthracene	17.354	178	1159	0.033	ng/ul#	1
20) Pyrene	19.654	202	2554	0.072	ng/ul#	1
26) Benzo(a)pyrene	23.673	252	4393	0.134	ng/ul#	58


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071423\
Data File : BM040906.D
Acq On : 15 Jul 2023 15:20
Operator : MA/JU
Sample : PB154014BL
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK014

Quant Time: Jul 16 00:29:12 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jul 15 03:58:02 2023
Response via : Initial Calibration




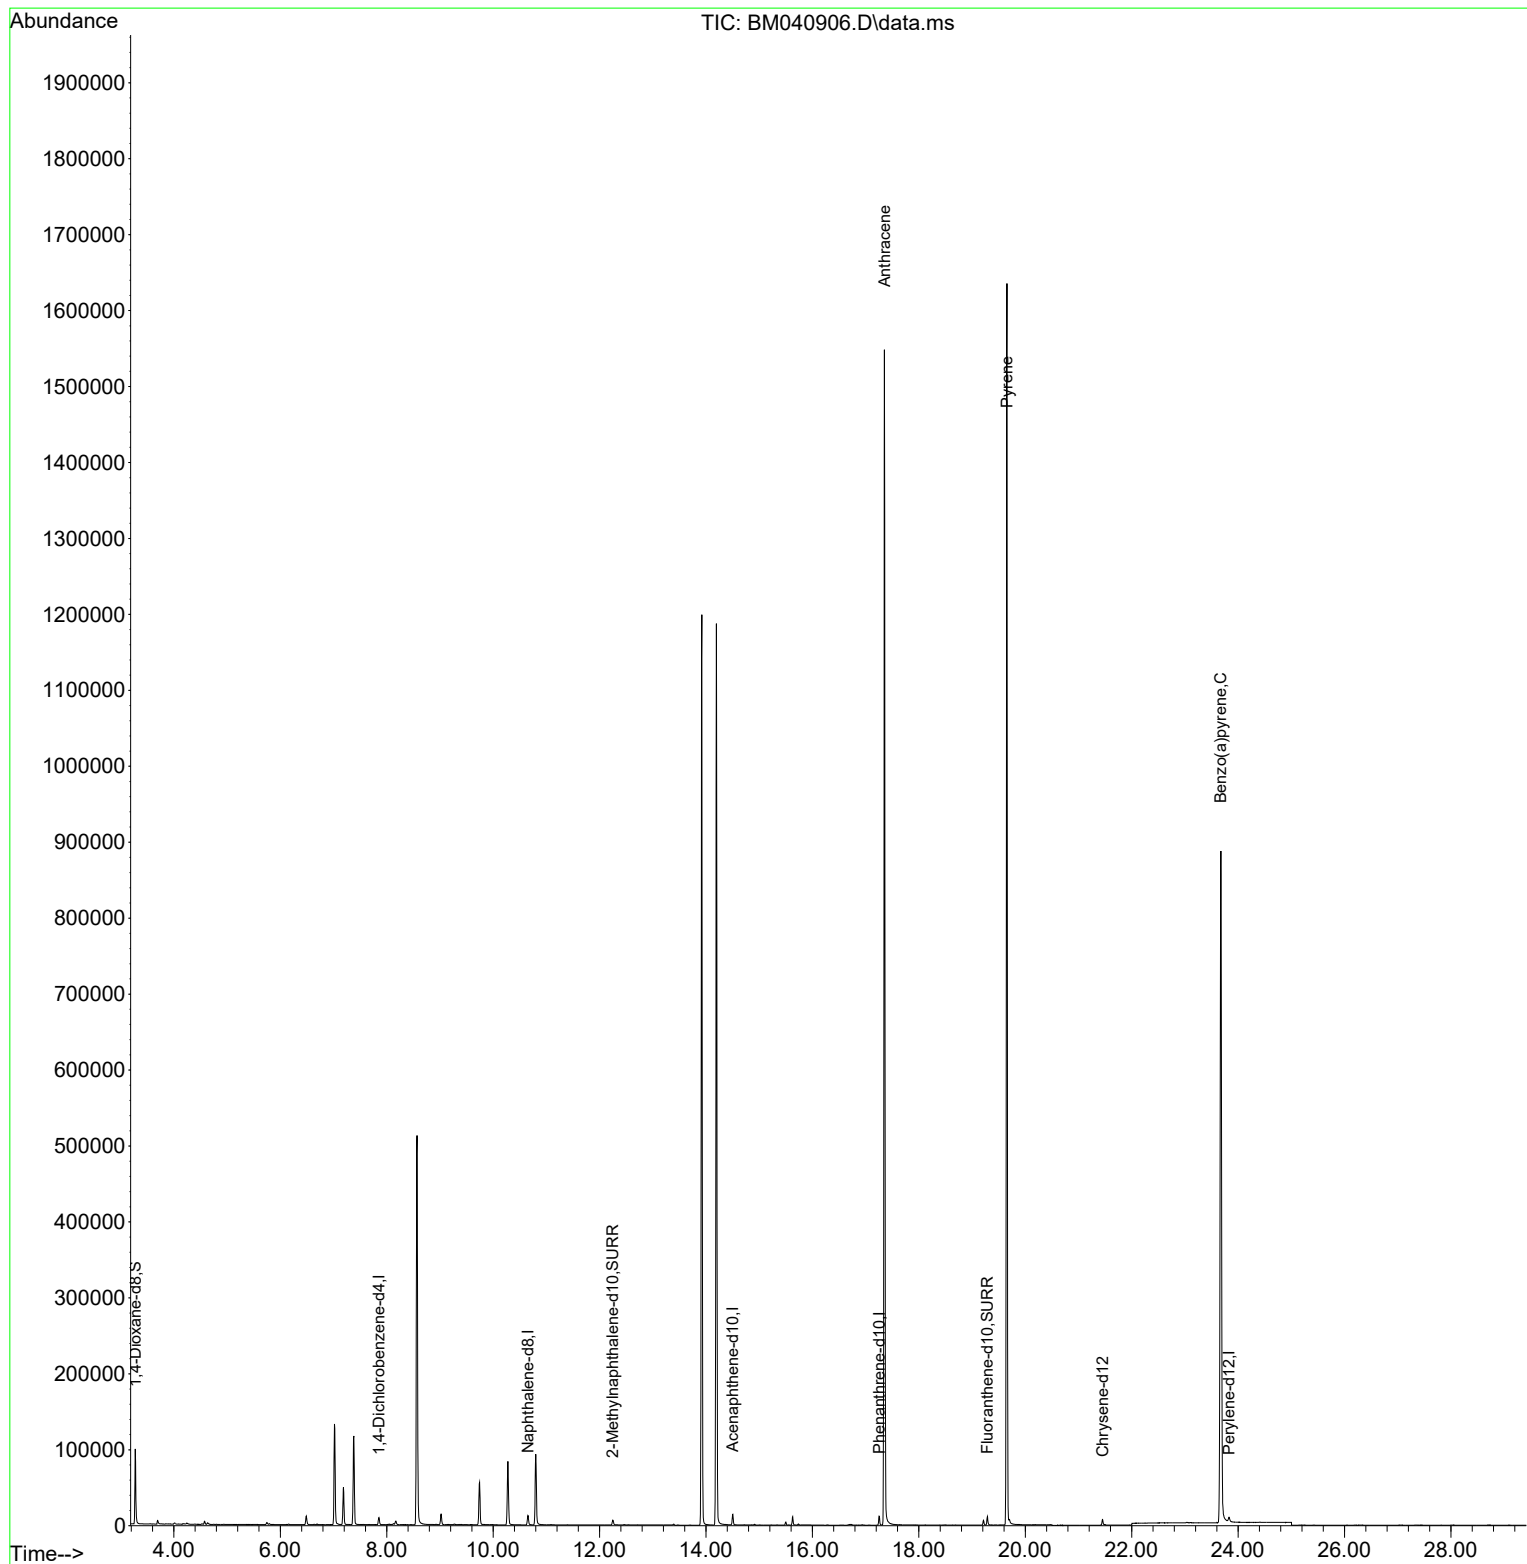


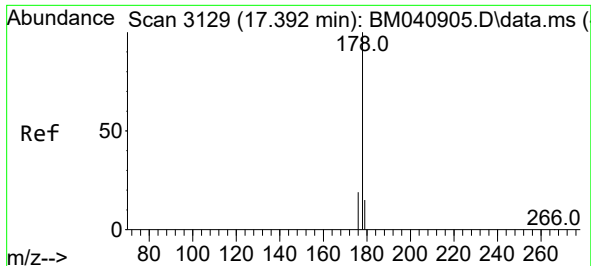

#16
 Anthracene
 Concen: 0.033 ng/ul
 RT: 17.354 min Scan# 3129
 Delta R.T. -0.042 min
 Lab File: BM040906.D
 Acq: 15 Jul 2023 15:20




Instrument :
 BNA_M
 ClientSampleId :
 SBLK014


Tgt Ion:178 Resp: 1159
 Ion Ratio Lower Upper
 178 100
 179 181.6 12.9 19.3#
 176 20.8 15.8 23.6

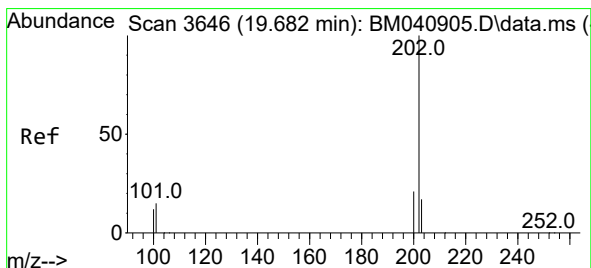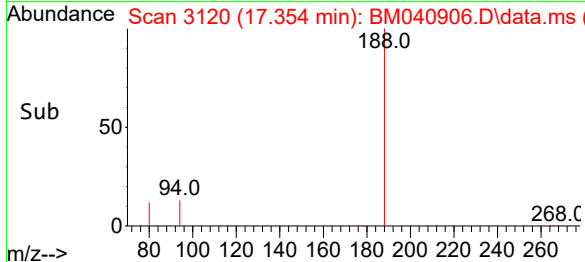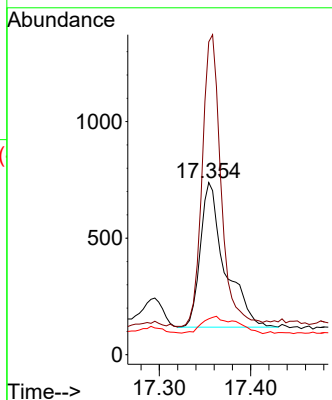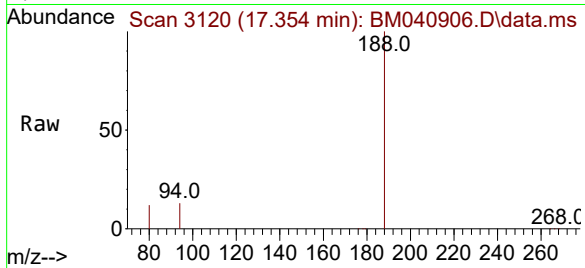

#20
 Pyrene
 Concen: 0.072 ng/ul
 RT: 19.654 min Scan# 3640
 Delta R.T. -0.032 min
 Lab File: BM040906.D
 Acq: 15 Jul 2023 15:20


Tgt Ion:202 Resp: 2554
 Ion Ratio Lower Upper
 202 100
 101 178.1 12.6 18.8#
 100 1323.3 9.8 14.6#

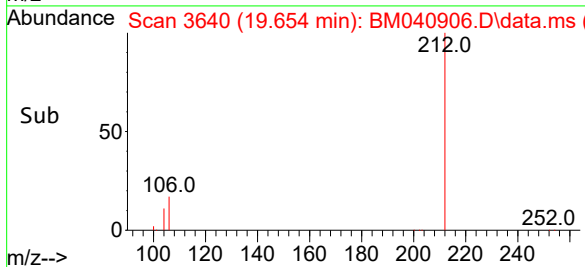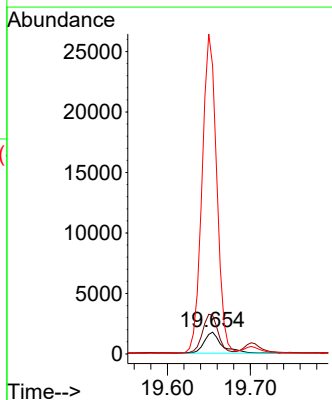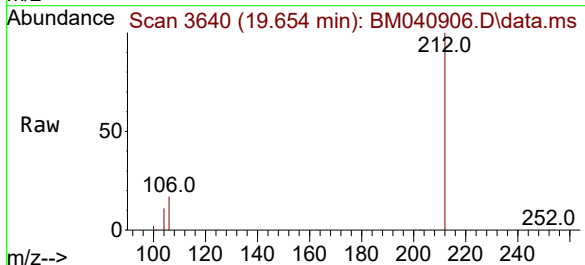

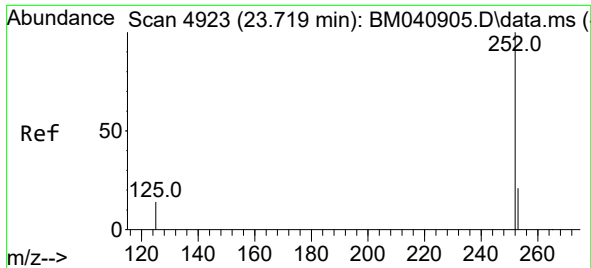

#26
Benzo(a)pyrene
Concen: 0.134 ng/ul
RT: 23.673 min Scan# 4923
Delta R.T. -0.050 min
Lab File: BM040906.D
Acq: 15 Jul 2023 15:20

Instrument :
BNA_M
ClientSampleId :
SBLK014

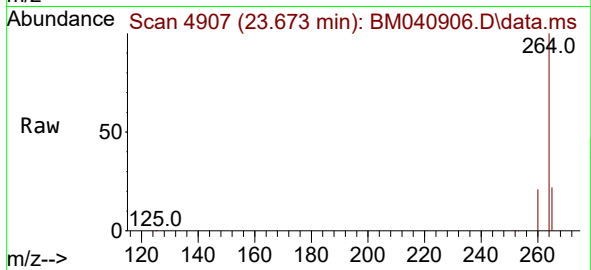

Tgt Ion:252 Resp: 4393
Ion Ratio Lower Upper
252 100
253 48.3 22.9 34.3#
125 50.2 21.0 31.4#

