
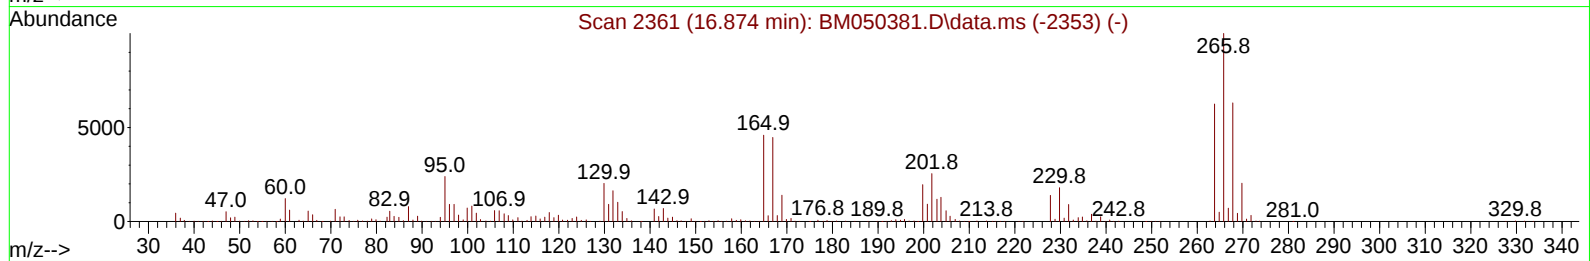
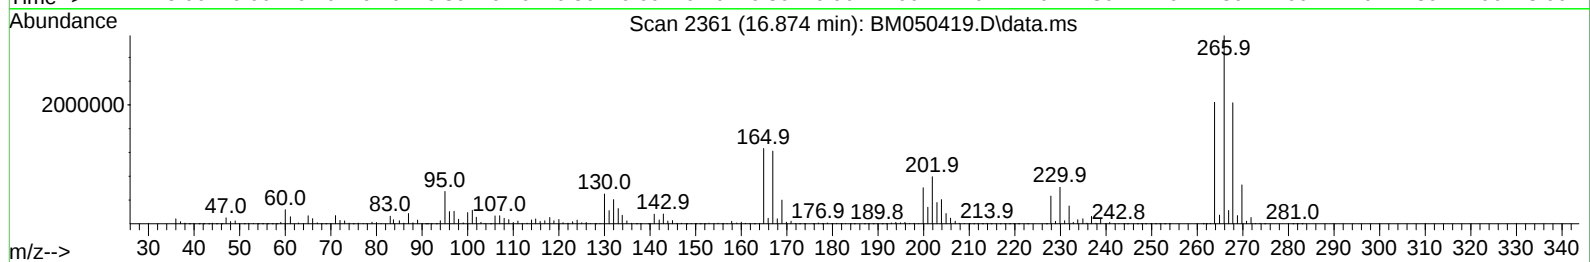


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071425\
Data File : BM050419.D
Acq On : 14 Jul 2025 09:30
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 14 11:57:50 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM070925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 08 18:32:25 2025
Response via : Initial Calibration

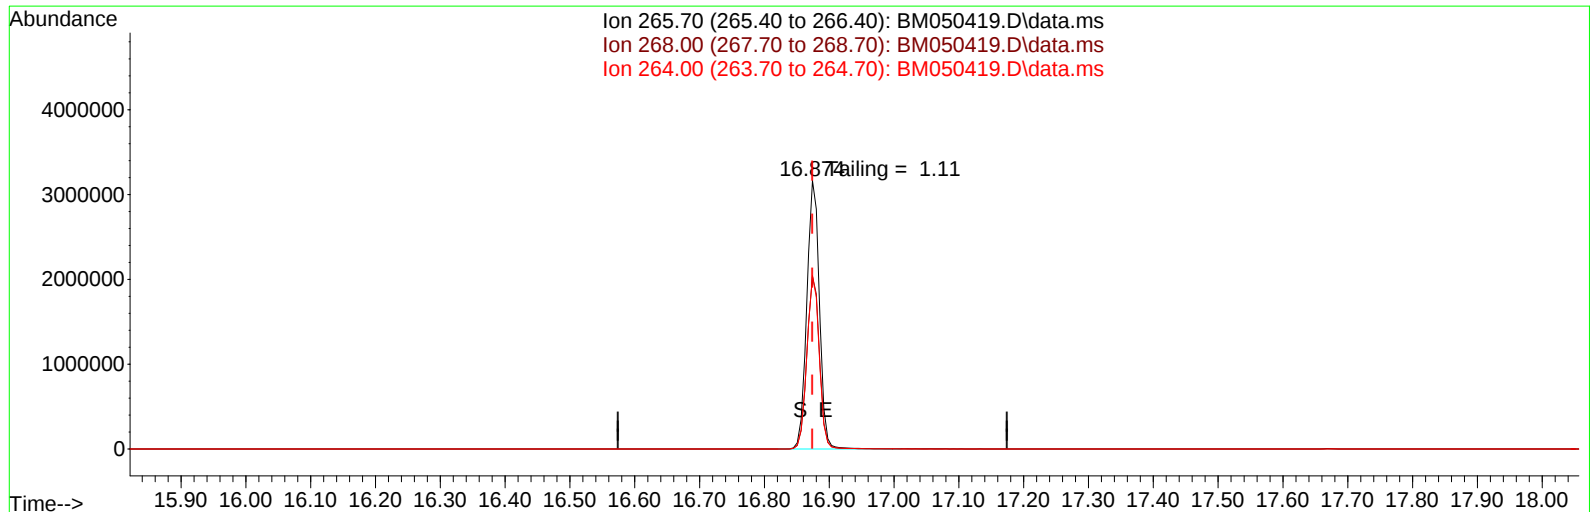

TIC: BM050419.D\data.ms

(70) Pentachlorophenol (C)




16.874min (-0.000) 1727729.72 ng

response 4282661

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	64.32
264.00	62.40	64.56
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071425\
Data File : BM050419.D
Acq On : 14 Jul 2025 09:30
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 14 11:57:50 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM070925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 08 18:32:25 2025
Response via : Initial Calibration

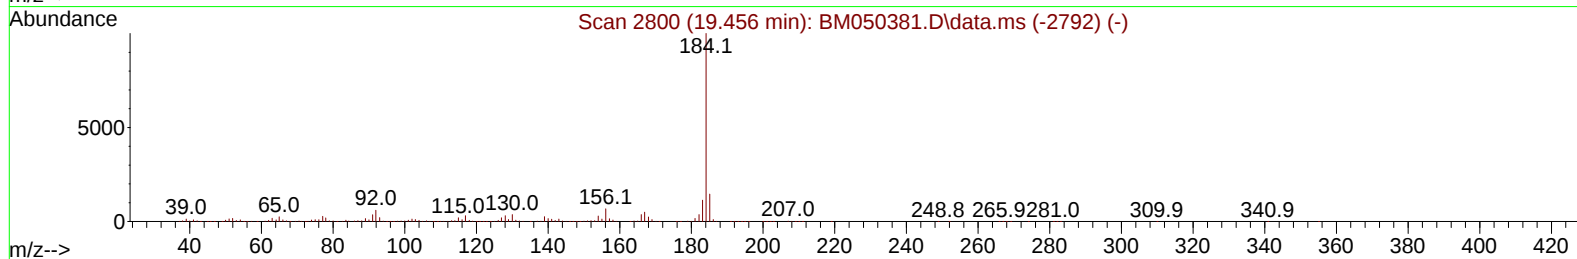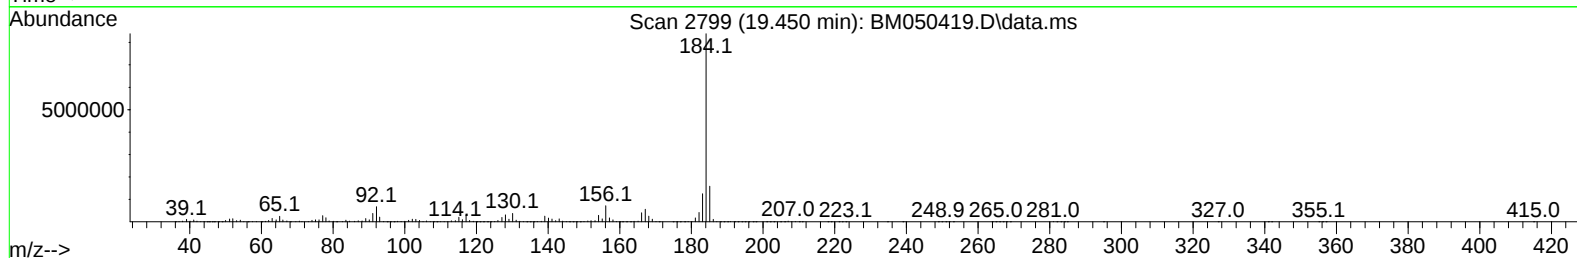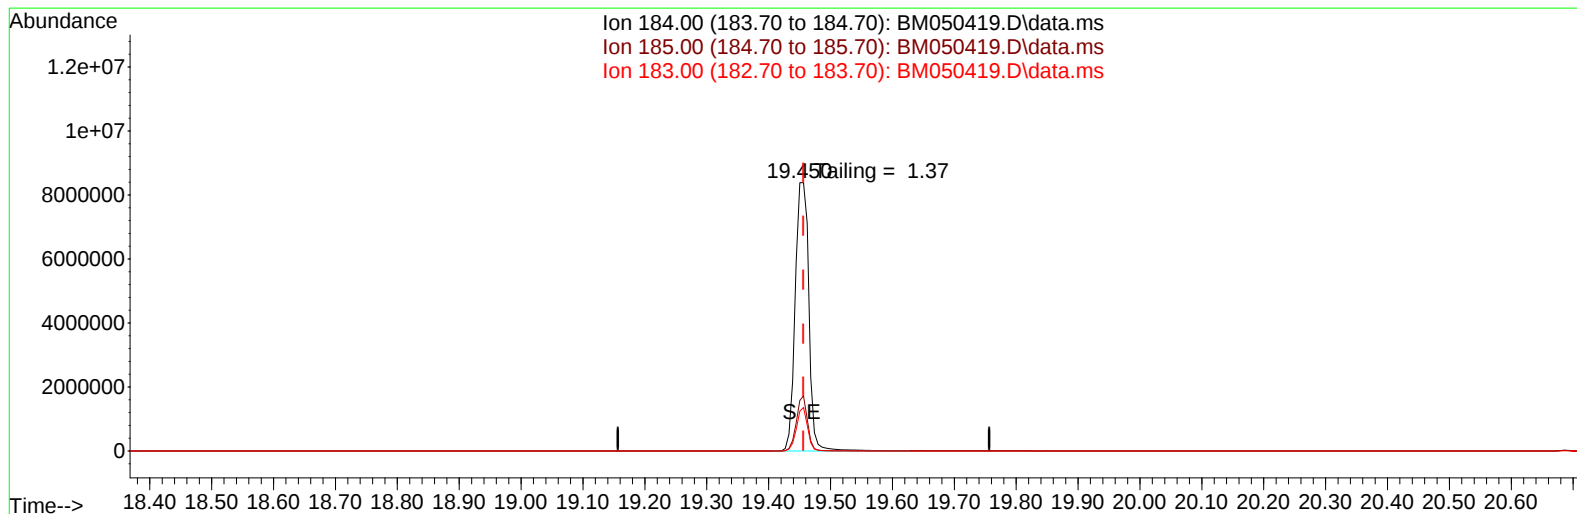

TIC: BM050419.D\data.ms

(77) Benzidine**19.450min (-0.006) 316675.61 ng****response 12931681**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	18.87#
183.00	11.30	14.88#
0.00	0.00	0.00