

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM071619\
 Data File : BM021463.D
 Acq On : 16 Jul 2019 10:05
 Operator : HP/JU
 Sample : K3760-02
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DB8X2

Quant Time: Jul 16 11:52:07 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM070819MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jul 12 05:46:23 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.73	152	175929	20.00	ng/ul	0.00
18) Naphthalene-d8	10.51	136	729237	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.37	164	449563	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.12	188	1006430	20.00	ng/ul	0.00
77) Chrysene-d12	21.31	240	838586	20.00	ng/ul	0.00
85) Perylene-d12	23.57	264	921717	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.26	96	22145	6.20	ng/uL	0.00
5) Phenol-d5	6.90	99	91948	6.72	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.07	67	252975	31.19	ng/ul	0.00
9) 2-Chlorophenol-d4	7.26	132	297440	25.26	ng/ul	0.00
13) 4-Methylphenol-d8	8.43	113	186523	17.12	ng/ul	0.00
19) Nitrobenzene-d5	8.89	128	189269	31.51	ng/ul	0.00
22) 2-Nitrophenol-d4	9.60	143	208012	30.62	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.14	165	378154	27.91	ng/ul	0.00
29) 4-Chloroaniline-d4	10.68	131	31626	2.58	ng/ul	0.01
43) Dimethylphthalate-d6	13.79	166	1313738	33.37	ng/ul	0.00
46) Acenaphthylene-d8	14.06	160	1517811	30.70	ng/ul	0.00
51) 4-Nitrophenol-d4	14.62	143	17682	2.83	ng/ul	0.02
57) Fluorene-d10	15.37	176	1161590	33.05	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.50	200	140311	20.74	ng/ul	0.00
70) Anthracene-d10	17.22	188	1855190	35.49	ng/ul	0.00
78) Pyrene-d10	19.52	212	1934418	42.03	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.43	264	1906650	35.97	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.83	163	138787	3.785	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM071619\
Data File : BM021463.D
Acq On : 16 Jul 2019 10:05
Operator : HP/JU
Sample : K3760-02
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DB8X2

Quant Time: Jul 16 11:52:07 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM070819MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jul 12 05:46:23 2019
Response via : Initial Calibration

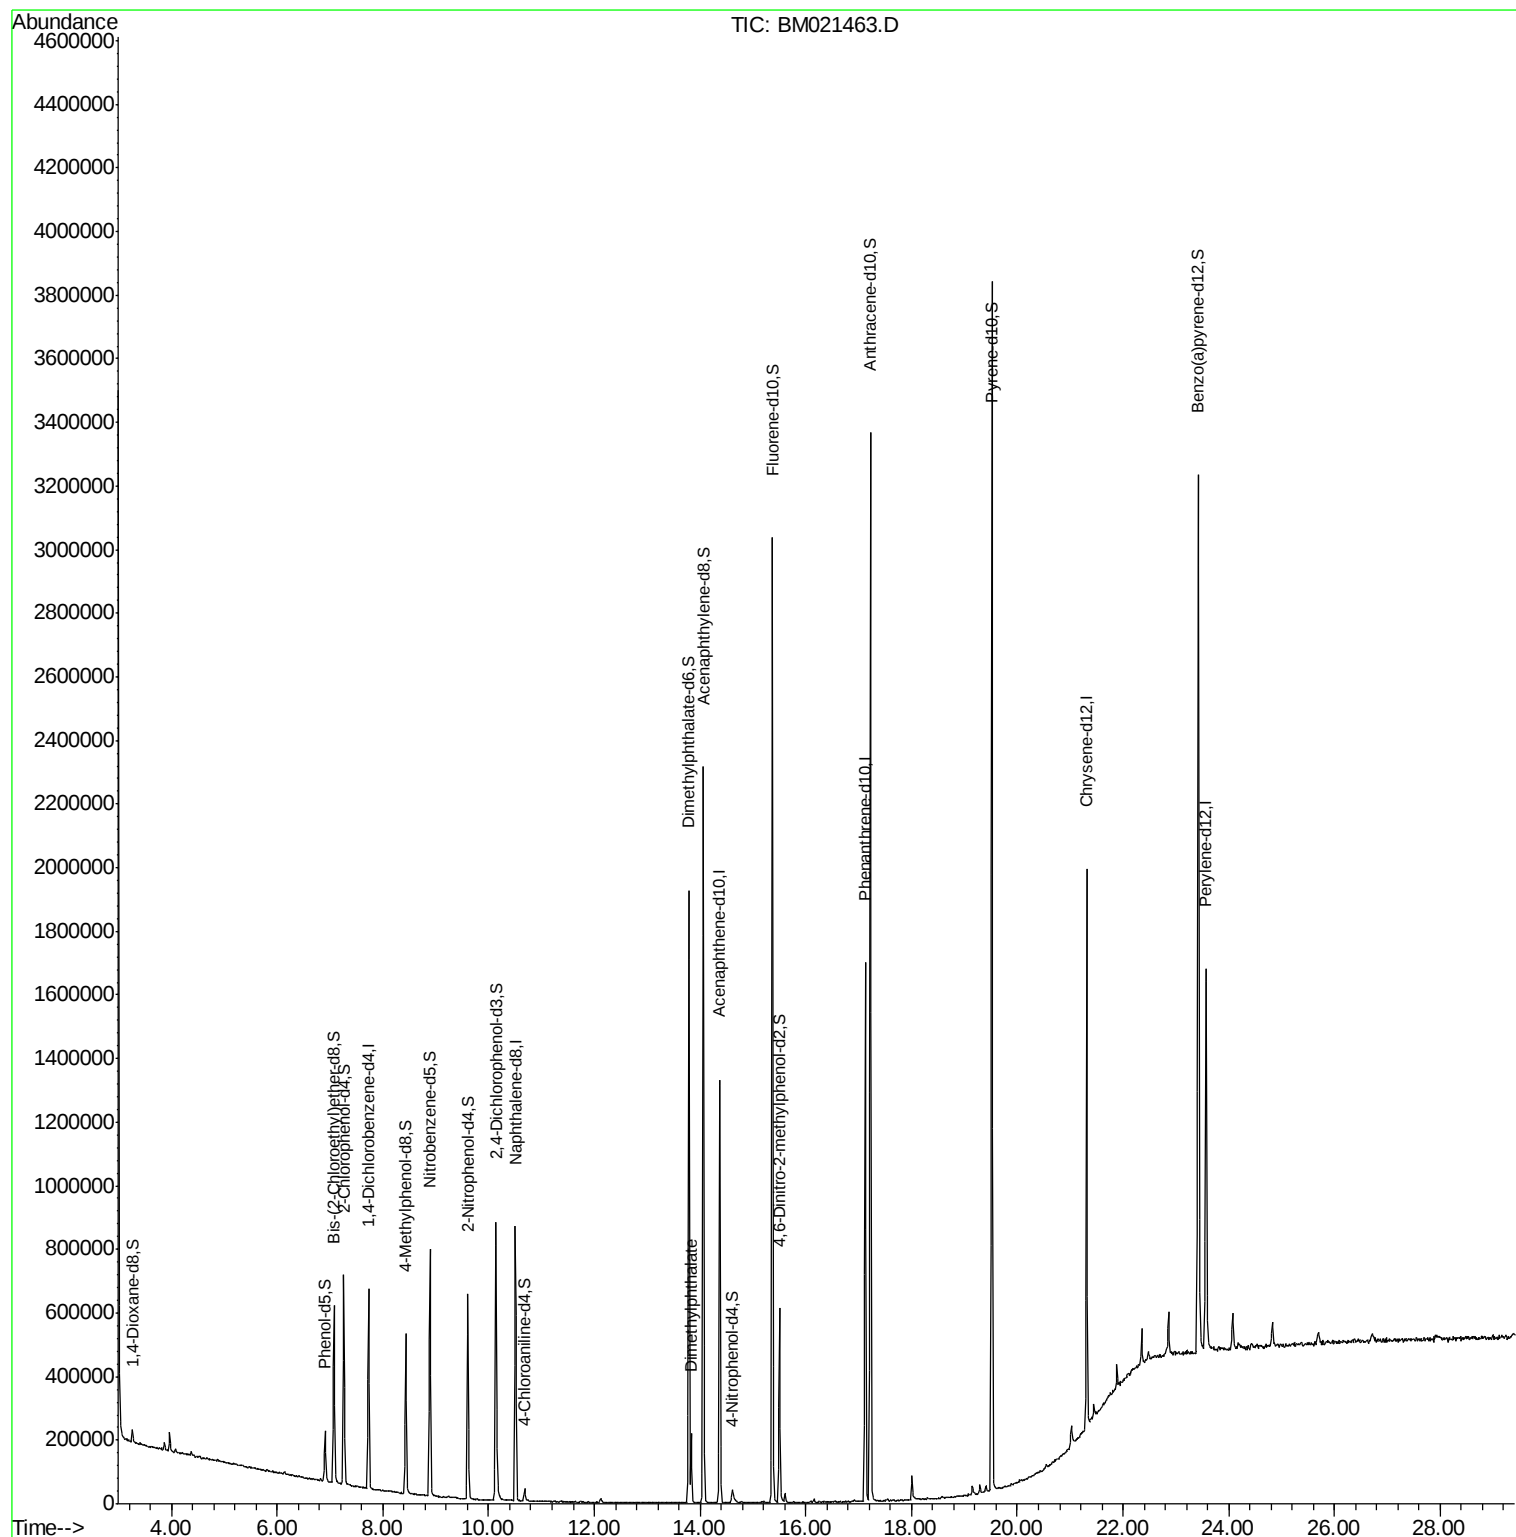

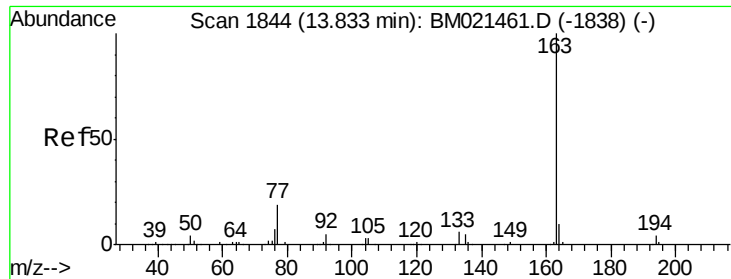

#44

Dimethylphthalate

Concen: 3.785 ng/ul

RT: 13.83 min Scan# 1844

Delta R.T. -0.01 min

Lab File: BM021463.D

Acq: 16 Jul 2019 10:05

Instrument :

BNA_M

ClientSampleId :

DB8X2


Tot Ion:163 Resp: 138787

Ion Ratio Lower Upper

163 100

194 4.0 3.6 5.4

164 9.7 8.3 12.5

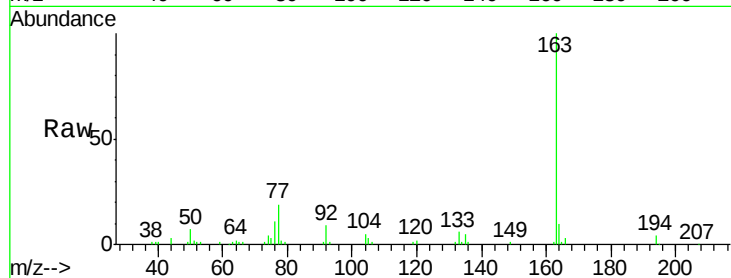

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

