

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM071619\
 Data File : BM021481.D
 Acq On : 16 Jul 2019 23:29
 Operator : HP/JU
 Sample : K3787-03
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0C91

Quant Time: Jul 17 01:24:02 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM070819MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jul 12 05:46:23 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.72	152	172983	20.00	ng/ul	-0.01
18) Naphthalene-d8	10.51	136	676374	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.37	164	388340	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.12	188	883376	20.00	ng/ul	0.00
77) Chrysene-d12	21.31	240	863432	20.00	ng/ul	0.00
85) Perylene-d12	23.57	264	1018331	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.26	96	21240	6.05	ng/uL	0.00
5) Phenol-d5	6.90	99	83679	6.22	ng/ul	-0.01
7) Bis-(2-Chloroethyl)ether-d	7.07	67	229917	28.83	ng/ul	0.00
9) 2-Chlorophenol-d4	7.26	132	268772	23.22	ng/ul	-0.01
13) 4-Methylphenol-d8	8.43	113	163396	15.25	ng/ul	0.00
19) Nitrobenzene-d5	8.89	128	167666	30.09	ng/ul	-0.01
22) 2-Nitrophenol-d4	9.60	143	181381	28.79	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.13	165	327908	26.10	ng/ul	-0.01
29) 4-Chloroaniline-d4	10.67	131	28527	2.51	ng/ul	0.00
43) Dimethylphthalate-d6	13.79	166	1062457	31.24	ng/ul	0.00
46) Acenaphthylene-d8	14.06	160	1245208	29.16	ng/ul	0.00
51) 4-Nitrophenol-d4	14.61	143	14346	2.66	ng/ul	0.01
57) Fluorene-d10	15.36	176	939251	30.94	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.50	200	111305	18.74	ng/ul	0.00
70) Anthracene-d10	17.22	188	1497420	32.63	ng/ul	0.00
78) Pyrene-d10	19.52	212	1697663	35.83	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.43	264	1955970	33.40	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.83	163	95075	3.002	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM071619\
Data File : BM021481.D
Acq On : 16 Jul 2019 23:29
Operator : HP/JU
Sample : K3787-03
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0C91

Quant Time: Jul 17 01:24:02 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM070819MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jul 12 05:46:23 2019
Response via : Initial Calibration

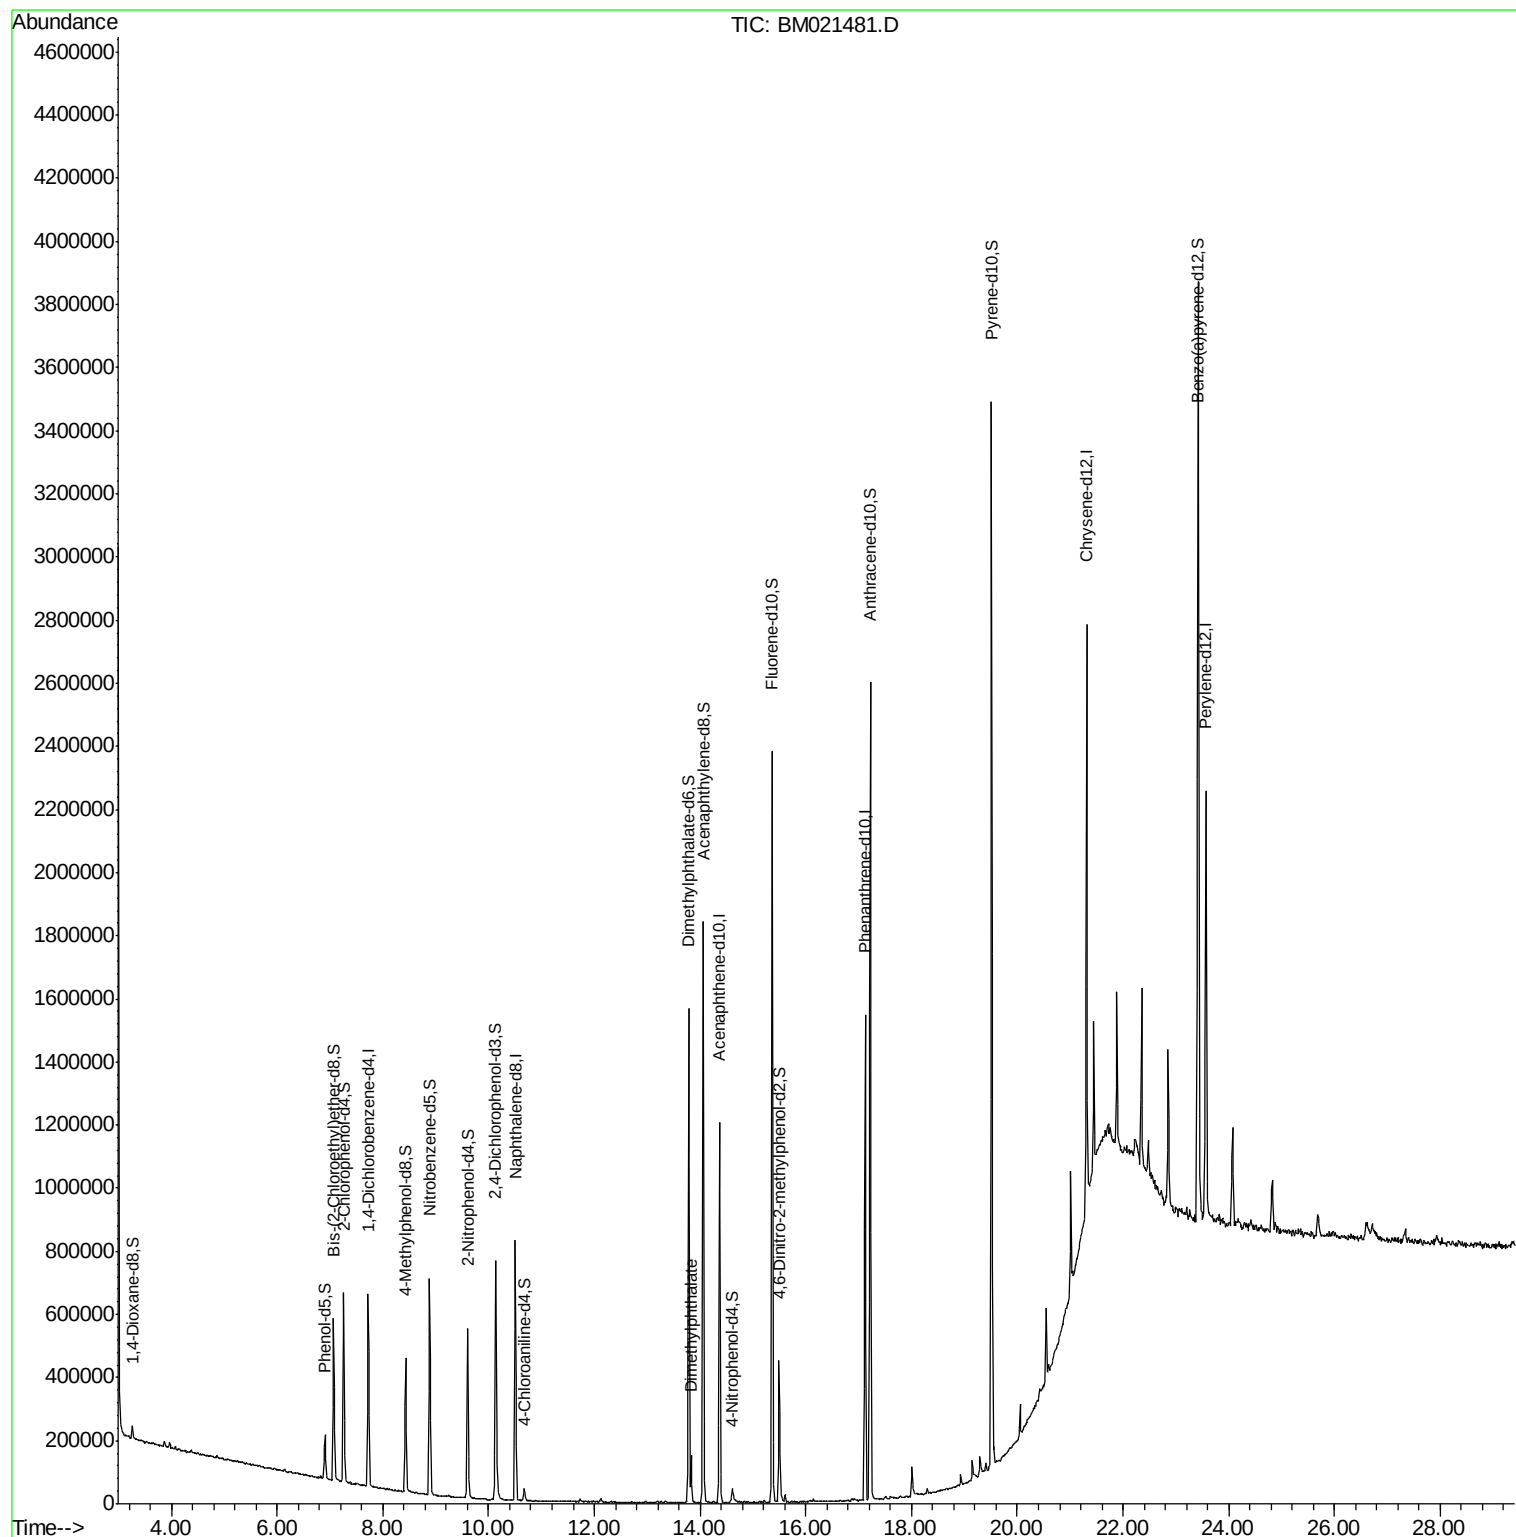

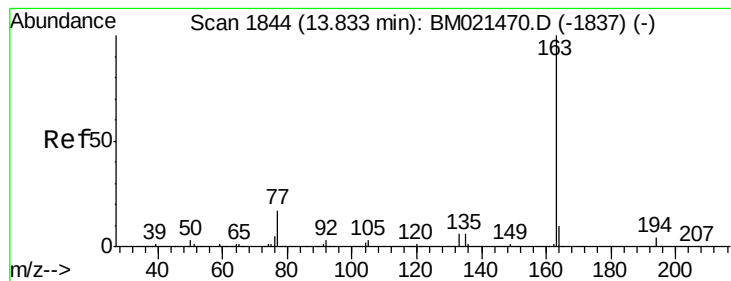

#44

Dimethylphthalate

Concen: 3.002 ng/ul

RT: 13.83 min Scan# 1844

Delta R.T. -0.01 min

Lab File: BM021481.D

Acq: 16 Jul 2019 23:29

Instrument :

BNA_M

ClientSampleId :

C0C91


Tot Ion:163 Resp: 95075

Ion Ratio Lower Upper

163 100

194 4.4 3.6 5.4

164 9.9 8.3 12.5

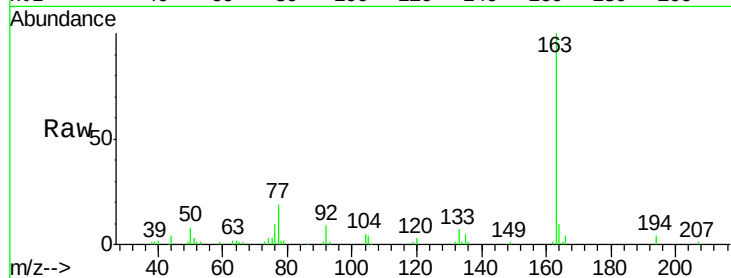

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

