

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM071719\
 Data File : BM021501.D
 Acq On : 17 Jul 2019 22:16
 Operator : HP/JU
 Sample : K3772-12
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Jul 18 02:37:49 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM070819MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jul 12 05:46:23 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.72	152	190744	20.00	ng/ul	-0.01
18) Naphthalene-d8	10.50	136	762531	20.00	ng/ul	-0.01
35) Acenaphthene-d10	14.36	164	426068	20.00	ng/ul	-0.01
61) Phenanthrene-d10	17.12	188	971870	20.00	ng/ul	-0.01
77) Chrysene-d12	21.30	240	956101	20.00	ng/ul	-0.01
85) Perylene-d12	23.56	264	1124776	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.26	96	23334	6.02	ng/uL	0.00
5) Phenol-d5	6.90	99	109467	7.38	ng/ul	-0.01
7) Bis-(2-Chloroethyl)ether-d	7.06	67	251669	28.62	ng/ul	-0.01
9) 2-Chlorophenol-d4	7.26	132	306421	24.00	ng/ul	-0.01
13) 4-Methylphenol-d8	8.43	113	188853	15.99	ng/ul	-0.01
19) Nitrobenzene-d5	8.89	128	180622	28.76	ng/ul	-0.01
22) 2-Nitrophenol-d4	9.60	143	203150	28.60	ng/ul	-0.01
26) 2,4-Dichlorophenol-d3	10.13	165	376952	26.61	ng/ul	-0.02
29) 4-Chloroaniline-d4	10.67	131	27818	2.17	ng/ul	0.00
43) Dimethylphthalate-d6	13.78	166	1187325	31.82	ng/ul	-0.01
46) Acenaphthylene-d8	14.06	160	1359929	29.02	ng/ul	-0.01
51) 4-Nitrophenol-d4	14.60	143	22373	3.78	ng/ul	0.00
57) Fluorene-d10	15.36	176	1023423	30.73	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.50	200	132555	20.29	ng/ul	0.00
70) Anthracene-d10	17.22	188	1565225	31.01	ng/ul	-0.01
78) Pyrene-d10	19.51	212	1813235	34.56	ng/ul	-0.01
89) Benzo(a)pyrene-d12	23.42	264	2074068	32.06	ng/ul	-0.02


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.83	163	115810	3.333	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM071719\
Data File : BM021501.D
Acq On : 17 Jul 2019 22:16
Operator : HP/JU
Sample : K3772-12
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Jul 18 02:37:49 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM070819MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jul 12 05:46:23 2019
Response via : Initial Calibration

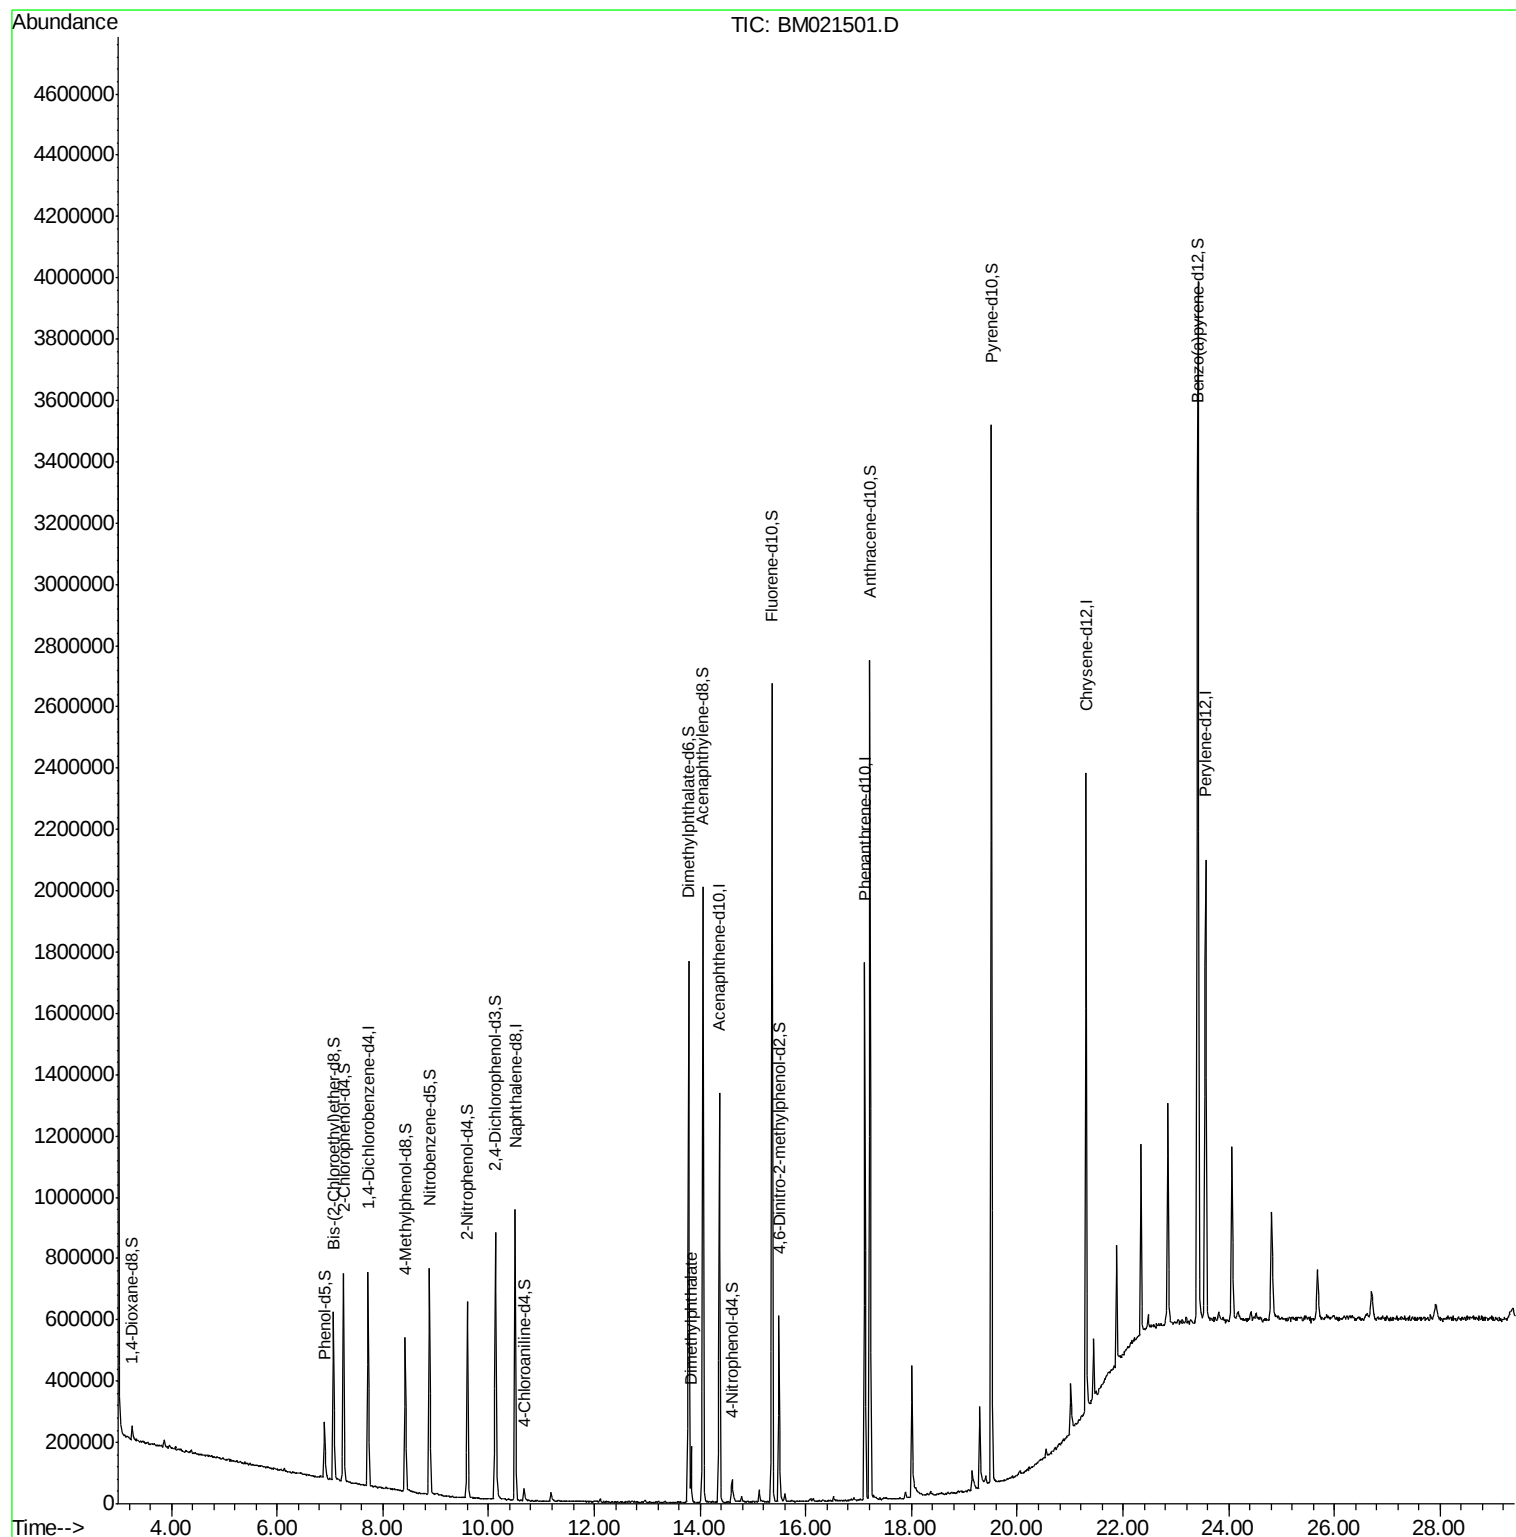

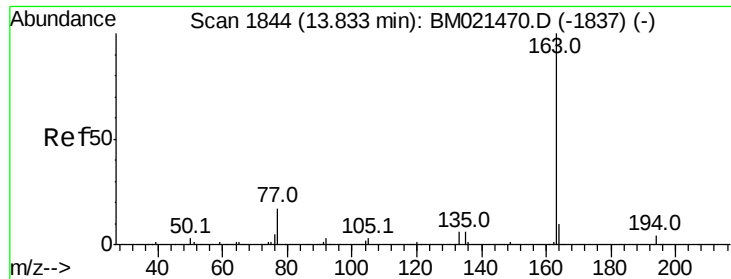

#44

Dimethylphthalate

Concen: 3.333 ng/ul

RT: 13.83 min Scan# 1843

Delta R.T. -0.01 min

Lab File: BM021501.D

Acq: 17 Jul 2019 22:16

Instrument :

BNA_M

ClientSampleId :


Tot Ion:163 Resp: 115810

Ion Ratio Lower Upper

163 100

194 4.2 3.6 5.4

164 10.5 8.3 12.5

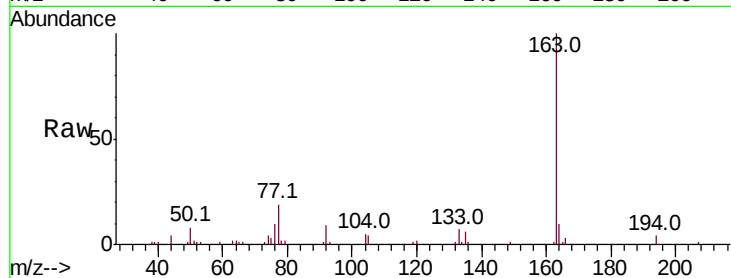

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

