

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM071719\
 Data File : BM021504.D
 Acq On : 18 Jul 2019 00:06
 Operator : HP/JU
 Sample : K3772-15
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Jul 18 02:38:05 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM070819MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jul 12 05:46:23 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.72	152	175773	20.00	ng/ul	-0.01
18) Naphthalene-d8	10.50	136	691021	20.00	ng/ul	-0.01
35) Acenaphthene-d10	14.36	164	395722	20.00	ng/ul	-0.01
61) Phenanthrene-d10	17.12	188	900632	20.00	ng/ul	-0.01
77) Chrysene-d12	21.30	240	866431	20.00	ng/ul	-0.01
85) Perylene-d12	23.56	264	1012087	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.26	96	25119	7.04	ng/uL	0.00
5) Phenol-d5	6.90	99	90941	6.65	ng/ul	-0.01
7) Bis-(2-Chloroethyl)ether-d	7.06	67	221345	27.31	ng/ul	-0.01
9) 2-Chlorophenol-d4	7.26	132	269441	22.91	ng/ul	-0.01
13) 4-Methylphenol-d8	8.43	113	171704	15.77	ng/ul	-0.01
19) Nitrobenzene-d5	8.89	128	161703	28.41	ng/ul	-0.01
22) 2-Nitrophenol-d4	9.60	143	176898	27.48	ng/ul	-0.01
26) 2,4-Dichlorophenol-d3	10.13	165	330199	25.72	ng/ul	-0.01
29) 4-Chloroaniline-d4	10.67	131	35320	3.04	ng/ul	0.00
43) Dimethylphthalate-d6	13.78	166	1077312	31.08	ng/ul	-0.01
46) Acenaphthylene-d8	14.06	160	1229556	28.25	ng/ul	-0.01
51) 4-Nitrophenol-d4	14.60	143	20327	3.70	ng/ul	0.00
57) Fluorene-d10	15.36	176	937092	30.29	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.50	200	119940	19.81	ng/ul	0.00
70) Anthracene-d10	17.22	188	1481695	31.67	ng/ul	-0.01
78) Pyrene-d10	19.52	212	1659079	34.89	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.41	264	1871328	32.15	ng/ul	-0.02


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.83	163	138156	4.281	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM071719\
Data File : BM021504.D
Acq On : 18 Jul 2019 00:06
Operator : HP/JU
Sample : K3772-15
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Jul 18 02:38:05 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM070819MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jul 12 05:46:23 2019
Response via : Initial Calibration

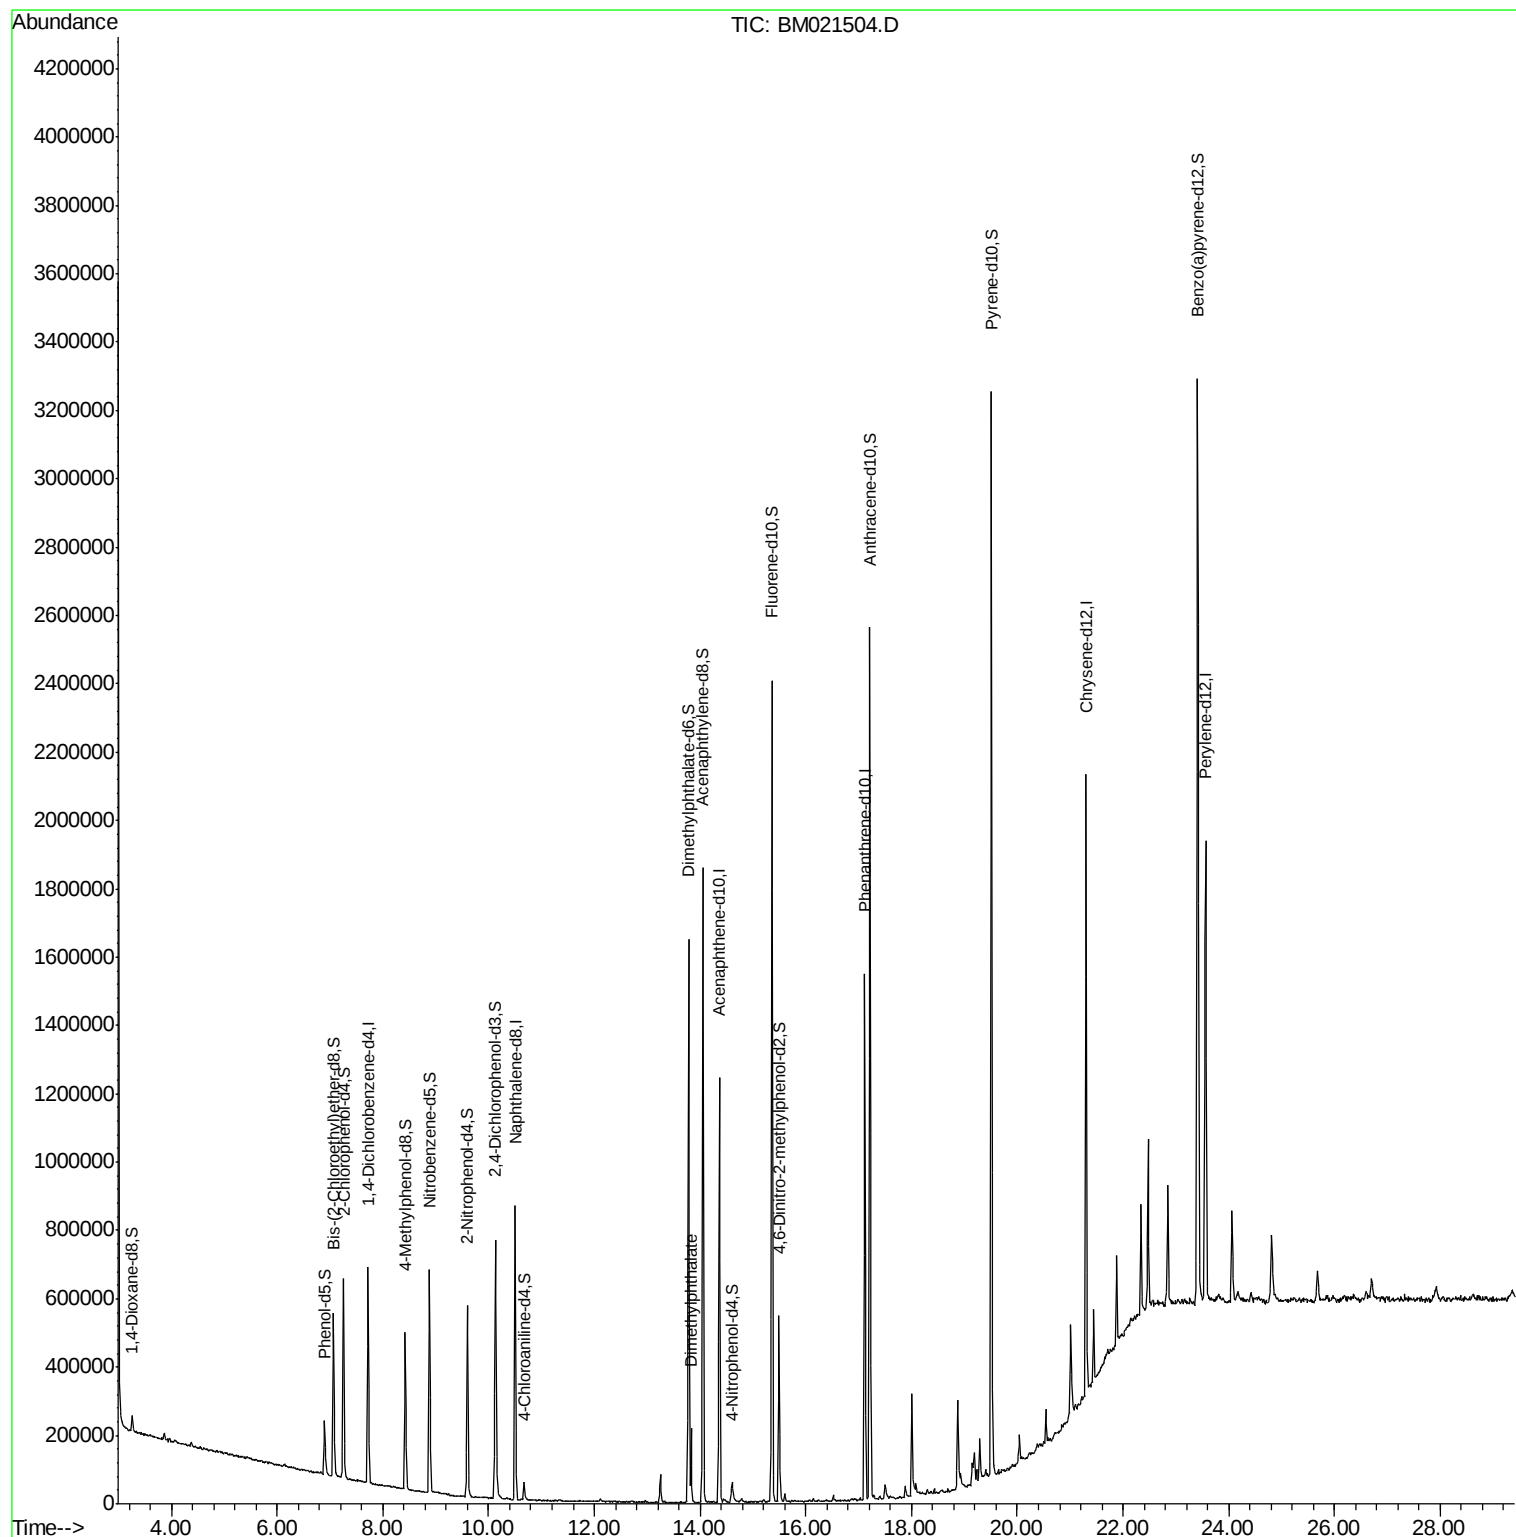

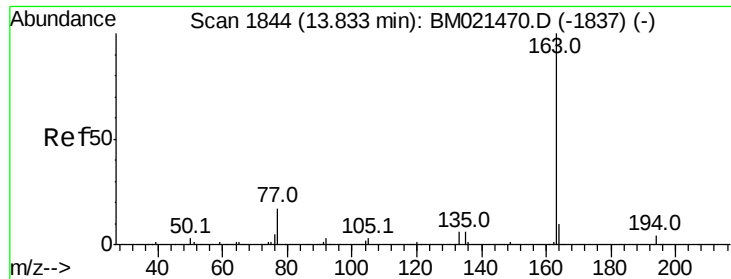

#44

Dimethylphthalate

Concen: 4.281 ng/ul

RT: 13.83 min Scan# 1843

Delta R.T. -0.01 min

Lab File: BM021504.D

Acq: 18 Jul 2019 00:06

Instrument :

BNA_M

ClientSampleId :



Tot Ion:163 Resp: 138156

Ion Ratio Lower Upper

163 100

194 3.9 3.6 5.4

164 10.1 8.3 12.5

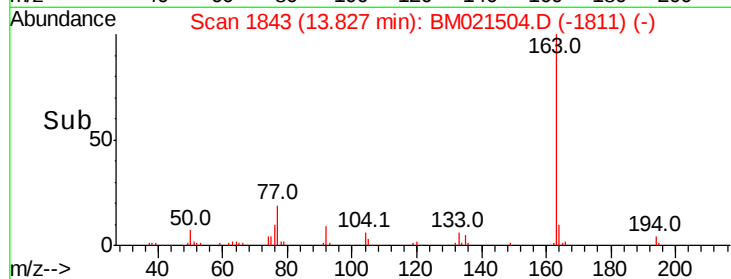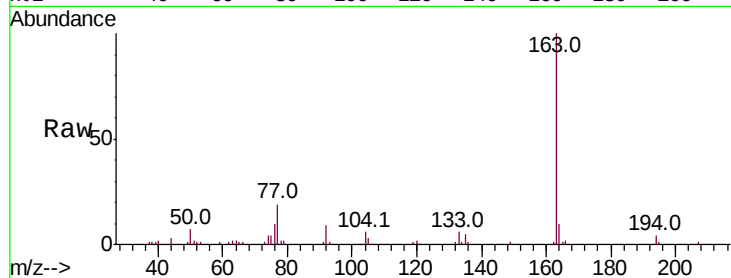

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

