

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM071719\
 Data File : BM021490.D
 Acq On : 17 Jul 2019 10:57
 Operator : HP/JU
 Sample : K3772-24MSD
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A52M0MSD

Manual Integrations
 APPROVED

mohammad
 7/19/2019 4:00:39 PM

Quant Time: Jul 17 17:40:02 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM070819MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jul 12 05:46:23 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.72	152	177084	20.00	ng/ul	-0.01
18) Naphthalene-d8	10.50	136	694108	20.00	ng/ul	-0.01
35) Acenaphthene-d10	14.36	164	388941	20.00	ng/ul	-0.01
61) Phenanthrene-d10	17.12	188	863160	20.00	ng/ul	-0.01
77) Chrysene-d12	21.31	240	830825	20.00	ng/ul	0.00
85) Perylene-d12	23.56	264	977783	20.00	ng/ul	-0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.26	96	24611	6.84	ng/uL	0.00
5) Phenol-d5	6.90	99	82525	5.99	ng/ul	-0.01
7) Bis-(2-Chloroethyl)ether-d	7.07	67	233829	28.64	ng/ul	0.00
9) 2-Chlorophenol-d4	7.26	132	277301	23.40	ng/ul	-0.01
13) 4-Methylphenol-d8	8.43	113	151864	13.85	ng/ul	0.00
19) Nitrobenzene-d5	8.89	128	172930	30.25	ng/ul	-0.01
22) 2-Nitrophenol-d4	9.60	143	190989	29.54	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.13	165	347290	26.93	ng/ul	-0.01
29) 4-Chloroaniline-d4	10.67	131	12708	1.09	ng/ul	0.00
43) Dimethylphthalate-d6	13.78	166	1125261	33.03	ng/ul	-0.01
46) Acenaphthylene-d8	14.06	160	1301668	30.43	ng/ul	-0.01
51) 4-Nitrophenol-d4	14.59	143	20602m	3.82	ng/ul	0.00
57) Fluorene-d10	15.36	176	989130	32.53	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.50	200	133534	23.01	ng/ul	0.00
70) Anthracene-d10	17.22	188	1496491	33.38	ng/ul	-0.01
78) Pyrene-d10	19.52	212	1668744	36.60	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.42	264	1900908	33.80	ng/ul	-0.01

Target Compounds

					Ovalue
6) Phenol	6.92	94	89603	6.799	ng/ul 99
10) 2-Chlorophenol	7.29	128	288594	25.338	ng/ul 98
15) N-Nitroso-di-n-propylamine	8.53	70	275904	33.308	ng/ul 96
33) 4-Chloro-3-methylphenol	11.80	107	300725	27.391	ng/ul 98
44) Dimethylphthalate	13.83	163	64396	2.030	ng/ul 99
49) Acenaphthene	14.43	153	942378	34.854	ng/ul 100
52) 4-Nitrophenol	14.61	109	19618	4.879	ng/ul 90
54) 2,4-Dinitrotoluene	14.75	165	282644	31.905	ng/ul 99
68) Pentachlorophenol	16.77	266	242097	36.172	ng/ul 98
79) Pyrene	19.54	202	2206349	40.126	ng/ul 100

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM071719\
Data File : BM021490.D
Acq On : 17 Jul 2019 10:57
Operator : HP/JU
Sample : K3772-24MSD
Misc :
ALS Vial : 6 Sample Multiplier: 1




Instrument :
BNA_M
ClientSampleId :
A52M0MSD

Manual Integrations
APPROVED

mohammad
7/19/2019 4:00:39 PM

Quant Time: Jul 17 17:40:02 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM070819MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jul 12 05:46:23 2019
Response via : Initial Calibration

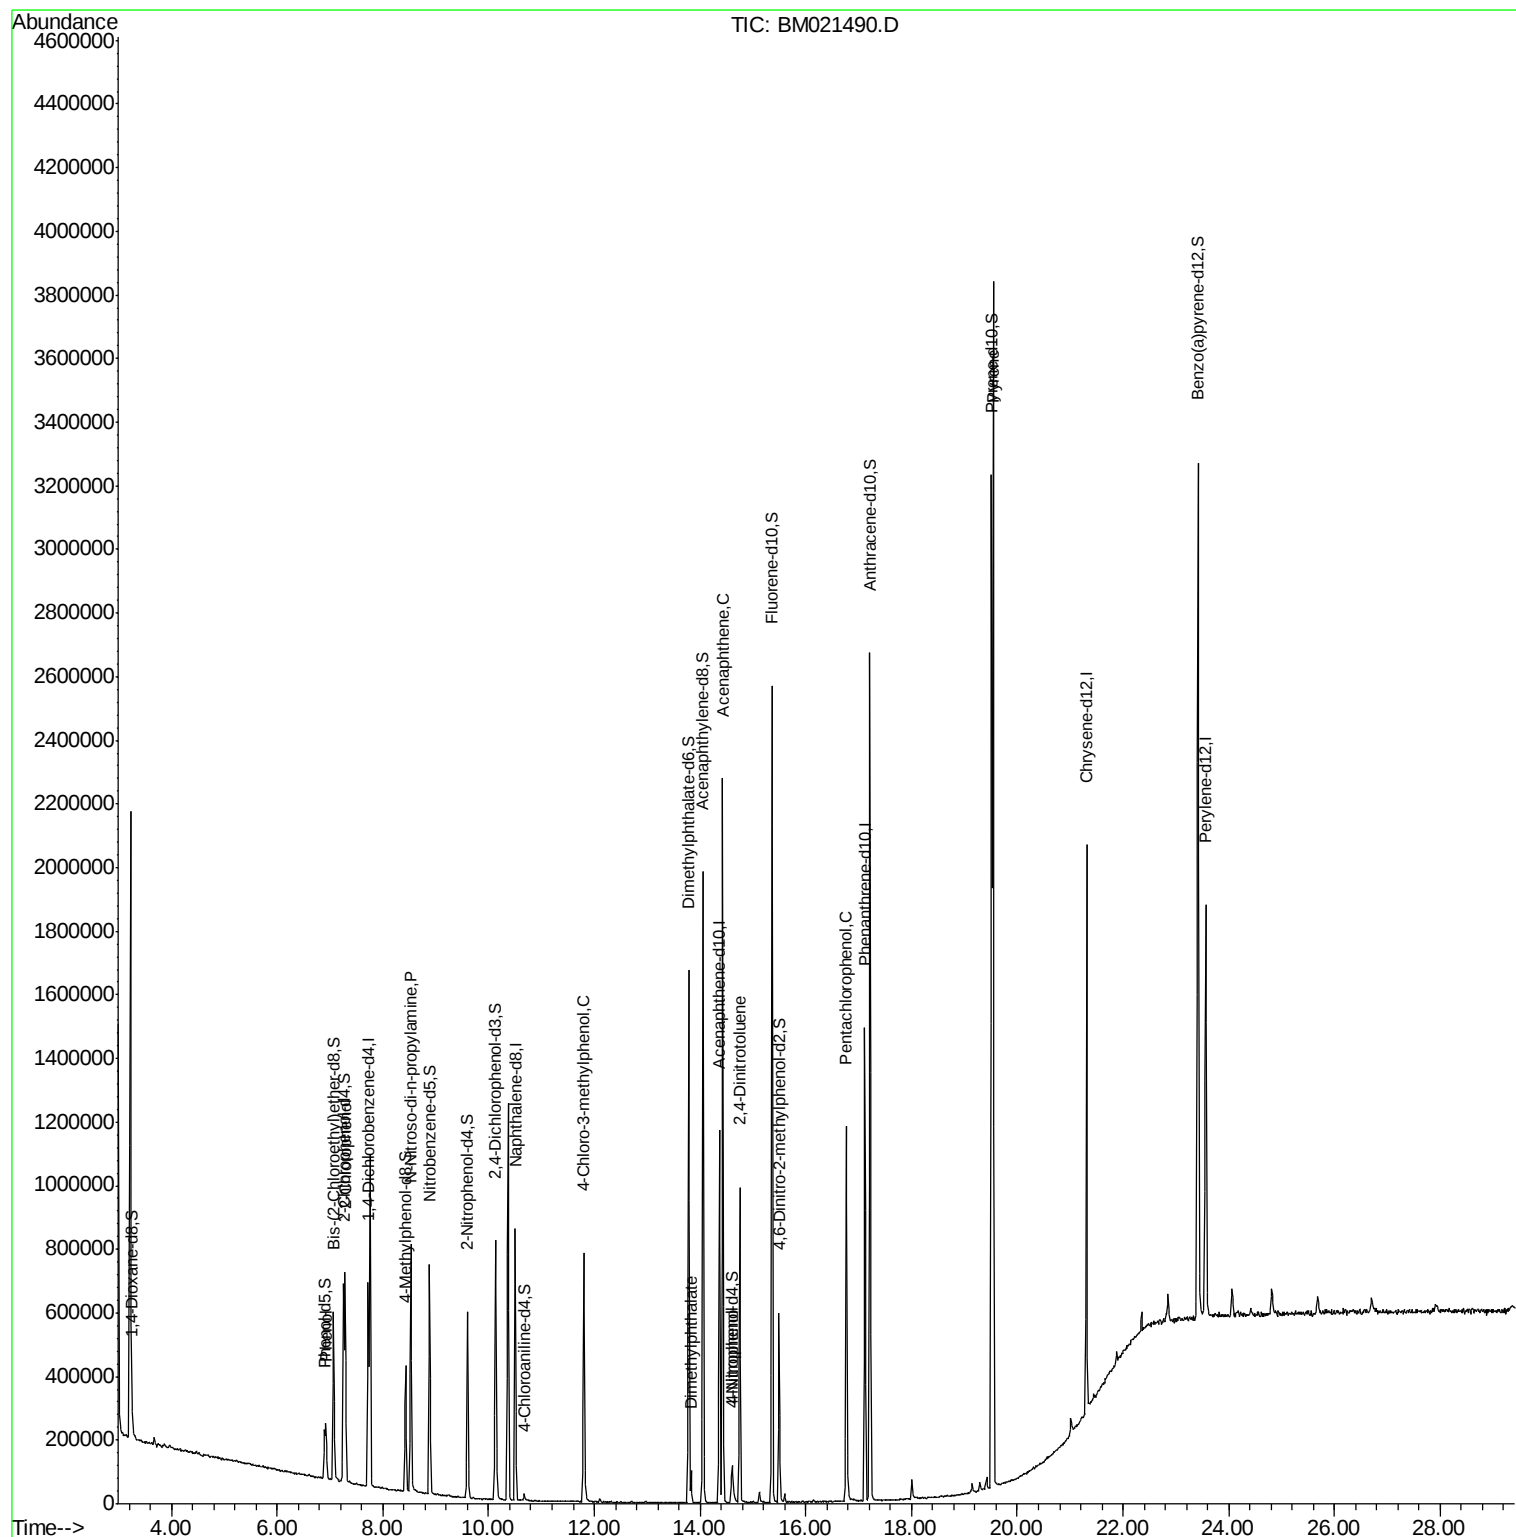

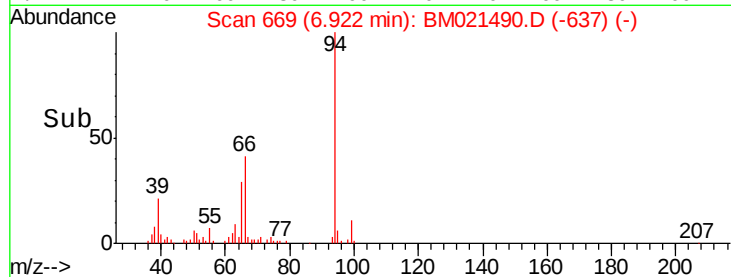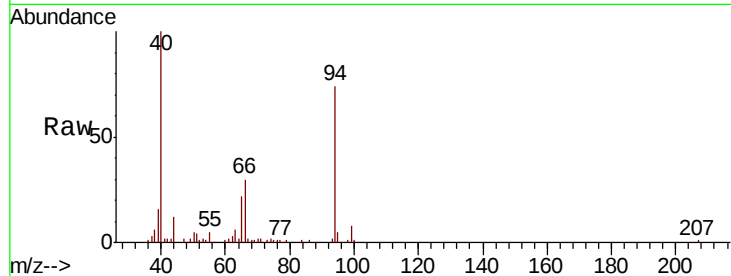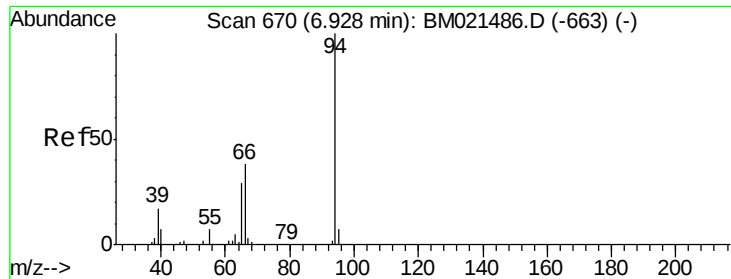

#6

Phenol

Concen: 6.799 ng/ul

RT: 6.92 min Scan# 669

Delta R.T. -0.01 min

Lab File: BM021490.D

Acq: 17 Jul 2019 10:57

Tot Ion:	94	Resp:	89603
Ion Ratio	Lower	Upper	
94	100		
65	29.2	23.0	34.6
66	40.6	31.6	47.4

Instrument :





BNA_M

ClientSampleId :

A52M0MSD

Manual Integrations
APPROVED

mohammad
7/19/2019 4:00:39 PM

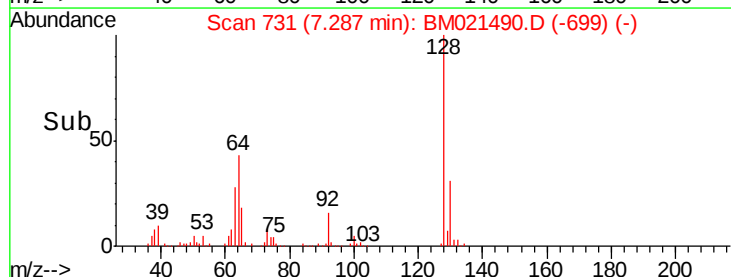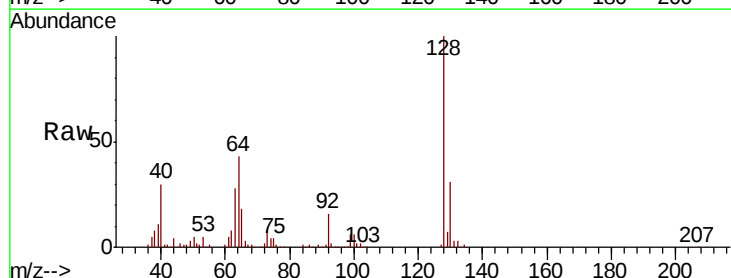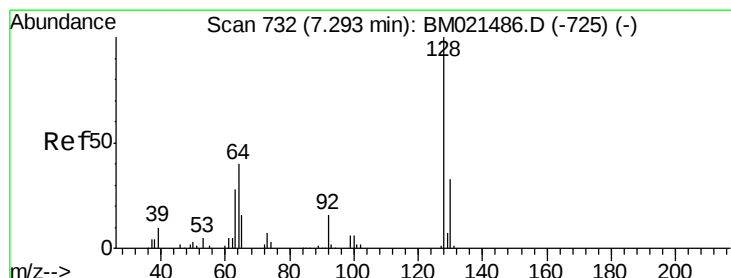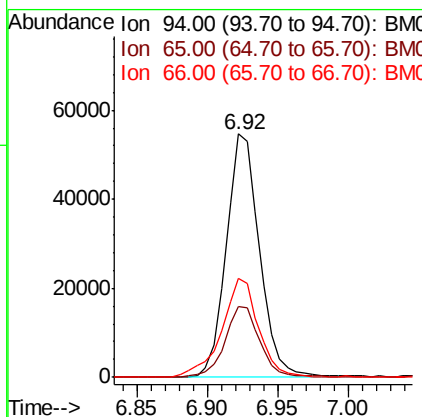

#10

2-Chlorophenol

Concen: 25.338 ng/ul


RT: 7.29 min Scan# 731




Delta R.T. -0.01 min

Lab File: BM021490.D

Acq: 17 Jul 2019 10:57

Tgt Ion:	128	Resp:	288594
Ion Ratio	Lower	Upper	
128	100		
64	42.9	34.4	51.6
130	31.0	26.9	40.3

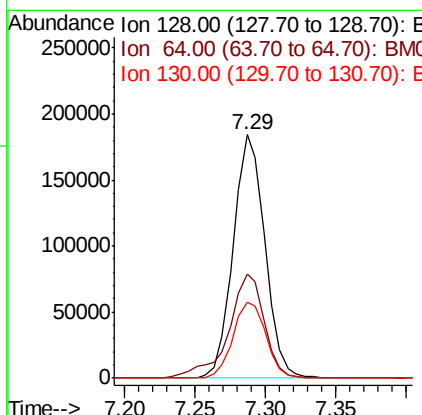

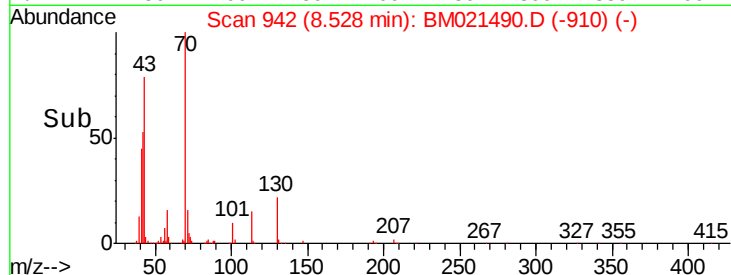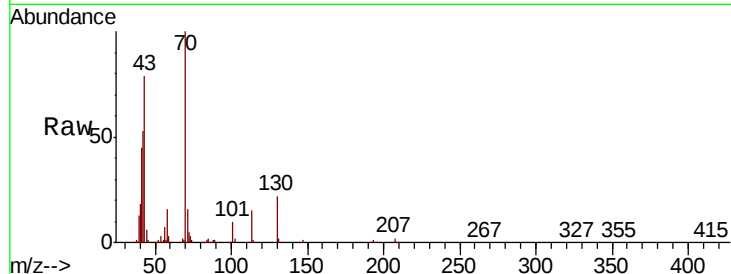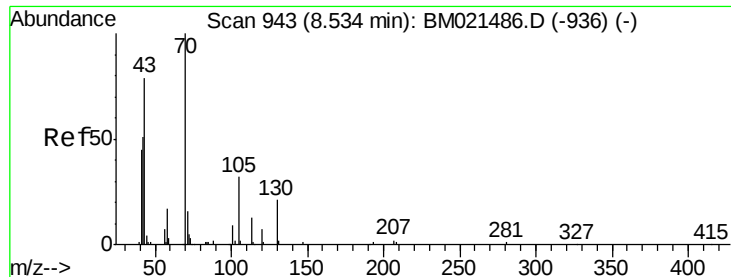





#15
N-Nitroso-di-n-propylamine
Concen: 33.308 ng/ul
RT: 8.53 min Scan# 942
Delta R.T. -0.01 min
Lab File: BM021490.D
Acq: 17 Jul 2019 10:57

Instrument :
BNA_M
ClientSampleId :
A52M0MSD

Tot Ion	Ion	Ratio	Resp	Lower	Upper
70	100				
42	53.1	39.9	59.9		
101	10.3	7.6	11.4		
130	21.9	18.5	27.7		


Manual Integrations
APPROVED


mohammad
7/19/2019 4:00:39 PM

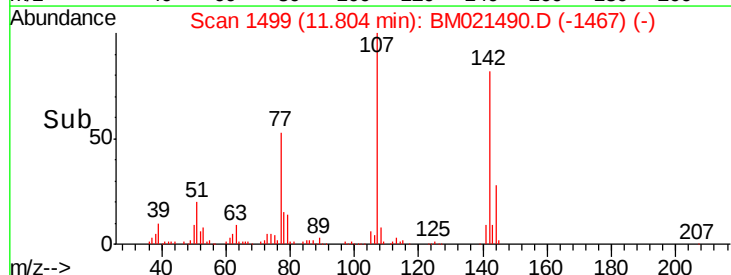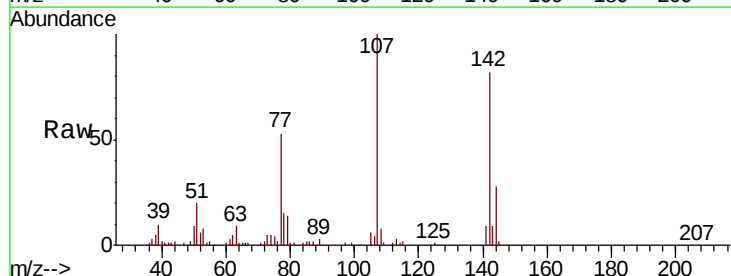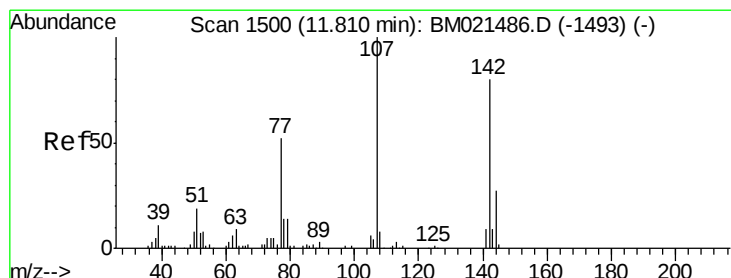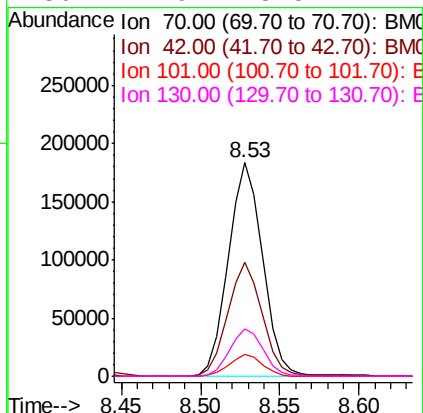

#33
4-Chloro-3-methylphenol
Concen: 27.391 ng/ul
RT: 11.80 min Scan# 1499
Delta R.T. -0.01 min
Lab File: BM021490.D
Acq: 17 Jul 2019 10:57

Tgt Ion	Ion	Ratio	Resp	Lower	Upper
107	100				
144	28.1	21.4	32.2		
142	82.1	64.7	97.1		

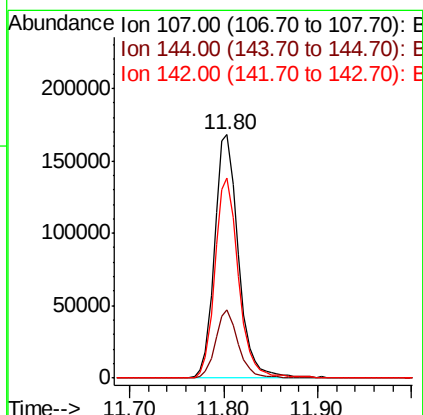

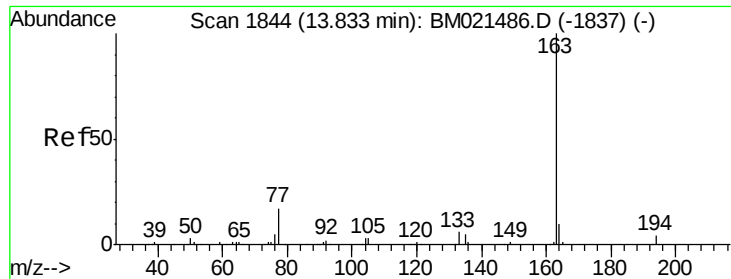


#44
Dimethylphthalate
Concen: 2.030 ng/ul
RT: 13.83 min Scan# 1843
Delta R.T. -0.01 min
Lab File: BM021490.D
Acq: 17 Jul 2019 10:57

Instrument :
BNA_M
ClientSampleId :
A52M0MSD

Tot Ion	Ratio	Lower	Upper
163	100		
194	4.1	3.6	5.4
164	10.0	8.3	12.5

Manual Integrations
APPROVED

mohammad
7/19/2019 4:00:39 PM



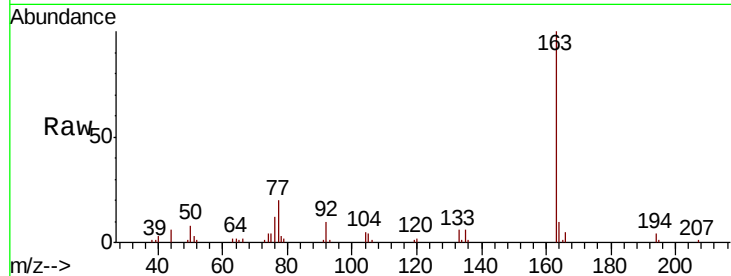


Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

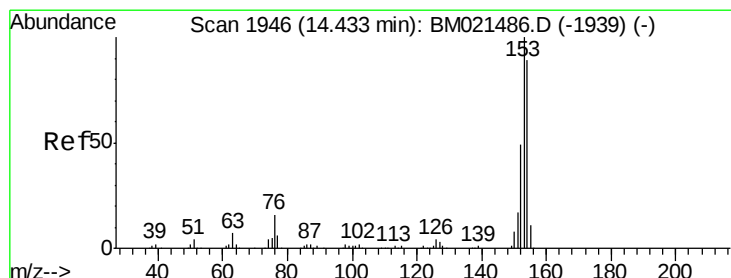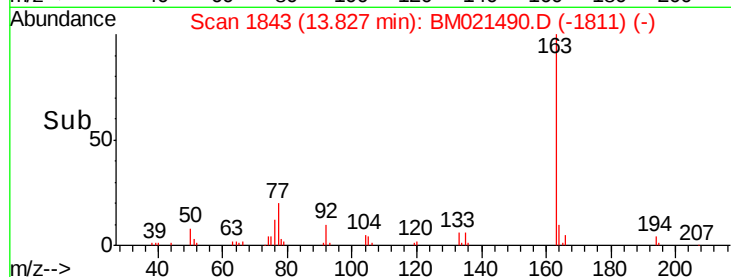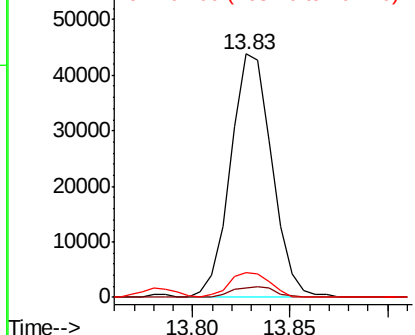

#49
Acenaphthene
Concen: 34.854 ng/ul
RT: 14.43 min Scan# 1946
Delta R.T. -0.01 min
Lab File: BM021490.D
Acq: 17 Jul 2019 10:57




Tgt Ion	Ratio	Lower	Upper
153	100		
152	47.9	38.2	57.4
154	87.8	70.0	105.0


Abundance

Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

Ion 154.00 (153.70 to 154.70): E

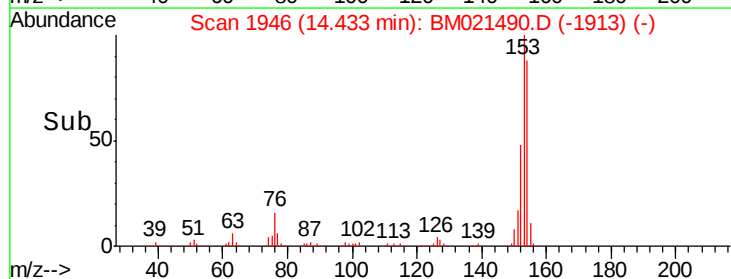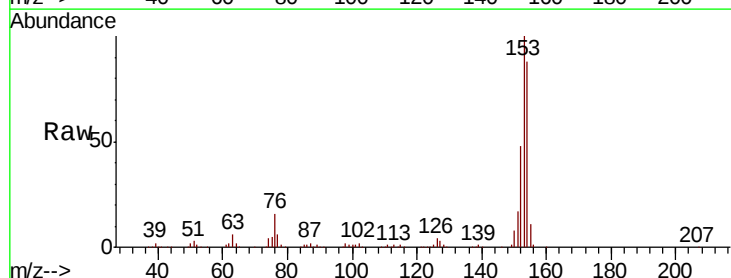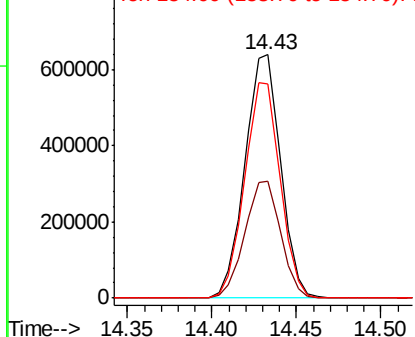

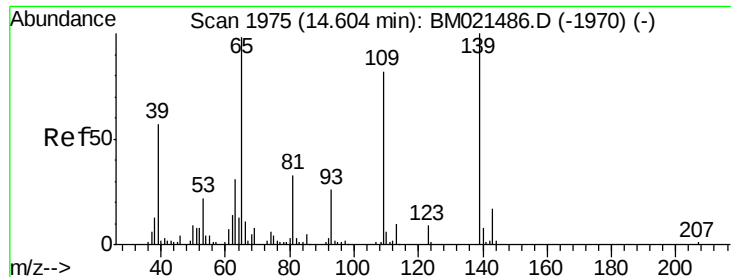





#52
4-Nitrophenol
Concen: 4.879 ng/ul
RT: 14.61 min Scan# 1976
Delta R.T. 0.00 min
Lab File: BM021490.D
Acq: 17 Jul 2019 10:57

Instrument :
BNA_M
ClientSampleId :
A52M0MSD

Tot Ion	Ratio	Lower	Upper
109	100		
139	120.7	107.6	161.4
65	136.5	101.0	151.6




Manual Integrations
APPROVED


mohammad
7/19/2019 4:00:39 PM

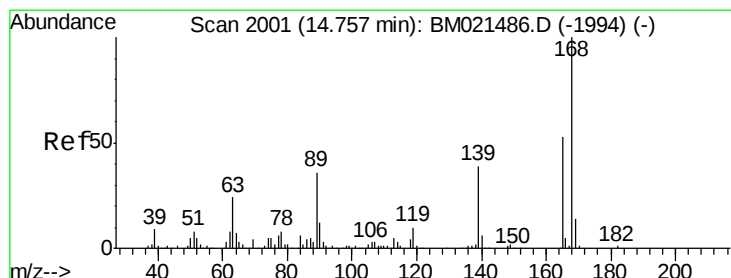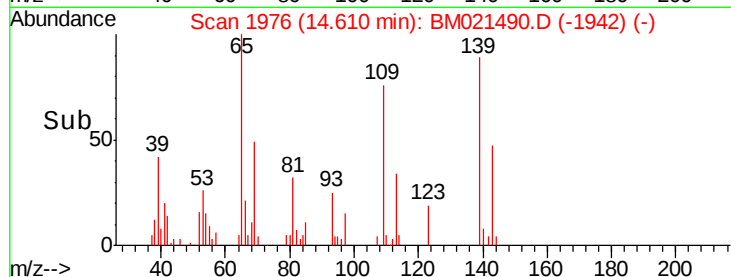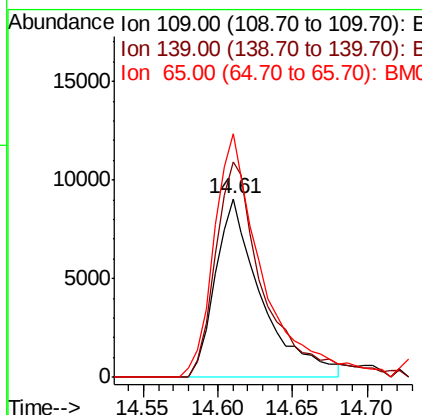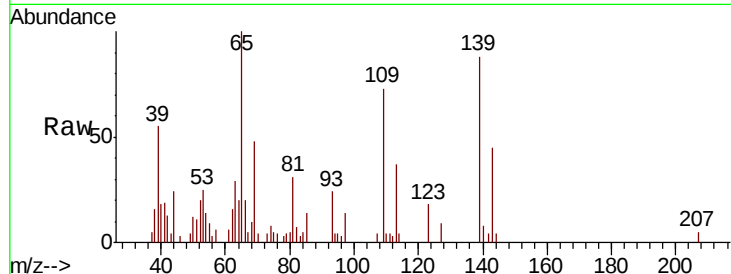

#54
2,4-Dinitrotoluene
Concen: 31.905 ng/ul
RT: 14.75 min Scan# 2000
Delta R.T. -0.01 min
Lab File: BM021490.D
Acq: 17 Jul 2019 10:57

Tgt Ion	Ratio	Lower	Upper
165	100		
63	40.5	33.1	49.7
182	3.2	2.2	3.4

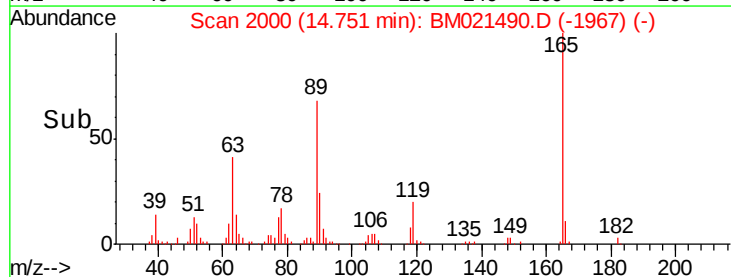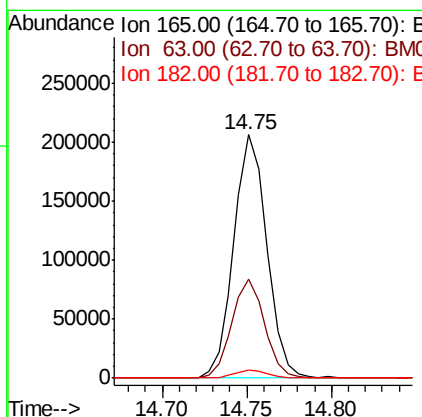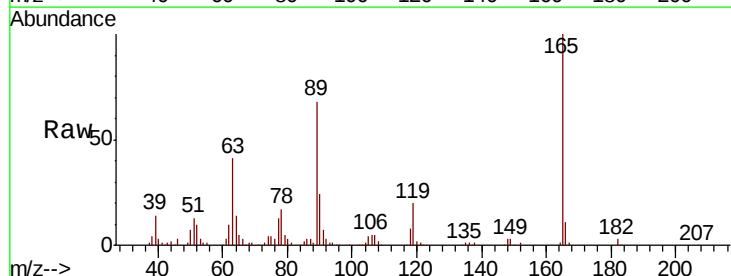

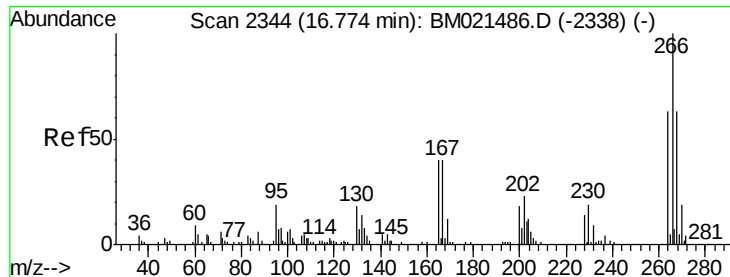


#68
 Pentachlorophenol
 Concen: 36.172 ng/ul
 RT: 16.77 min Scan# 2343
 Delta R.T. -0.01 min
 Lab File: BM021490.D
 Acq: 17 Jul 2019 10:57

Instrument :
 BNA_M
 ClientSampleId :
 A52M0MSD




Tot Ion:	266	Resp:	242097
Ion Ratio	Lower	Upper	
266	100		
264	62.8	49.2	73.8
268	64.5	50.6	76.0

Manual Integrations
 APPROVED

mohammad
 7/19/2019 4:00:39 PM

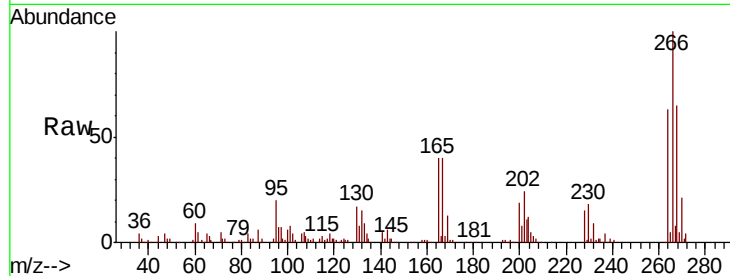

Abundance Ion 265.70 (265.40 to 266.40): E
 Ion 264.00 (263.70 to 264.70): E
 Ion 268.00 (267.70 to 268.70): E

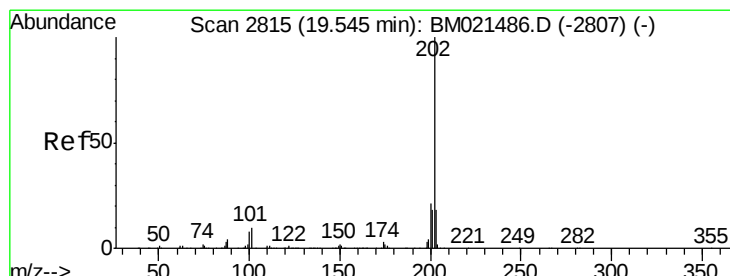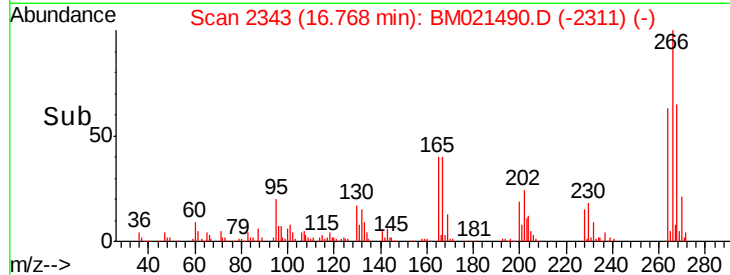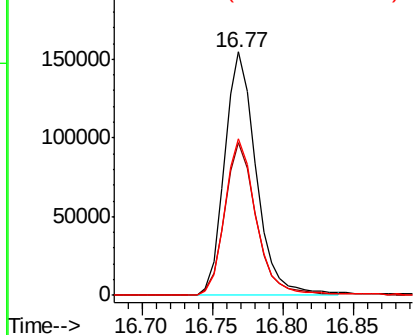

#79
 Pyrene
 Concen: 40.126 ng/ul
 RT: 19.54 min Scan# 2815
 Delta R.T. -0.01 min
 Lab File: BM021490.D
 Acq: 17 Jul 2019 10:57

Tgt Ion:	202	Resp:	2206349
Ion Ratio	Lower	Upper	
202	100		
101	9.7	7.8	11.8
100	8.0	6.4	9.6

Abundance Ion 202.00 (201.70 to 202.70): E
 Ion 101.00 (100.70 to 101.70): E
 Ion 100.00 (99.70 to 100.70): B

