

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM071719\
 Data File : BM021517.D
 Acq On : 18 Jul 2019 08:37
 Operator : HP/JU
 Sample : K3760-13
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DB8Z3

Quant Time: Jul 18 09:16:18 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM070819MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 18 02:48:00 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.72	152	189086	20.00	ng/ul	-0.01
18) Naphthalene-d8	10.50	136	748535	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.36	164	436284	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.12	188	992081	20.00	ng/ul	0.00
77) Chrysene-d12	21.30	240	965599	20.00	ng/ul	-0.01
85) Perylene-d12	23.56	264	1120565	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.26	96	14804	3.86	ng/uL	0.00
5) Phenol-d5	6.89	99	315339	21.45	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.06	67	191046	21.91	ng/ul	0.00
9) 2-Chlorophenol-d4	7.25	132	272302	21.52	ng/ul	0.00
13) 4-Methylphenol-d8	8.43	113	262033	22.38	ng/ul	0.00
19) Nitrobenzene-d5	8.88	128	131794	21.38	ng/ul	0.00
22) 2-Nitrophenol-d4	9.60	143	145654	20.89	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.13	165	289648	20.83	ng/ul	0.00
29) 4-Chloroaniline-d4	10.66	131	339608	27.01	ng/ul	0.00
43) Dimethylphthalate-d6	13.78	166	867757	22.71	ng/ul	0.00
46) Acenaphthylene-d8	14.06	160	1010477	21.06	ng/ul	0.00
51) 4-Nitrophenol-d4	14.59	143	83964	13.87	ng/ul	0.00
57) Fluorene-d10	15.36	176	761699	22.33	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.50	200	82549	12.38	ng/ul	0.00
70) Anthracene-d10	17.22	188	1156387	22.44	ng/ul	0.00
78) Pyrene-d10	19.51	212	1301660	24.56	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.41	264	1481603	22.99	ng/ul	-0.02


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.83	163	86722	2.437	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM071719\
Data File : BM021517.D
Acq On : 18 Jul 2019 08:37
Operator : HP/JU
Sample : K3760-13
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DB8Z3

Quant Time: Jul 18 09:16:18 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM070819MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 18 02:48:00 2019
Response via : Initial Calibration

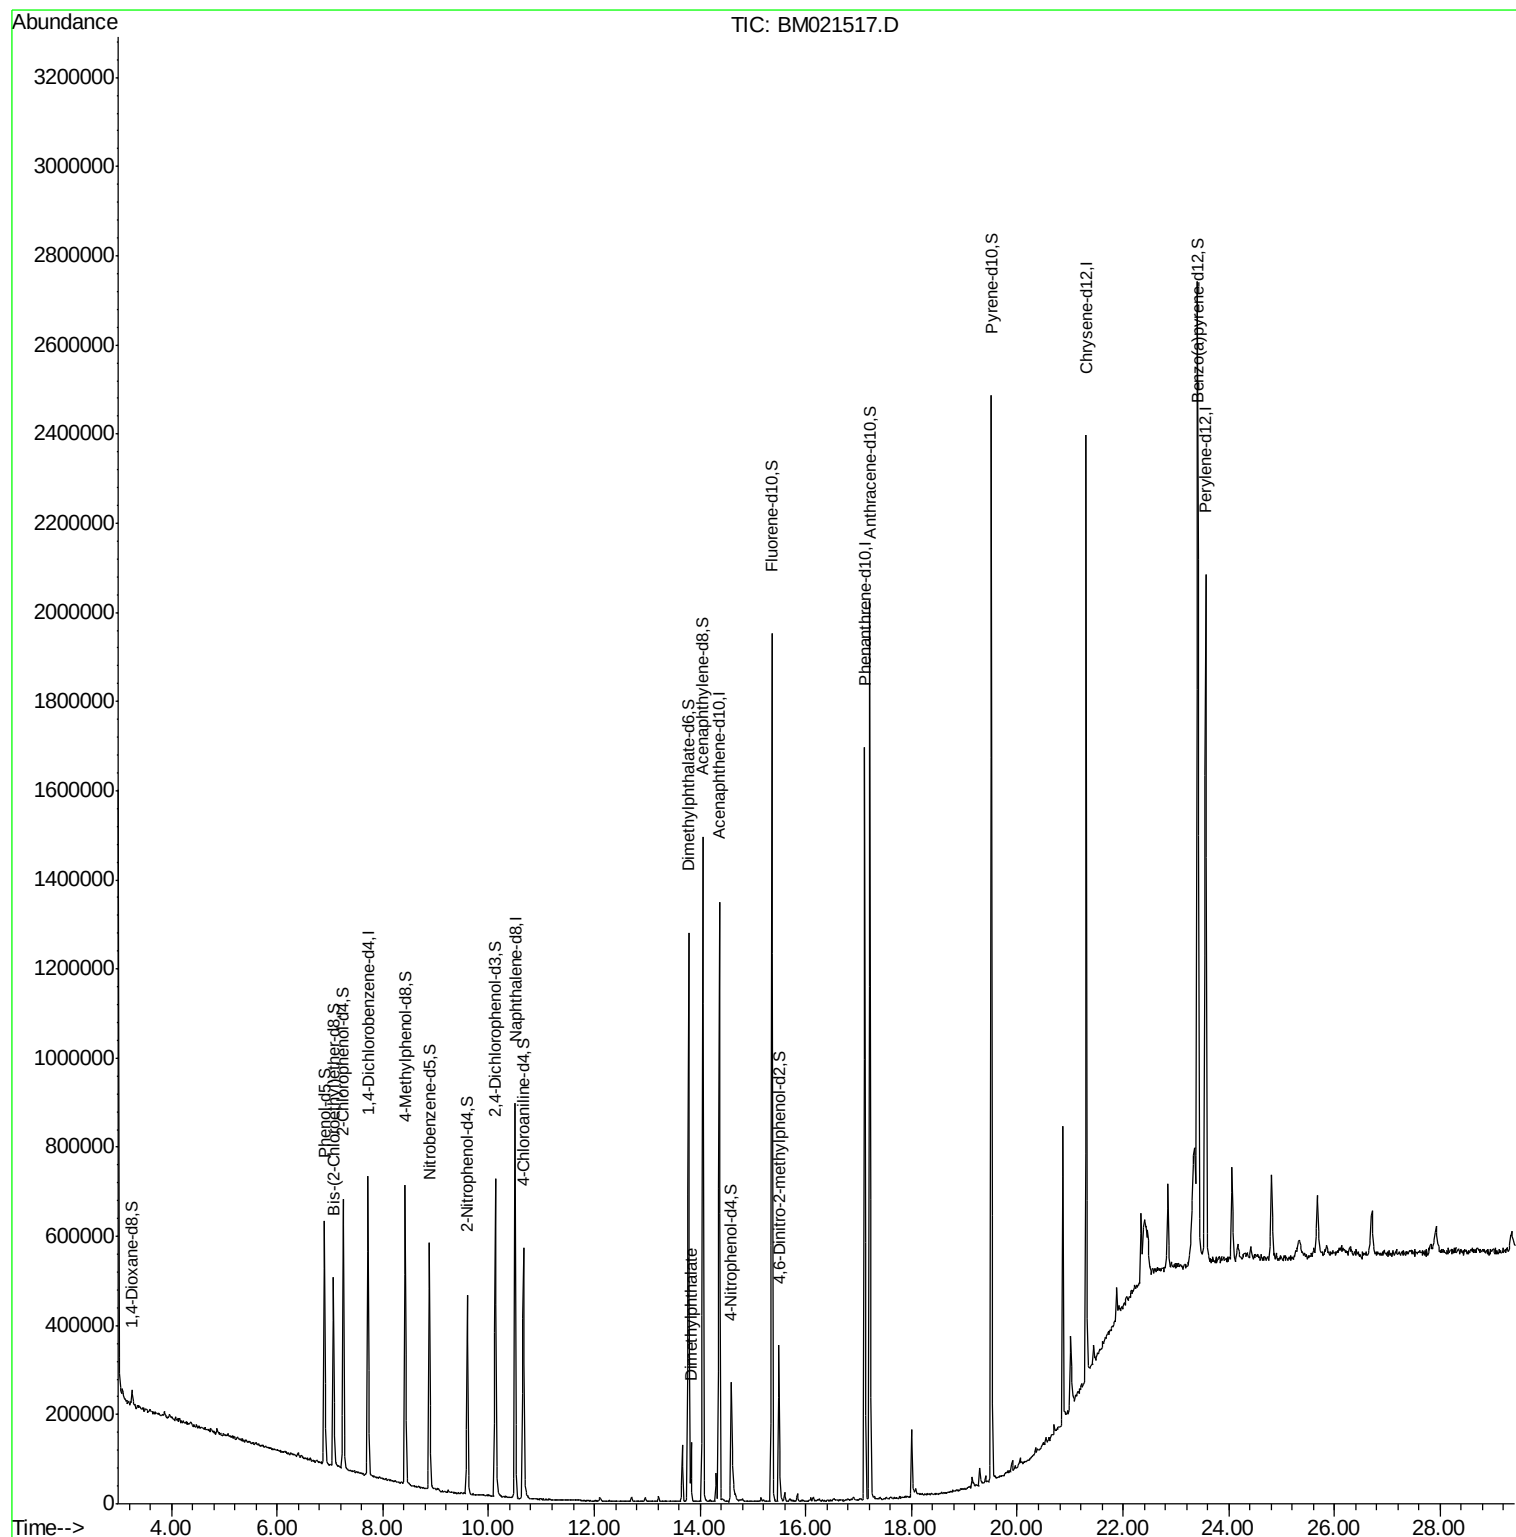

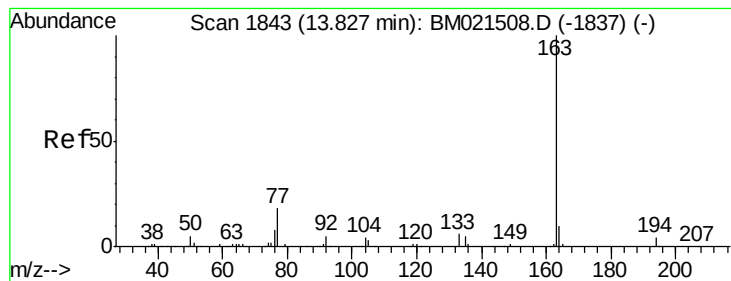

#44
 Dimethylphthalate
 Concen: 2.437 ng/ul
 RT: 13.83 min Scan# 1843
 Delta R.T. -0.01 min
 Lab File: BM021517.D
 Acq: 18 Jul 2019 08:37

Instrument :
 BNA_M
 ClientSampleId :
 DB8Z3

Tot Ion:163	Resp:	86722
Ion Ratio	Lower	Upper
163	100	
194	4.5	3.6 5.4
164	9.7	8.3 12.5

