

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM071719\
 Data File : BM021546.D
 Acq On : 19 Jul 2019 06:04
 Operator : HP/JU
 Sample : K3764-06
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A52H8

Quant Time: Jul 19 06:59:49 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM070819MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jul 19 00:39:42 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.72	152	199298	20.00	ng/ul	0.00
18) Naphthalene-d8	10.50	136	821037	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.36	164	469355	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.11	188	996291	20.00	ng/ul	0.00
77) Chrysene-d12	21.30	240	871208	20.00	ng/ul	-0.01
85) Perylene-d12	23.55	264	988121	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.25	96	23147	5.72	ng/uL	0.00
5) Phenol-d5	6.89	99	492567	31.79	ng/ul	-0.01
7) Bis-(2-Chloroethyl)ether-d	7.06	67	294390	32.04	ng/ul	0.00
9) 2-Chlorophenol-d4	7.25	132	414553	31.08	ng/ul	0.00
13) 4-Methylphenol-d8	8.42	113	416789	33.77	ng/ul	0.00
19) Nitrobenzene-d5	8.88	128	202392	29.93	ng/ul	0.00
22) 2-Nitrophenol-d4	9.59	143	216079	28.25	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.12	165	455034	29.83	ng/ul	0.00
29) 4-Chloroaniline-d4	10.65	131	544644	39.49	ng/ul	0.00
43) Dimethylphthalate-d6	13.77	166	1377706	33.52	ng/ul	0.00
46) Acenaphthylene-d8	14.05	160	1541010	29.86	ng/ul	0.00
51) 4-Nitrophenol-d4	14.58	143	128116	19.67	ng/ul	0.00
57) Fluorene-d10	15.36	176	1172724	31.96	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.49	200	120131	17.94	ng/ul	0.00
70) Anthracene-d10	17.21	188	1760121	34.01	ng/ul	0.00
78) Pyrene-d10	19.51	212	1820696	38.08	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.41	264	1964395	34.57	ng/ul	-0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.82	163	510804	13.345	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM071719\
Data File : BM021546.D
Acq On : 19 Jul 2019 06:04
Operator : HP/JU
Sample : K3764-06
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A52H8

Quant Time: Jul 19 06:59:49 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM070819MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jul 19 00:39:42 2019
Response via : Initial Calibration

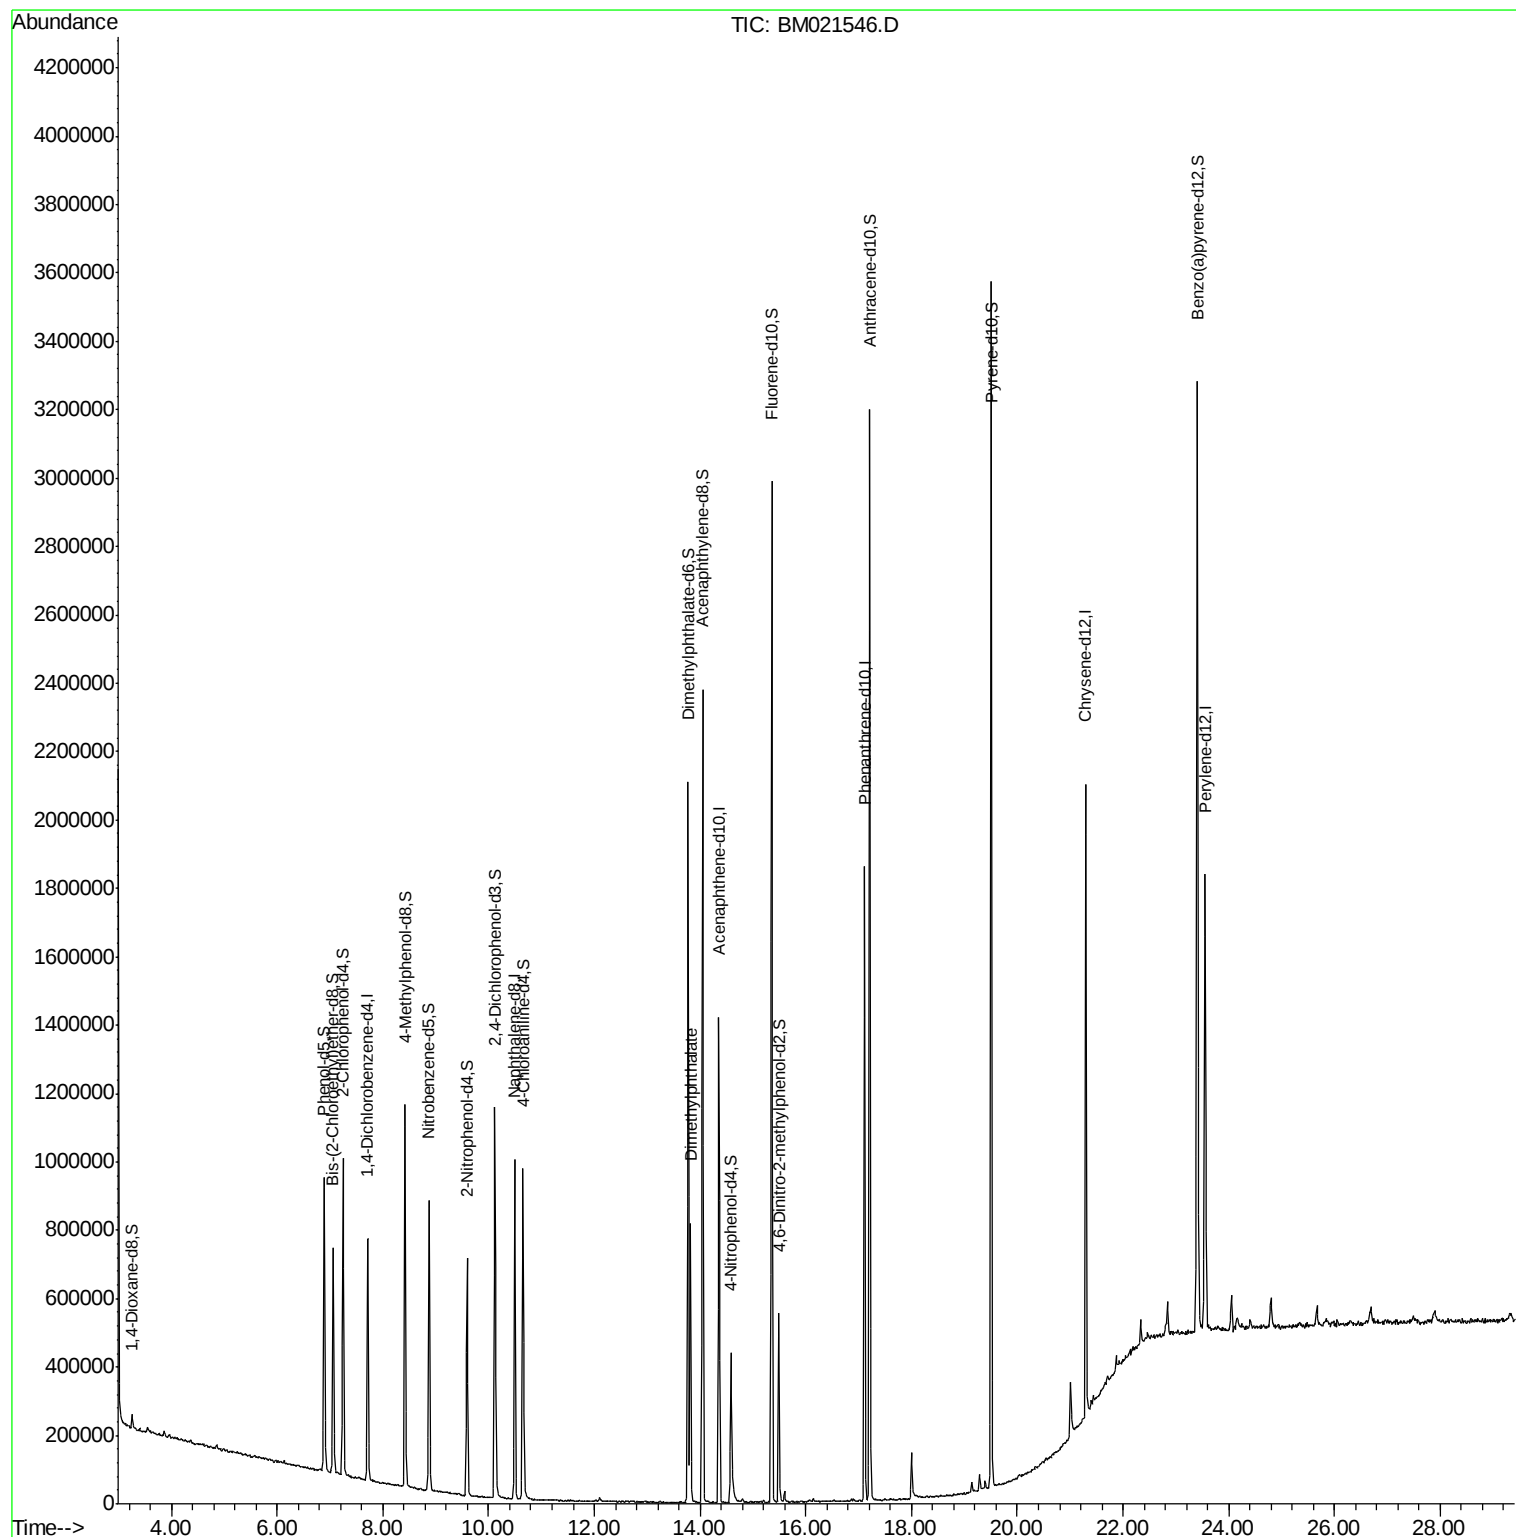

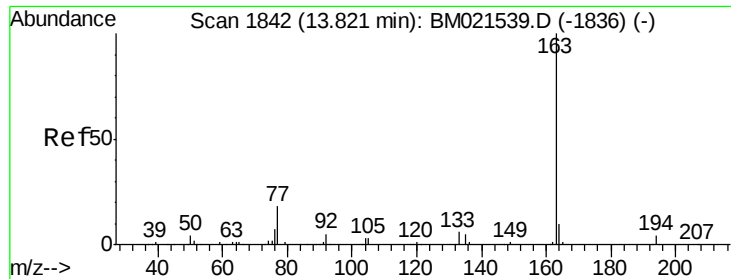

#44
 Dimethylphthalate
 Concen: 13.345 ng/ul
 RT: 13.82 min Scan# 1842
 Delta R.T. -0.01 min
 Lab File: BM021546.D
 Acq: 19 Jul 2019 06:04

Instrument :
 BNA_M
 ClientSampleId :
 A52H8

Tot Ion	Ratio	Lower	Upper
163	100		
194	4.2	3.6	5.4
164	10.3	8.3	12.5

