

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM071719\
 Data File : BM021525.D
 Acq On : 18 Jul 2019 16:03
 Operator : HP/JU
 Sample : PB121446BL
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK46

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM070819MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.893	658	664	673	rBV	705255	1110234	26.97%	2.611%
2	7.063	688	693	702	rVB	541301	845430	20.54%	1.988%
3	7.251	719	725	734	rVB	762011	1222435	29.69%	2.875%
4	7.716	798	804	813	rVB	645422	1029558	25.01%	2.421%
5	8.422	918	924	942	rVB	863021	1459472	35.45%	3.432%
6	8.881	995	1002	1013	rVB	726331	1193204	28.98%	2.806%
7	9.592	1117	1123	1135	rVB	587766	989204	24.03%	2.326%
8	10.128	1207	1214	1231	rBV	890649	1565321	38.02%	3.681%
9	10.498	1270	1277	1286	rVB	906718	1475896	35.85%	3.471%
10	10.651	1296	1303	1320	rBV	802291	1502518	36.50%	3.533%
11	12.104	1545	1550	1558	rVB3	10306	19264	0.47%	0.045%
12	13.780	1828	1835	1847	rBV	1562365	2212762	53.75%	5.203%
13	14.051	1875	1881	1893	rBV	1880684	2771713	67.32%	6.518%
14	14.363	1926	1934	1942	rBV2	1300490	1914435	46.50%	4.502%
15	14.586	1966	1972	1987	rBV	354502	724218	17.59%	1.703%
16	15.357	2097	2103	2115	rBV	2239556	3346013	81.27%	7.868%
17	15.492	2120	2126	2140	rVV	419371	675899	16.42%	1.589%
18	15.598	2140	2144	2149	rVB	23477	32511	0.79%	0.076%
19	16.139	2233	2236	2241	rBV3	7481	10930	0.27%	0.026%
20	16.904	2361	2366	2371	rVB5	5206	7495	0.18%	0.018%
21	17.115	2395	2402	2410	rBV2	1553760	2156261	52.38%	5.070%
22	17.215	2412	2419	2432	rVV	2332396	3430072	83.32%	8.066%
23	18.039	2555	2559	2562	rBV4	3454	5464	0.13%	0.013%
24	19.151	2743	2748	2751	rBV	23153	36616	0.89%	0.086%
25	19.398	2788	2790	2794	rVB	15051	15374	0.37%	0.036%
26	19.509	2803	2809	2819	rBV	2732216	3893035	94.56%	9.154%
27	21.309	3110	3115	3122	rBV	1700624	2317683	56.30%	5.450%
28	23.421	3467	3474	3485	rVB	2194863	4116929	100.00%	9.681%
29	23.562	3492	3498	3511	rVB	1278531	2446569	59.43%	5.753%


Sum of corrected areas: 42526515

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM071719\
Data File : BM021525.D
Acq On : 18 Jul 2019 16:03
Operator : HP/JU
Sample : PB121446BL
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK46

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM070819MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

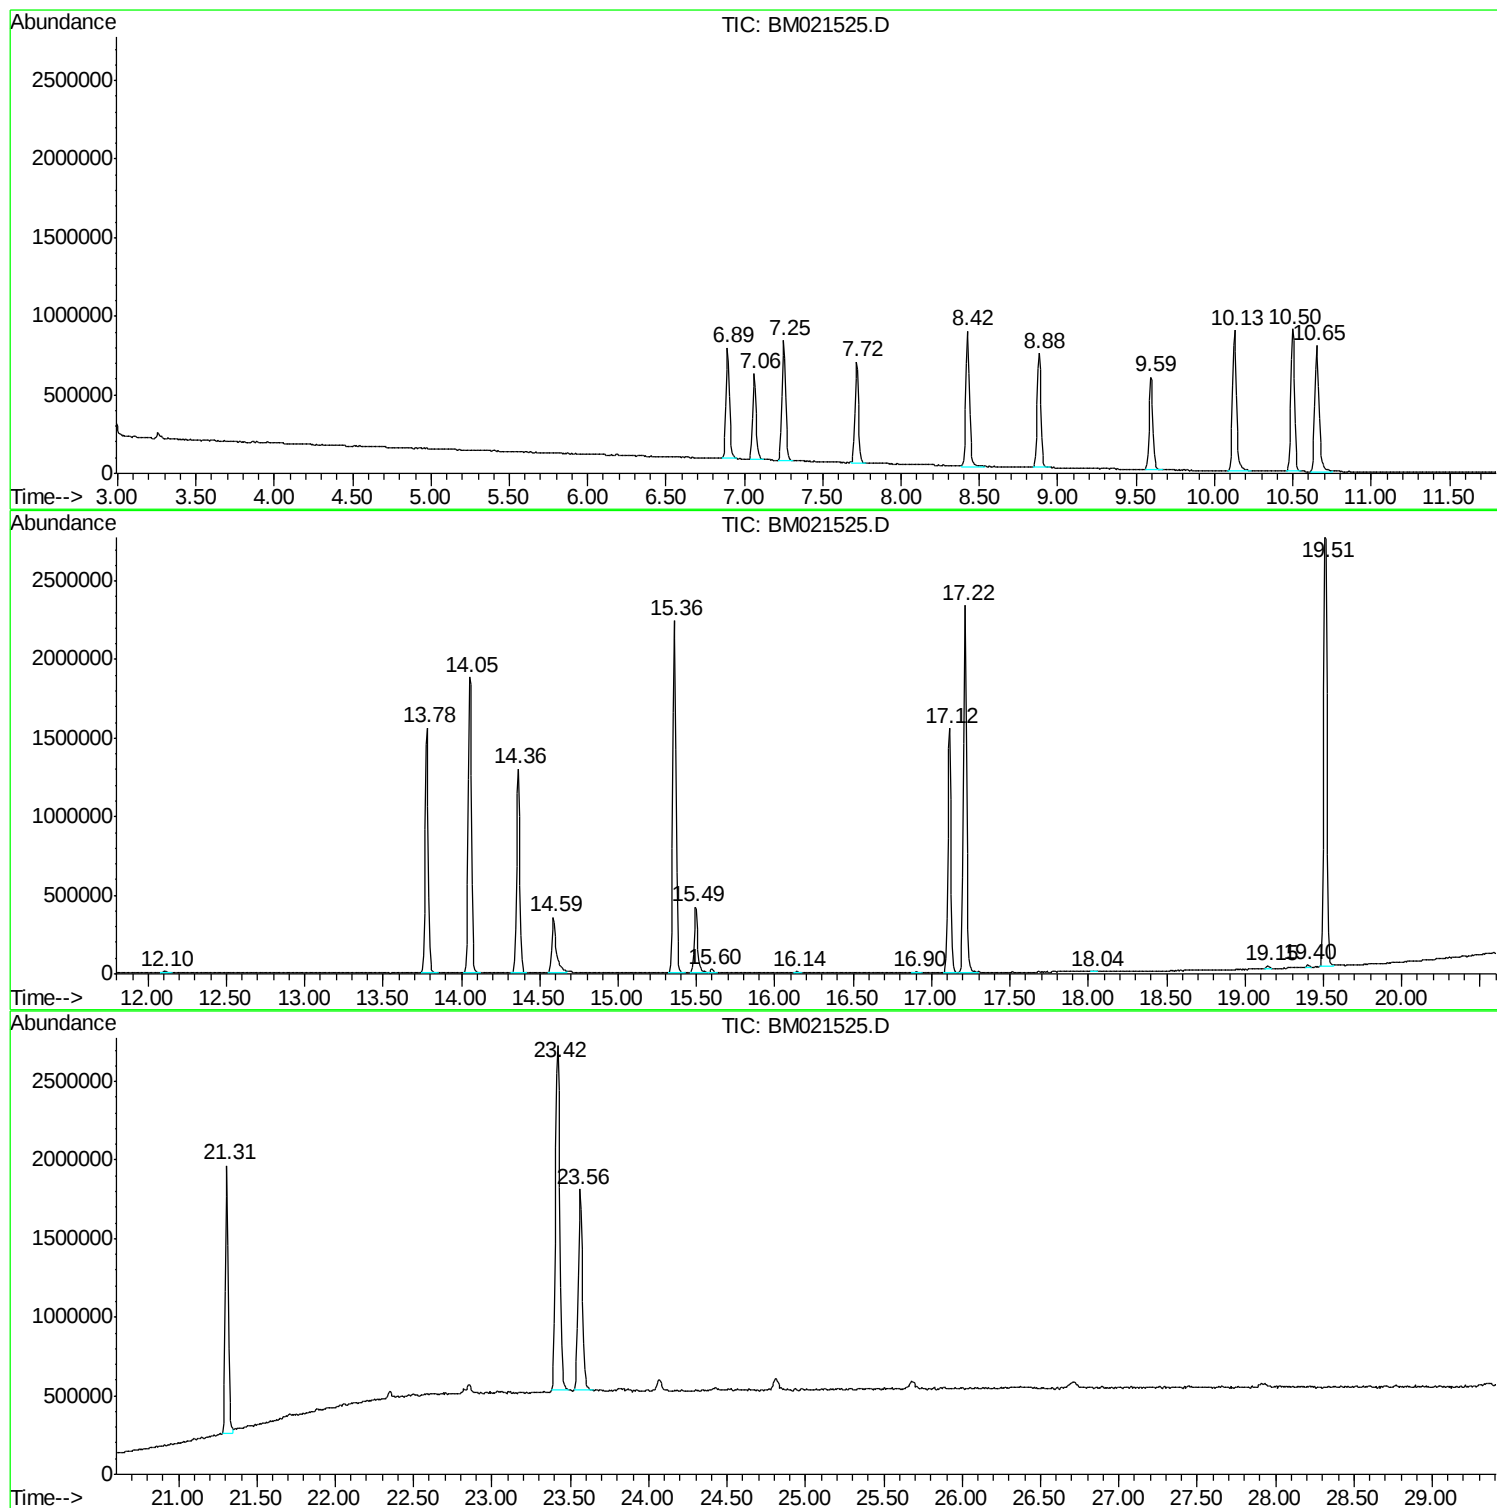

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM071719\
Data File : BM021525.D
Acq On : 18 Jul 2019 16:03
Operator : HP/JU
Sample : PB121446BL
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK46

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM070819MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM071719\
Data File : BM021525.D
Acq On : 18 Jul 2019 16:03
Operator : HP/JU
Sample : PB121446BL
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK46

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM070819MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc