

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM071719\
 Data File : BM021552.D
 Acq On : 19 Jul 2019 10:19
 Operator : HP/JU
 Sample : K3764-21
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A52H0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM070819MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.887	657	663	676	rVB	704036	1160473	26.88%	2.555%
2	7.057	687	692	703	rVB	548109	867745	20.10%	1.911%
3	7.245	718	724	736	rVB	789695	1244497	28.83%	2.740%
4	7.710	797	803	811	rVB	681601	1094693	25.36%	2.410%
5	8.416	917	923	938	rVB	874903	1444203	33.45%	3.180%
6	8.875	995	1001	1010	rBV	726608	1176846	27.26%	2.591%
7	9.592	1116	1123	1133	rVB	572258	948521	21.97%	2.089%
8	10.122	1206	1213	1233	rVB	909921	1589278	36.81%	3.499%
9	10.492	1269	1276	1285	rVB	908237	1533782	35.53%	3.377%
10	10.645	1295	1302	1323	rBV	697754	1383201	32.04%	3.046%
11	10.963	1352	1356	1361	rVB4	5172	9162	0.21%	0.020%
12	11.133	1381	1385	1388	rBV4	2999	4505	0.10%	0.010%
13	11.298	1410	1413	1420	rVB6	4044	8617	0.20%	0.019%
14	11.498	1441	1447	1457	rBV4	11218	26155	0.61%	0.058%
15	11.757	1487	1491	1494	rBV4	3946	5519	0.13%	0.012%
16	12.098	1545	1549	1553	rBV	12138	20948	0.49%	0.046%
17	12.539	1620	1624	1629	rBV6	4138	5892	0.14%	0.013%
18	12.692	1646	1650	1654	rBV7	3115	4926	0.11%	0.011%
19	12.869	1675	1680	1683	rVV4	15353	22337	0.52%	0.049%
20	12.951	1692	1694	1701	rVB2	4405	7154	0.17%	0.016%
21	13.139	1718	1726	1730	rBV4	4607	8723	0.20%	0.019%
22	13.180	1730	1733	1737	rVV5	3153	4912	0.11%	0.011%
23	13.245	1740	1744	1748	rVV4	5949	9416	0.22%	0.021%
24	13.304	1748	1754	1755	rVV3	3343	5958	0.14%	0.013%
25	13.316	1755	1756	1762	rVB3	5535	8203	0.19%	0.018%
26	13.774	1827	1834	1838	rBV	1507358	2142781	49.63%	4.718%
27	13.821	1838	1842	1855	rVB	559710	789586	18.29%	1.739%
28	14.051	1874	1881	1894	rBV	1866993	2724403	63.11%	5.999%
29	14.168	1898	1901	1903	rBV4	5215	5718	0.13%	0.013%
30	14.233	1908	1912	1913	rBV3	4249	4611	0.11%	0.010%
31	14.357	1927	1933	1942	rVV2	1332094	1979608	45.85%	4.359%
32	14.439	1944	1947	1950	rVB4	5260	5199	0.12%	0.011%
33	14.580	1965	1971	1986	rBV	320630	697961	16.17%	1.537%
34	14.868	2016	2020	2026	rBV6	5268	8315	0.19%	0.018%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM071719\
 Data File : BM021552.D
 Acq On : 19 Jul 2019 10:19
 Operator : HP/JU
 Sample : K3764-21
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A52H0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM070819MA.M
 Title : SVOA CALIBRATION

35	15.198	2073	2076	2079	rVB3	4750	5747	0.13%	0.013%
36	15.357	2096	2103	2114	rBV	2330364	3415112	79.11%	7.520%
37	15.492	2120	2126	2139	rBV	410460	649747	15.05%	1.431%
38	15.598	2139	2144	2149	rVB2	33884	49326	1.14%	0.109%
39	15.727	2162	2166	2170	rBV3	8681	12095	0.28%	0.027%
40	16.086	2219	2227	2233	rBV6	20512	47187	1.09%	0.104%
41	16.139	2233	2236	2239	rVB2	8899	10285	0.24%	0.023%
42	16.192	2239	2245	2250	rBV	21235	35089	0.81%	0.077%
43	16.245	2250	2254	2260	rVV3	23099	42627	0.99%	0.094%
44	16.310	2260	2265	2269	rVV3	21201	28419	0.66%	0.063%
45	16.351	2269	2272	2277	rVB4	13917	18309	0.42%	0.040%
46	16.404	2277	2281	2285	rBV4	7374	15477	0.36%	0.034%
47	16.457	2288	2290	2294	rVB3	6601	7245	0.17%	0.016%
48	16.509	2294	2299	2305	rVB5	18774	32130	0.74%	0.071%
49	16.574	2305	2310	2313	rBV	18431	26756	0.62%	0.059%
50	16.651	2319	2323	2329	rVB2	13414	18596	0.43%	0.041%
51	16.786	2342	2346	2349	rVB6	4140	5986	0.14%	0.013%
52	16.904	2361	2366	2372	rVB3	14523	25392	0.59%	0.056%
53	17.021	2383	2386	2390	rVB3	3083	4538	0.11%	0.010%
54	17.109	2394	2401	2411	rBV	1689483	2310206	53.51%	5.087%
55	17.209	2411	2418	2429	rBV	2362411	3398393	78.72%	7.483%
56	17.404	2445	2451	2453	rBV5	3162	4897	0.11%	0.011%
57	17.598	2480	2484	2487	rBV5	5869	8630	0.20%	0.019%
58	17.751	2507	2510	2517	rBV6	4050	8941	0.21%	0.020%
59	17.892	2529	2534	2540	rVB6	5682	10955	0.25%	0.024%
60	17.998	2548	2552	2563	rBV	135054	229363	5.31%	0.505%
61	18.468	2629	2632	2634	rBV4	3608	4497	0.10%	0.010%
62	18.927	2706	2710	2717	rVB7	9030	14636	0.34%	0.032%
63	19.139	2742	2746	2756	rBV	25287	52700	1.22%	0.116%
64	19.286	2767	2771	2776	rBV2	61641	89095	2.06%	0.196%
65	19.392	2786	2789	2793	rBV	21825	24064	0.56%	0.053%
66	19.509	2803	2809	2816	rBV	2818167	3971481	91.99%	8.745%
67	21.009	3060	3064	3072	rBV3	98839	190180	4.41%	0.419%
68	21.303	3109	3114	3123	rBV	1925909	2608192	60.41%	5.743%
69	23.409	3466	3472	3482	rBV	2381654	4317159	100.00%	9.506%
70	23.556	3491	3497	3511	rVB	1411285	2767764	64.11%	6.094%

LSC Area Percent Report

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM071719\
Data File : BM021552.D
Acq On : 19 Jul 2019 10:19
Operator : HP/JU
Sample : K3764-21
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A52H0

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM070819MA.M
Title : SVOA CALIBRATION


Sum of corrected areas: 45415064

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM071719\
Data File : BM021552.D
Acq On : 19 Jul 2019 10:19
Operator : HP/JU
Sample : K3764-21
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A52H0

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM070819MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

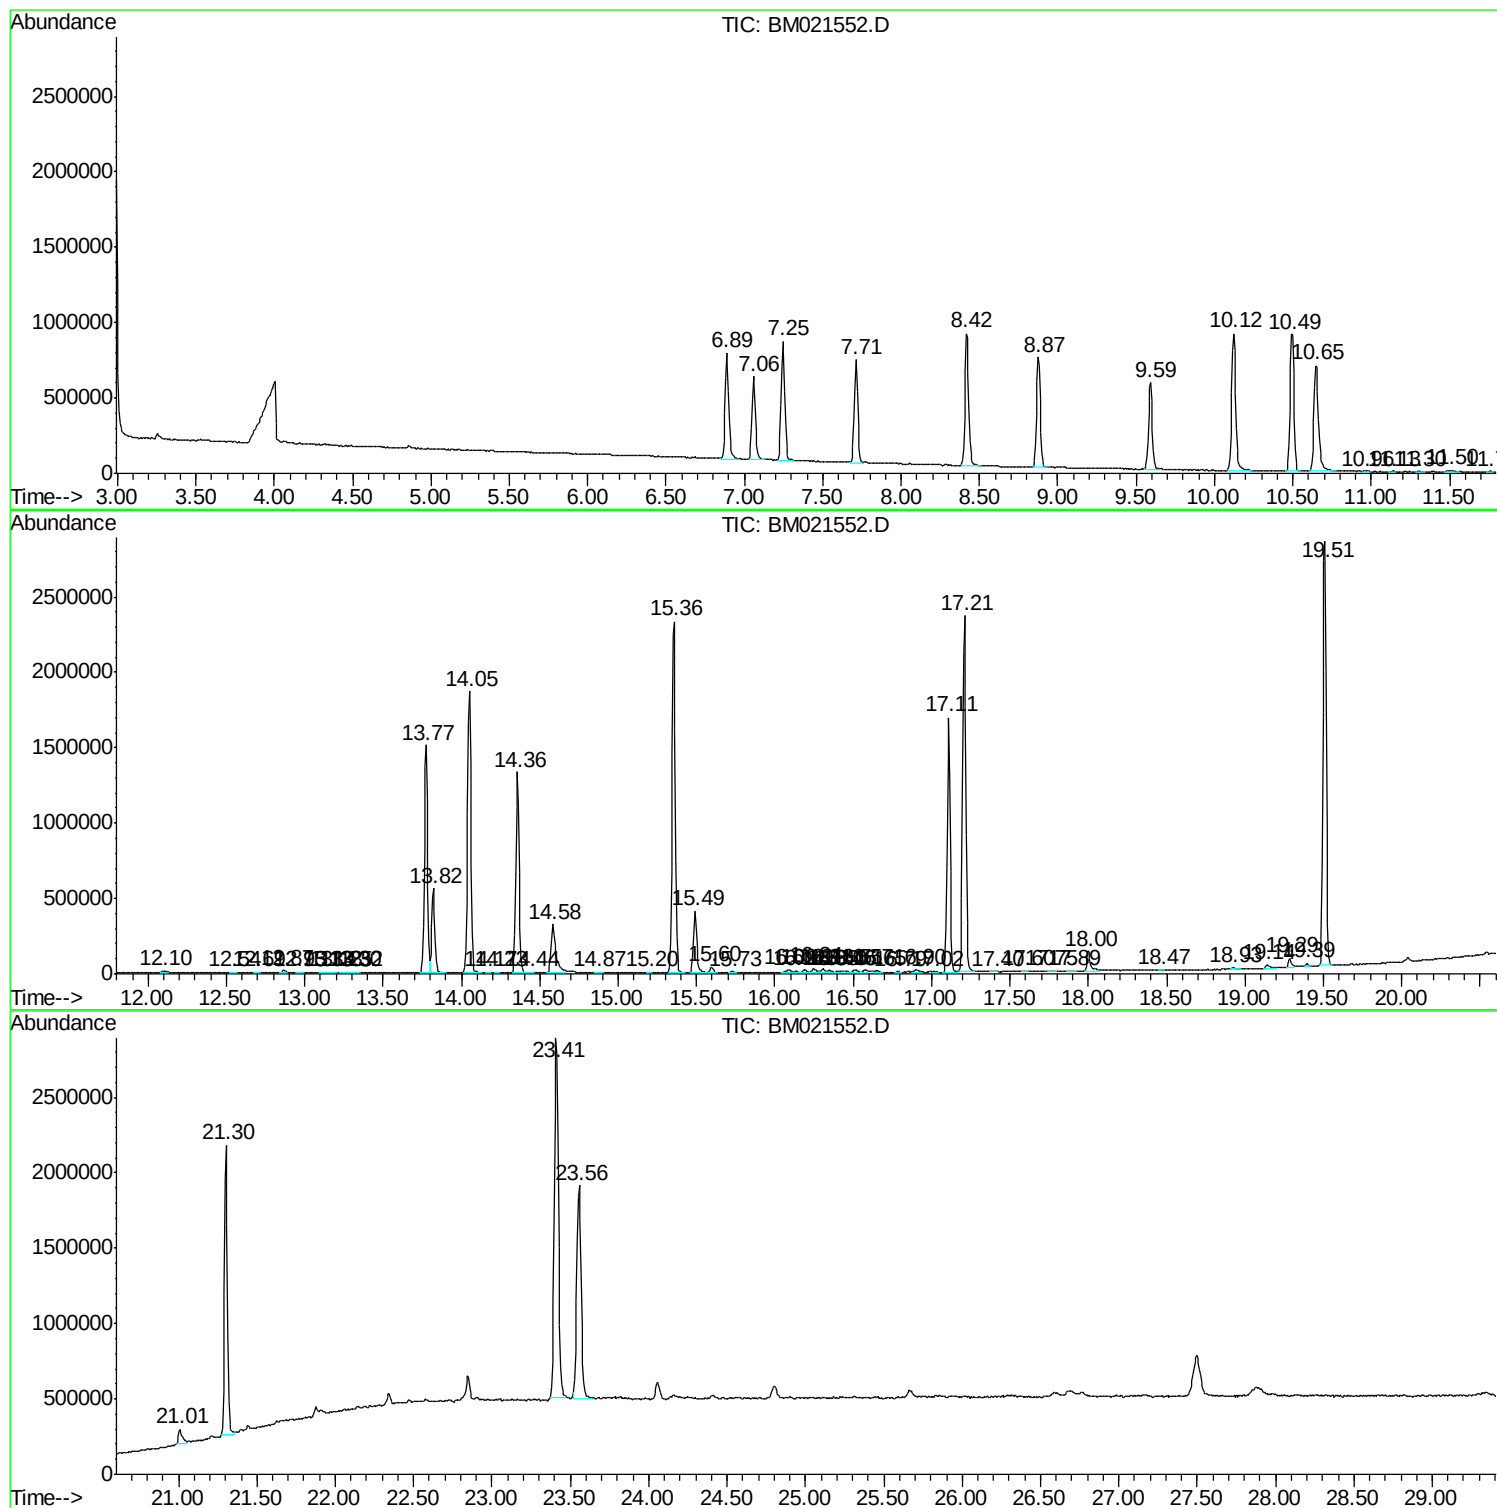

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM071719\
Data File : BM021552.D
Acq On : 19 Jul 2019 10:19
Operator : HP/JU
Sample : K3764-21
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A52H0

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM070819MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM071719\
Data File : BM021552.D
Acq On : 19 Jul 2019 10:19
Operator : HP/JU
Sample : K3764-21
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A52H0

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM070819MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc