

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071723\
 Data File : BM040921.D
 Acq On : 17 Jul 2023 14:02
 Operator : MA/JU
 Sample : 03437-05
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A46H6

Quant Time: Jul 18 02:46:21 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jul 15 03:58:02 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.857	152	4294	0.400	ng/ul	0.00
4) Naphthalene-d8	10.658	136	13976	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.504	164	6498	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.253	188	11503	0.400	ng/ul	0.00
17) Chrysene-d12	21.451	240	7751	0.400	ng/ul	0.00
23) Perylene-d12	23.824	264	10029	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.279	96	27265	4.042	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.253	152	6815	0.348	ng/ul	0.00
18) Fluoranthene-d10	19.287	212	11067	0.445	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.499	166	2869	0.110	ng/ul#	13
20) Pyrene	19.650	202	2605	0.074	ng/ul#	1
26) Benzo(a)pyrene	23.672	252	5353	0.153	ng/ul#	67


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071723\
Data File : BM040921.D
Acq On : 17 Jul 2023 14:02
Operator : MA/JU
Sample : 03437-05
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A46H6

Quant Time: Jul 18 02:46:21 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jul 15 03:58:02 2023
Response via : Initial Calibration




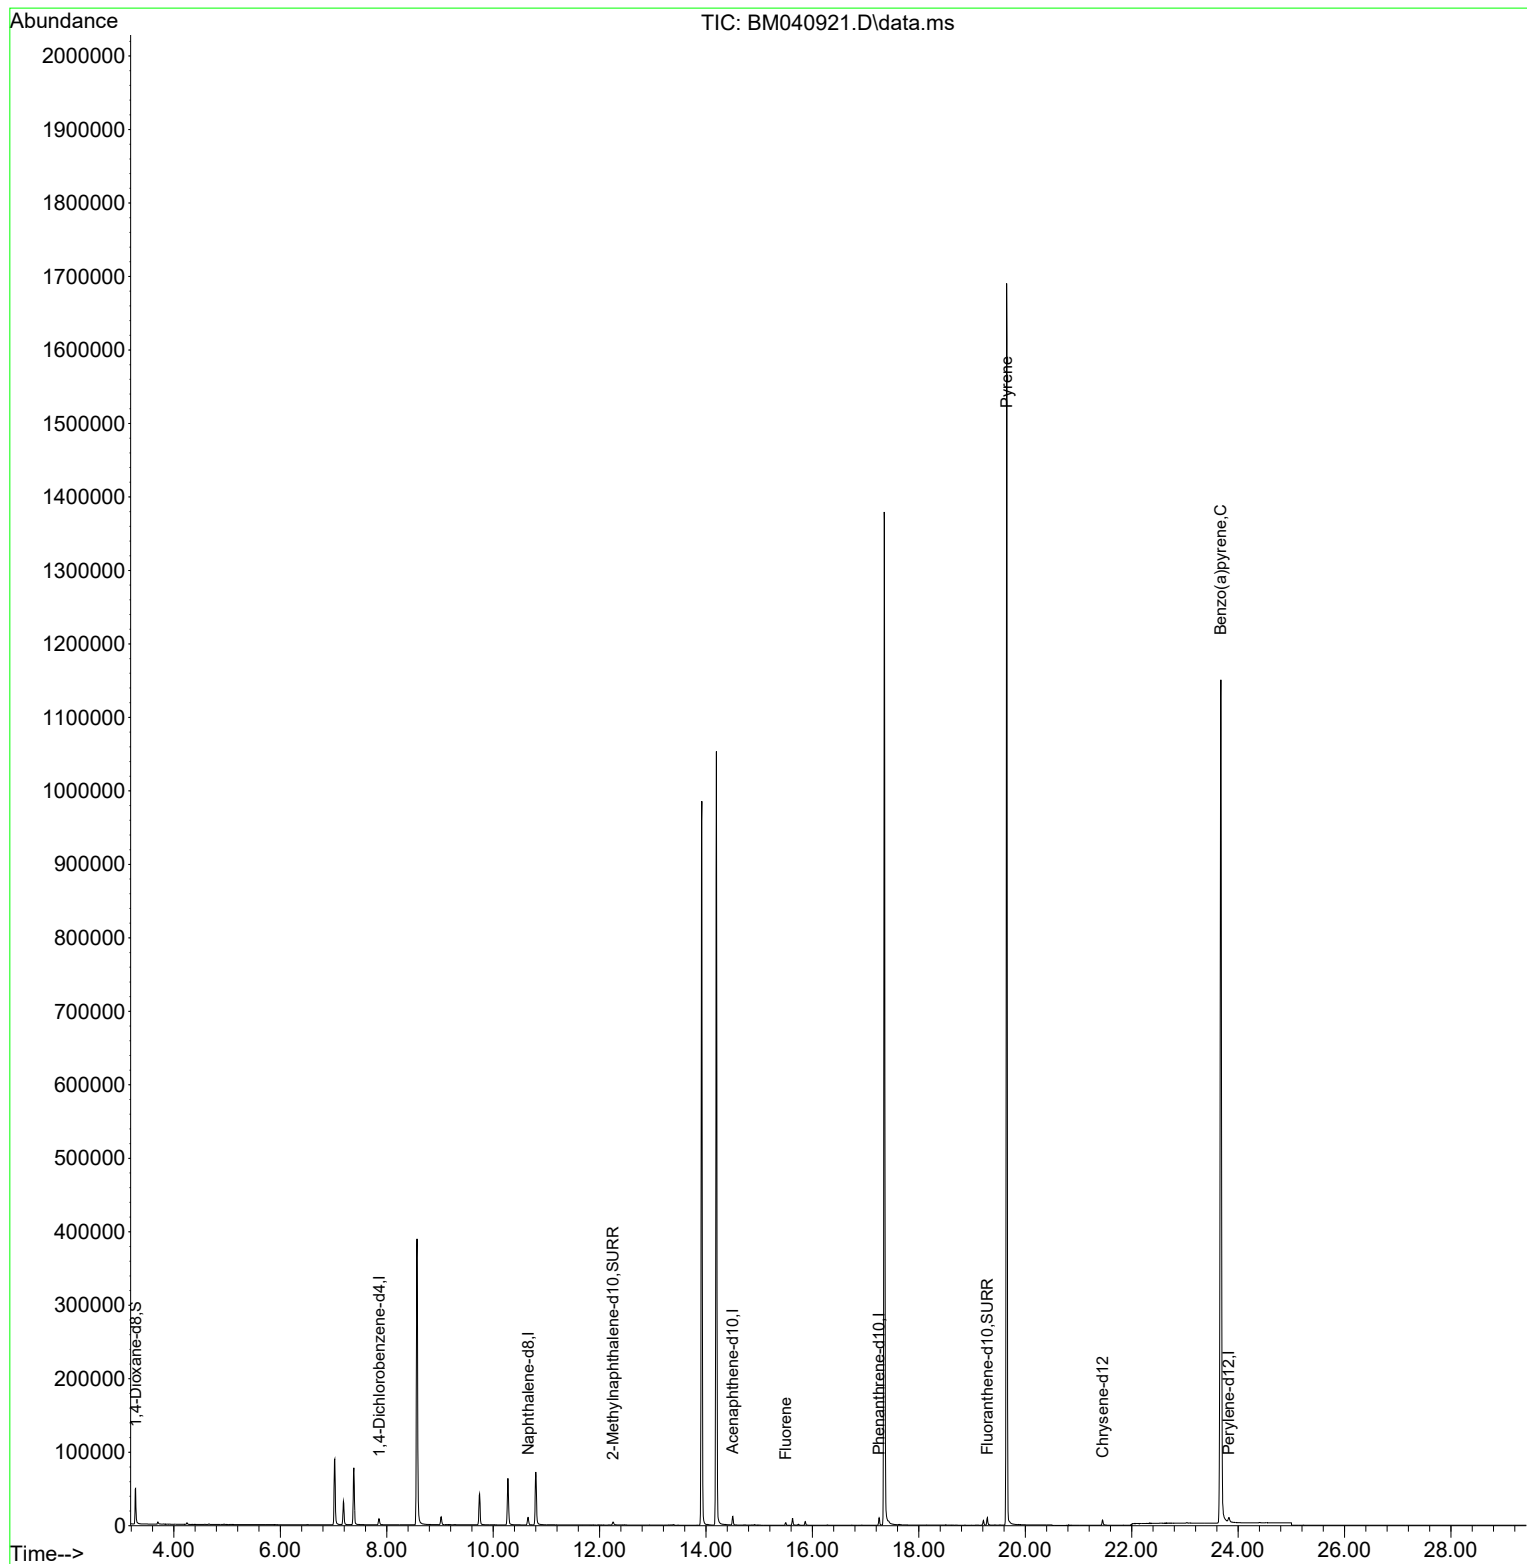


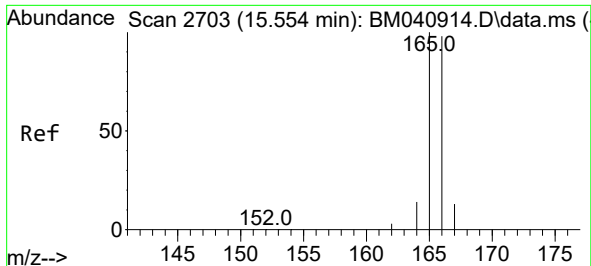

#12
Fluorene
Concen: 0.110 ng/ul
RT: 15.499 min Scan# 2
Delta R.T. -0.060 min
Lab File: BM040921.D
Acq: 17 Jul 2023 14:02




Instrument :
BNA_M
ClientSampleId :
A46H6


Tgt Ion:166 Resp: 2869
Ion Ratio Lower Upper
166 100
165 7.7 79.6 119.4#
167 35.1 11.4 17.0#

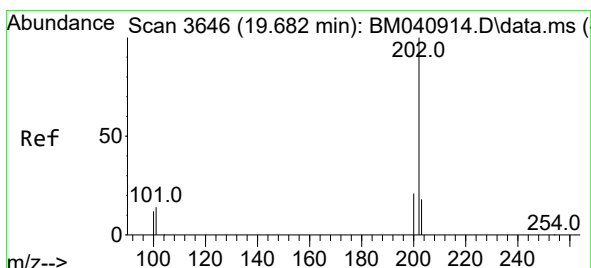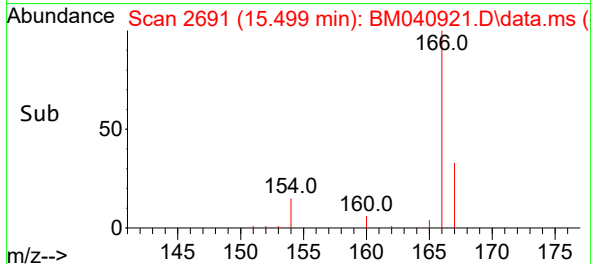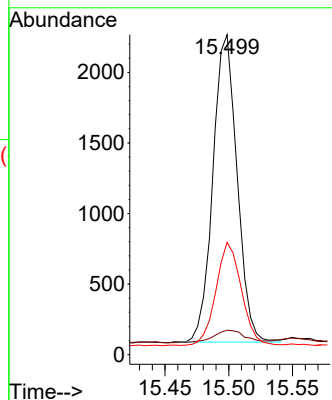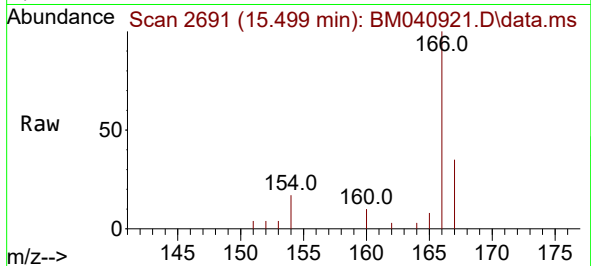

#20
Pyrene
Concen: 0.074 ng/ul
RT: 19.650 min Scan# 3639
Delta R.T. -0.037 min
Lab File: BM040921.D
Acq: 17 Jul 2023 14:02


Tgt Ion:202 Resp: 2605
Ion Ratio Lower Upper
202 100
101 192.8 12.6 18.8#
100 1526.4 9.8 14.6#

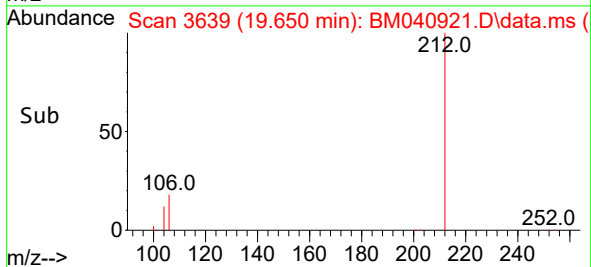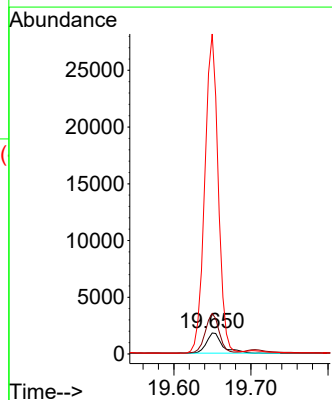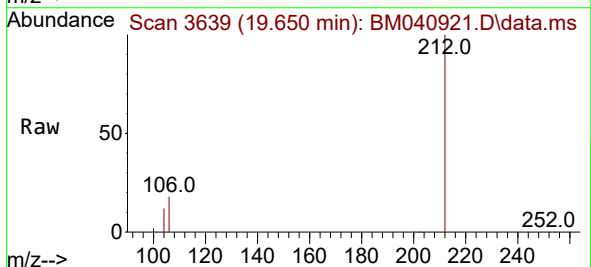

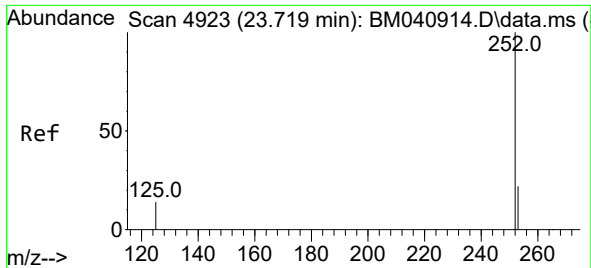

#26
Benzo(a)pyrene
Concen: 0.153 ng/ul
RT: 23.672 min Scan# 4907
Delta R.T. -0.050 min
Lab File: BM040921.D
Acq: 17 Jul 2023 14:02

Instrument :
BNA_M
ClientSampleId :
A46H6

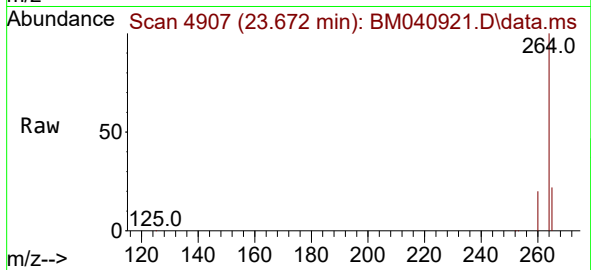

Tgt Ion:252 Resp: 5353
Ion Ratio Lower Upper
252 100
253 44.4 22.9 34.3#
125 44.6 21.0 31.4#

