

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071723\
 Data File : BM040924.D
 Acq On : 17 Jul 2023 15:58
 Operator : MA/JU
 Sample : PB153935BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK976

Quant Time: Jul 18 02:46:49 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jul 15 03:58:02 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.857	152	3835	0.400	ng/ul	0.00
4) Naphthalene-d8	10.658	136	12669	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.504	164	5841	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.257	188	9725	0.400	ng/ul	0.00
17) Chrysene-d12	21.457	240	5648	0.400	ng/ul	0.00
23) Perylene-d12	23.830	264	7578	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.275	96	32555	5.404	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.258	152	4851	0.273	ng/ul	0.00
18) Fluoranthene-d10	19.287	212	5890	0.325	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.650	202	1248	0.049	ng/ul#	1
26) Benzo(a)pyrene	23.673	252	2683	0.102	ng/ul#	44


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071723\
Data File : BM040924.D
Acq On : 17 Jul 2023 15:58
Operator : MA/JU
Sample : PB153935BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK976

Quant Time: Jul 18 02:46:49 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jul 15 03:58:02 2023
Response via : Initial Calibration




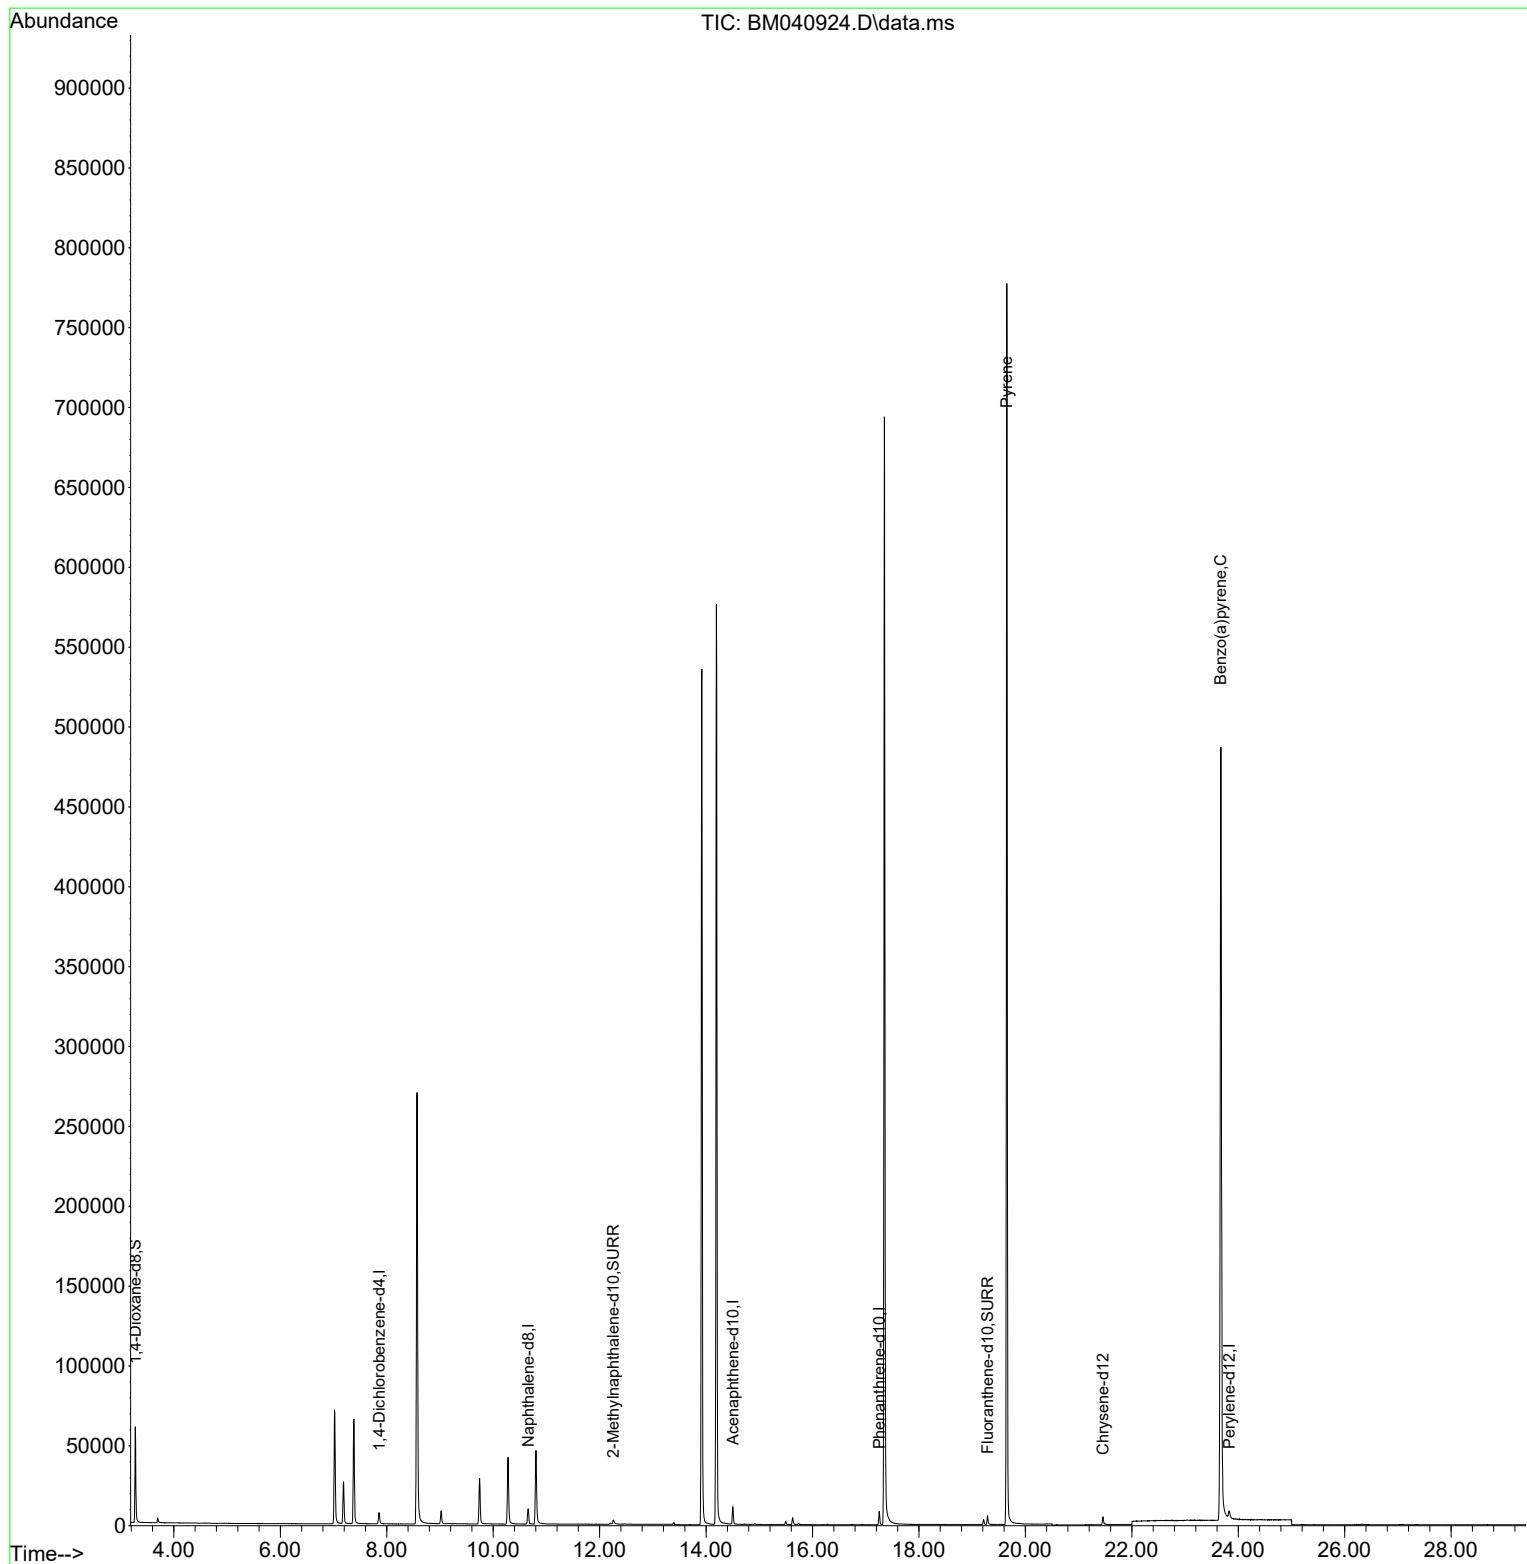


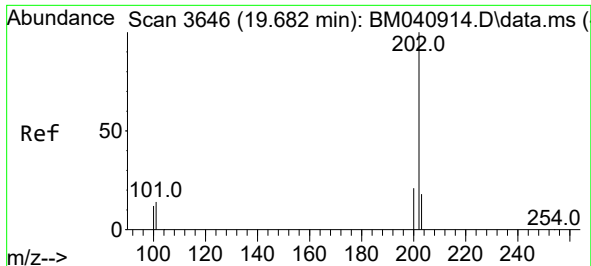

#20
Pyrene
Concen: 0.049 ng/ul
RT: 19.650 min Scan# 3639
Delta R.T. -0.037 min
Lab File: BM040924.D
Acq: 17 Jul 2023 15:58

Instrument :
BNA_M
ClientSampleId :
SBLK976

Tgt Ion:202 Resp: 1248
Ion Ratio Lower Upper
202 100
101 199.9 12.6 18.8#
100 1519.8 9.8 14.6#

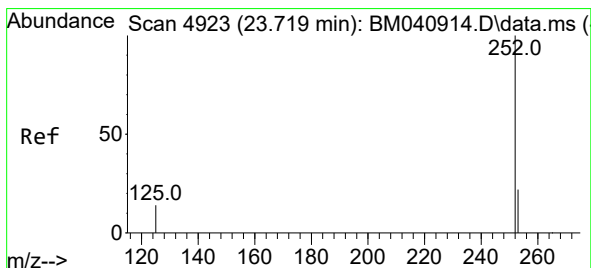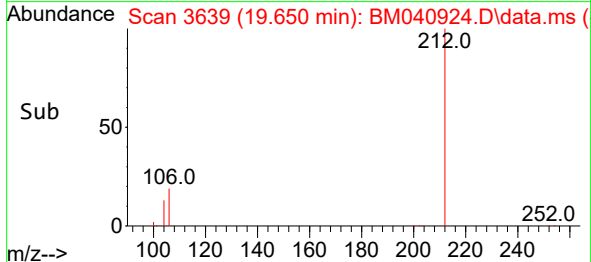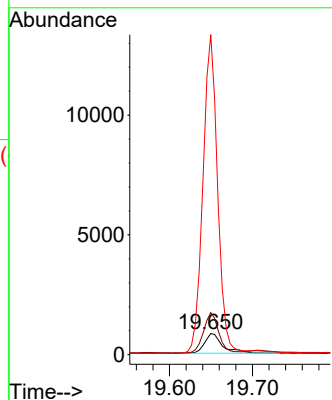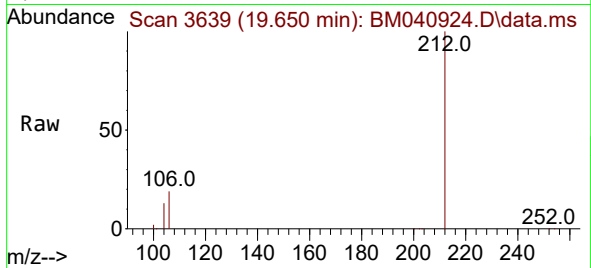

#26
Benzo(a)pyrene
Concen: 0.102 ng/ul
RT: 23.673 min Scan# 4907
Delta R.T. -0.050 min
Lab File: BM040924.D
Acq: 17 Jul 2023 15:58

Tgt Ion:252 Resp: 2683
Ion Ratio Lower Upper
252 100
253 54.5 22.9 34.3#
125 59.2 21.0 31.4#

