

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071723\
 Data File : BM040925.D
 Acq On : 17 Jul 2023 16:50
 Operator : MA/JU
 Sample : PB153934BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK935

Quant Time: Jul 18 02:46:55 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jul 15 03:58:02 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.857	152	4401	0.400	ng/ul	0.00
4) Naphthalene-d8	10.658	136	15329	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.504	164	7443	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.257	188	12340	0.400	ng/ul	0.00
17) Chrysene-d12	21.454	240	6163	0.400	ng/ul	0.00
23) Perylene-d12	23.830	264	7827	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.275	96	37722	5.457	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.258	152	6062	0.282	ng/ul	0.00
18) Fluoranthene-d10	19.287	212	7089	0.359	ng/ul	0.00
Target Compounds						Qvalue
20) Pyrene	19.650	202	1558	0.056	ng/ul#	1
26) Benzo(a)pyrene	23.673	252	2748	0.101	ng/ul#	45


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071723\
Data File : BM040925.D
Acq On : 17 Jul 2023 16:50
Operator : MA/JU
Sample : PB153934BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK935

Quant Time: Jul 18 02:46:55 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jul 15 03:58:02 2023
Response via : Initial Calibration

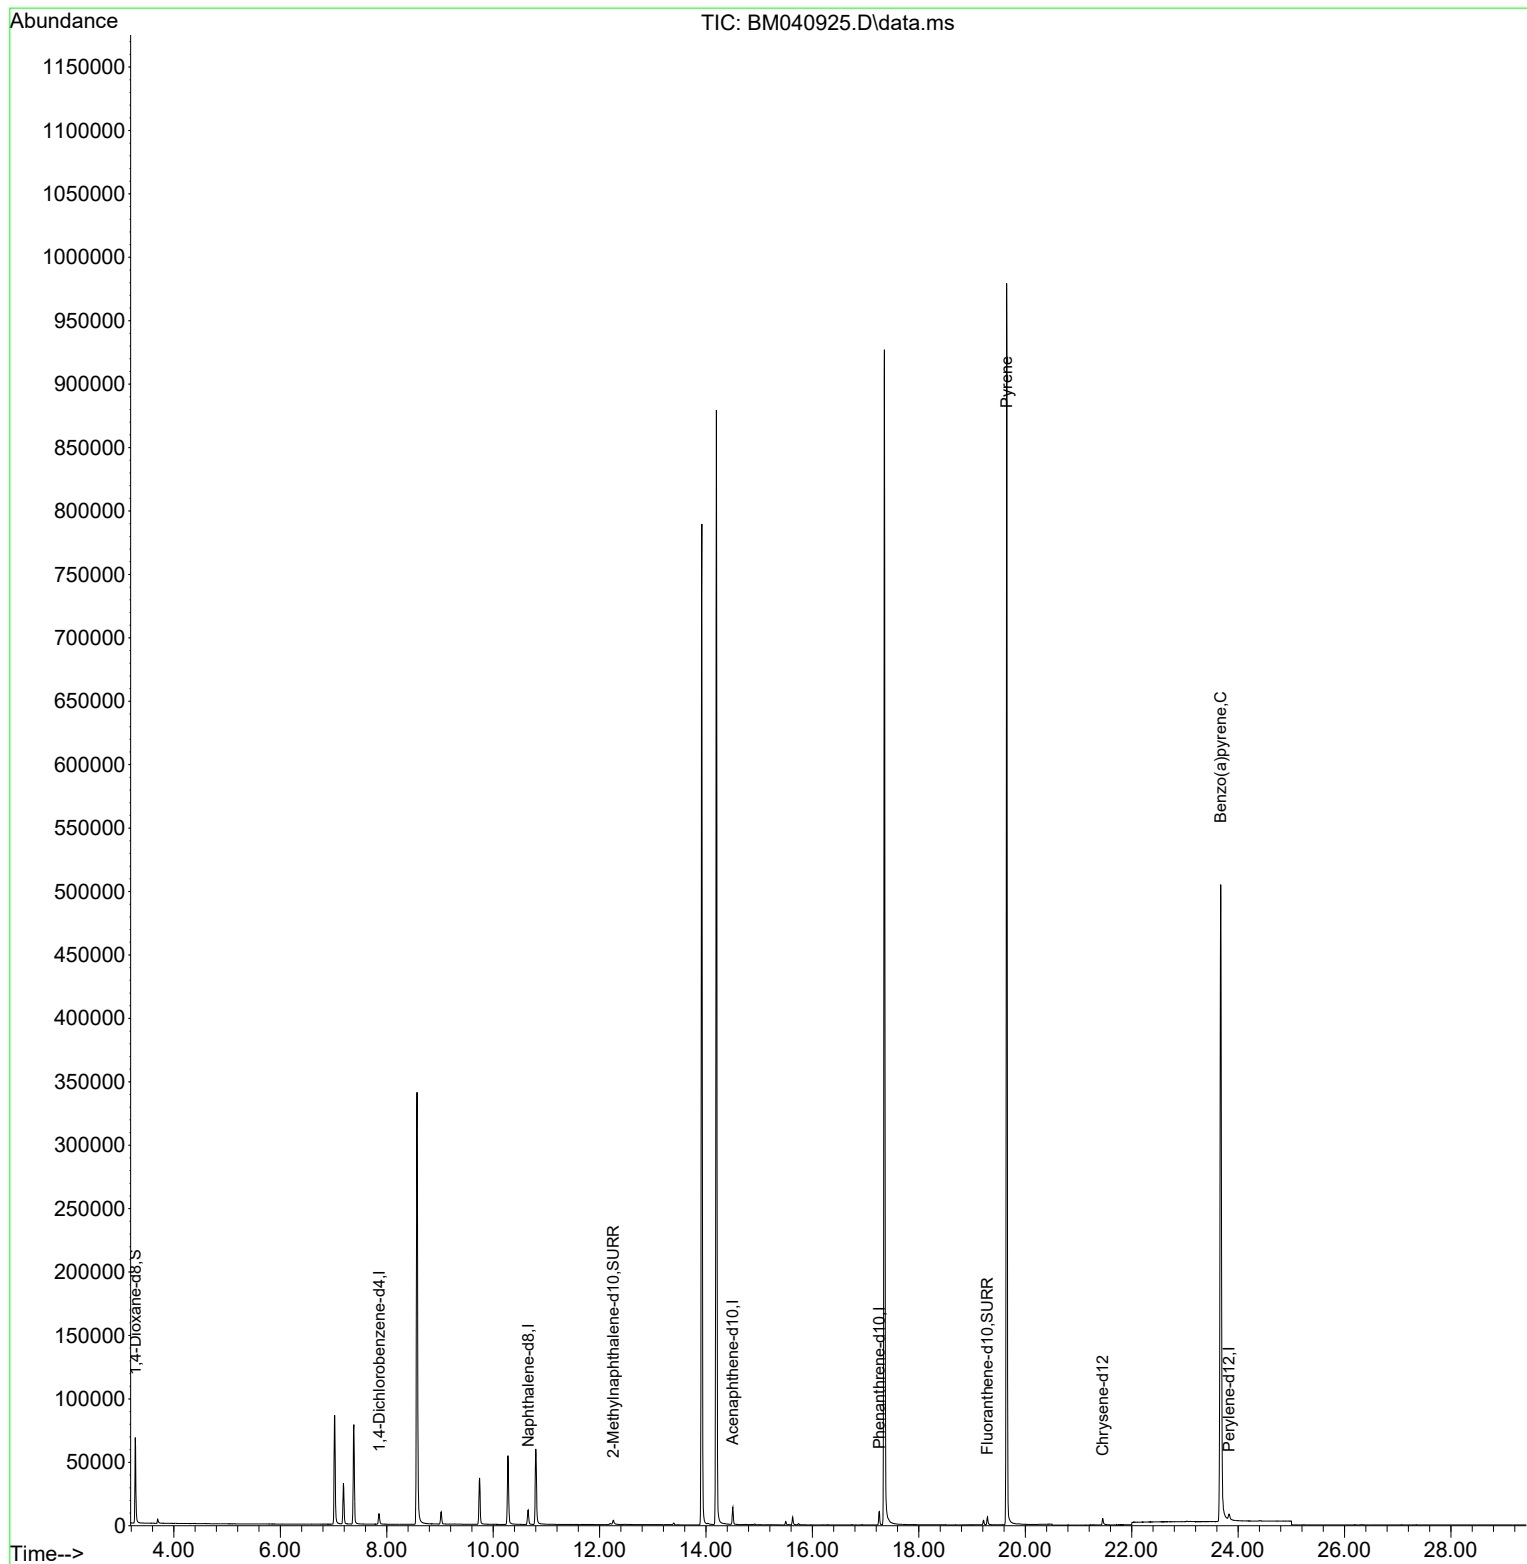

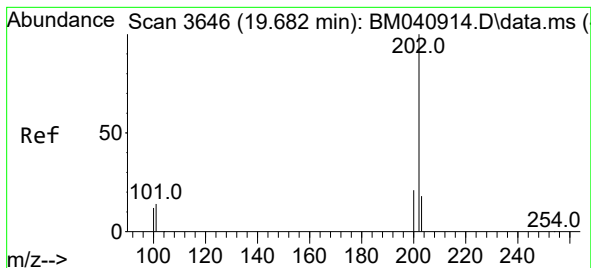

#20

Pyrene

Concen: 0.056 ng/ul

RT: 19.650 min Scan# 3

Delta R.T. -0.037 min

Lab File: BM040925.D

Acq: 17 Jul 2023 16:50

Instrument :

BNA_M

ClientSampleId :

SBLK935





Tgt Ion:202 Resp: 1558

Ion Ratio Lower Upper

202 100

101 204.0 12.6 18.8#

100 1572.2 9.8 14.6#

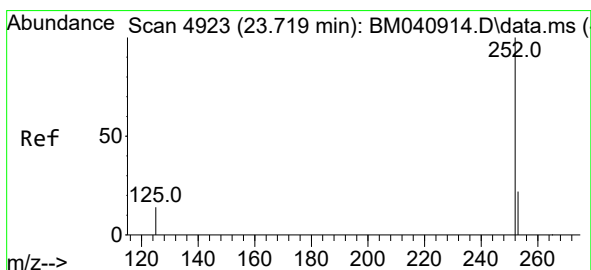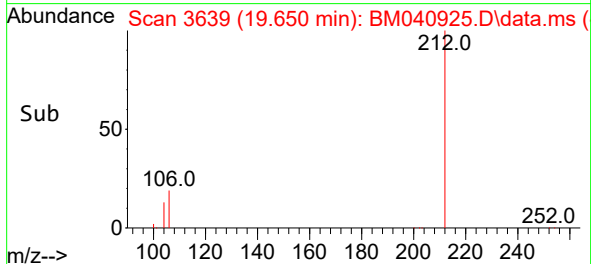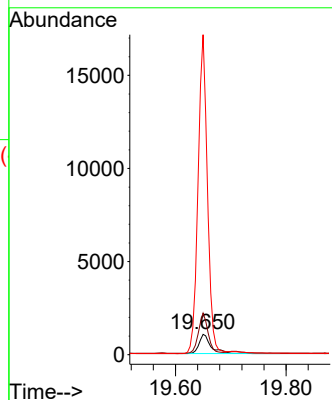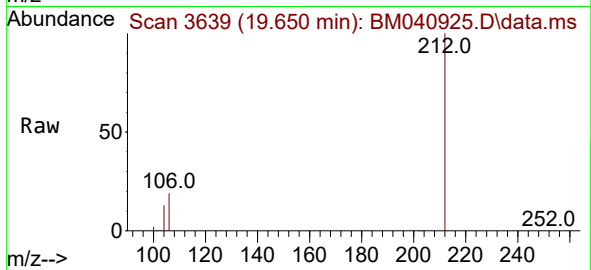

#26

Benzo(a)pyrene

Concen: 0.101 ng/ul

RT: 23.673 min Scan# 4907

Delta R.T. -0.050 min

Lab File: BM040925.D

Acq: 17 Jul 2023 16:50

Tgt Ion:252 Resp: 2748

Ion Ratio Lower Upper

252 100

253 53.5 22.9 34.3#

125 58.7 21.0 31.4#

