

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071723\
 Data File : BM040928.D
 Acq On : 17 Jul 2023 18:43
 Operator : MA/JU
 Sample : PB153934BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK935

Quant Time: Jul 18 02:47:24 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jul 15 03:58:02 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.857	152	3710	0.400	ng/ul	0.00
4) Naphthalene-d8	10.658	136	11468	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.504	164	7491	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.253	188	8277	0.400	ng/ul	0.00
17) Chrysene-d12	21.457	240	5163	0.400	ng/ul	0.00
23) Perylene-d12	23.825	264	7650	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.280	96	32368	5.554	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.258	152	4247	0.264	ng/ul	0.00
18) Fluoranthene-d10	19.287	212	5103	0.308	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.650	202	1125	0.048	ng/ul#	1
26) Benzo(a)pyrene	23.670	252	2504	0.094	ng/ul#	46


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071723\
Data File : BM040928.D
Acq On : 17 Jul 2023 18:43
Operator : MA/JU
Sample : PB153934BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK935

Quant Time: Jul 18 02:47:24 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jul 15 03:58:02 2023
Response via : Initial Calibration




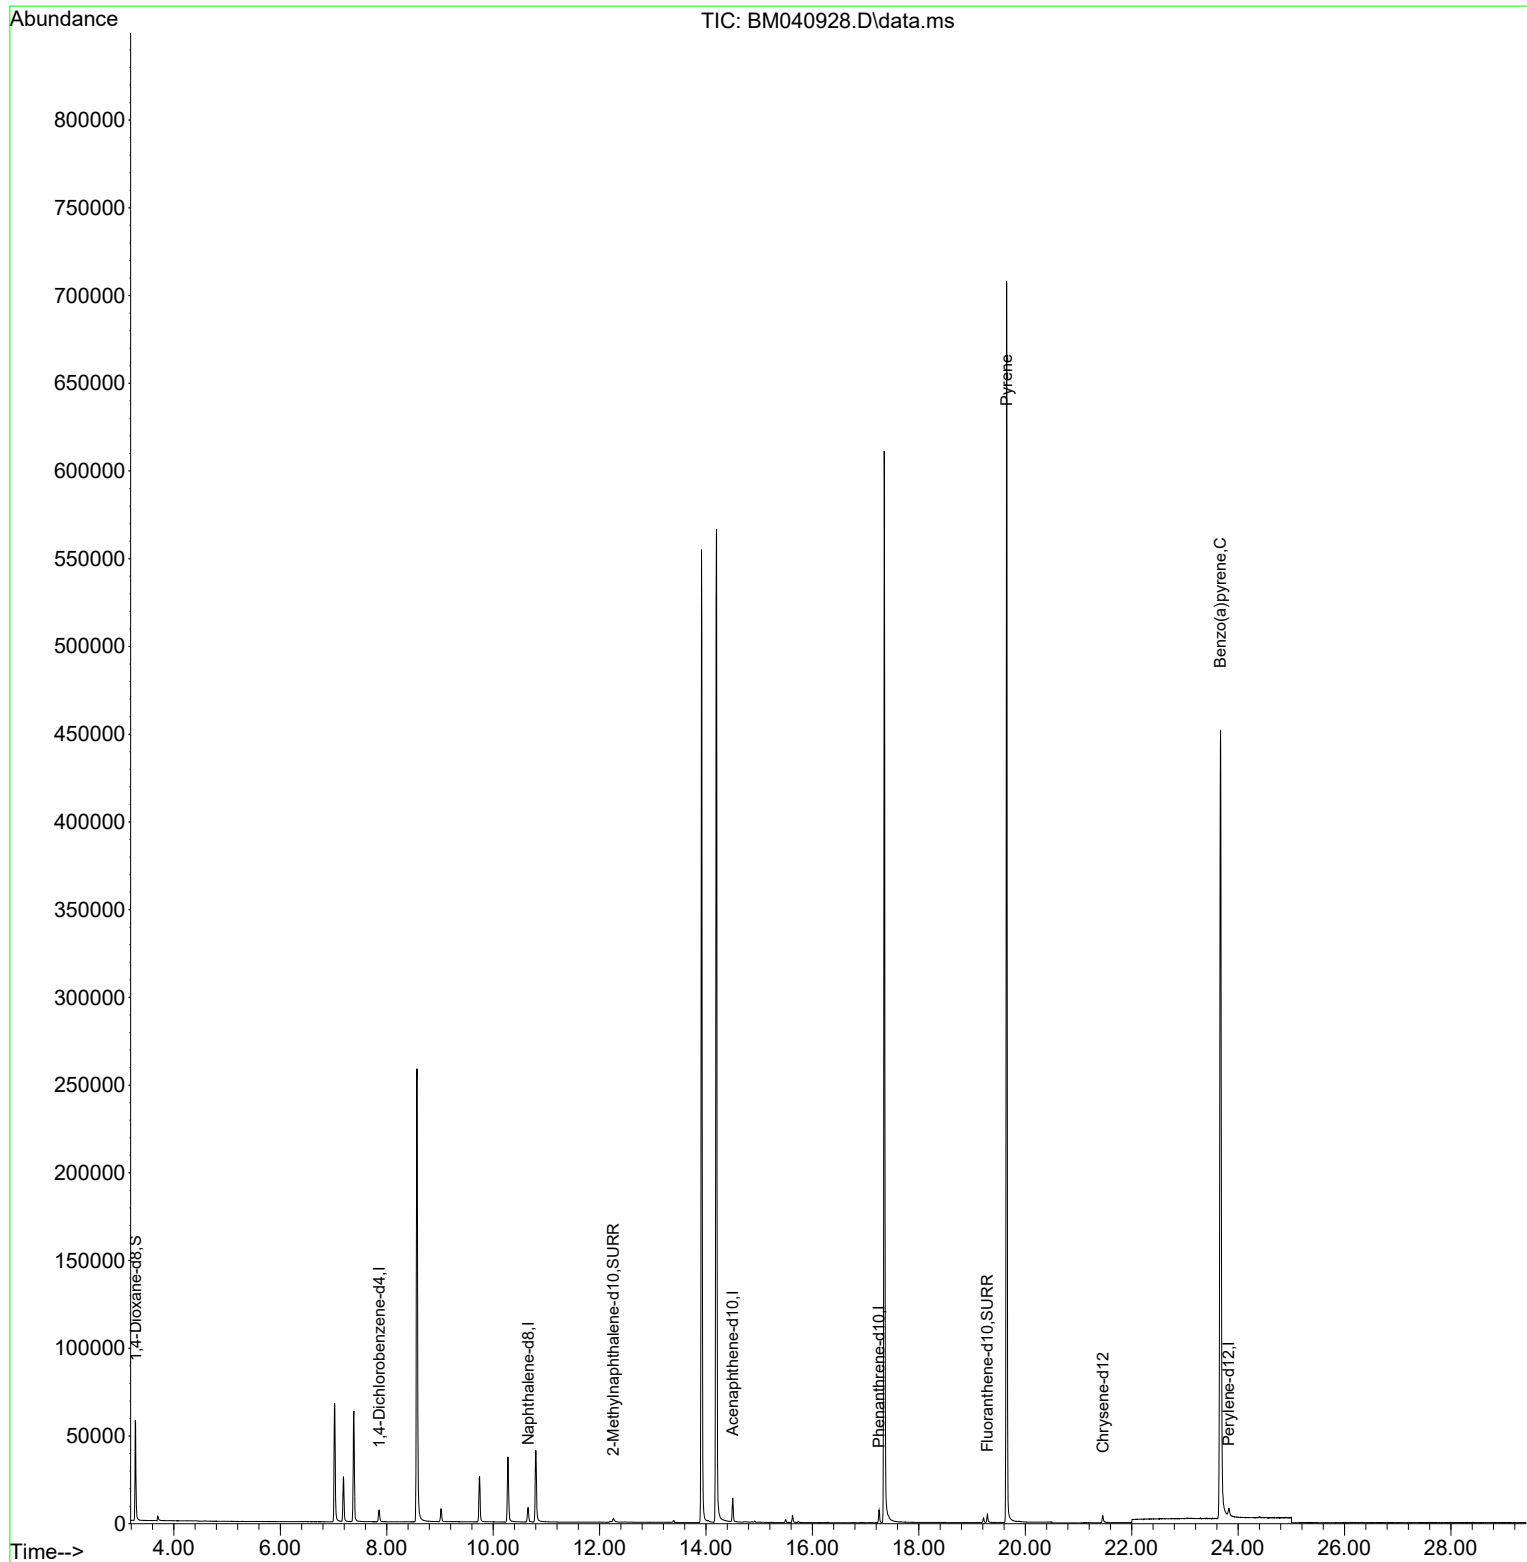


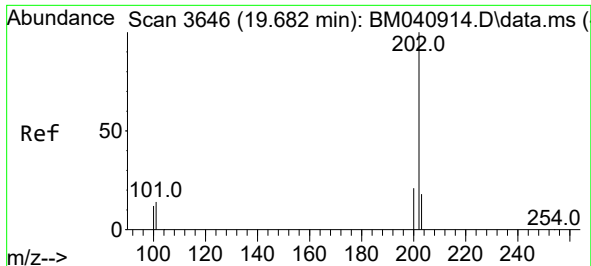

#20
Pyrene
Concen: 0.048 ng/ul
RT: 19.650 min Scan# 3646
Delta R.T. -0.037 min
Lab File: BM040928.D
Acq: 17 Jul 2023 18:43

Instrument :
BNA_M
ClientSampleId :
SBLK935

Tgt Ion:202 Resp: 1125
Ion Ratio Lower Upper
202 100
101 190.5 12.6 18.8#
100 1455.3 9.8 14.6#

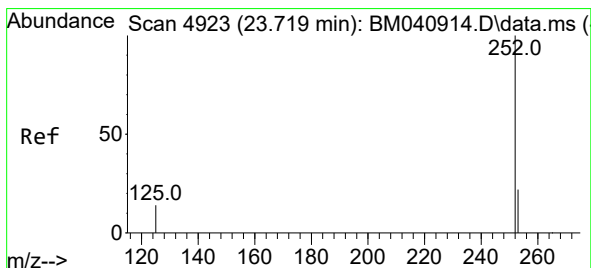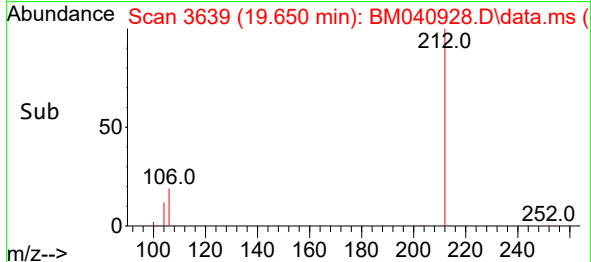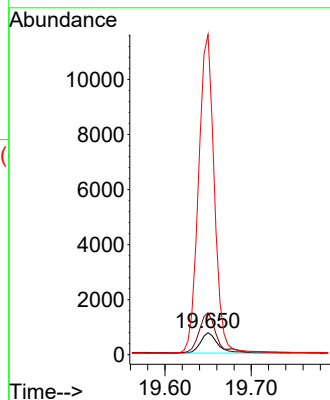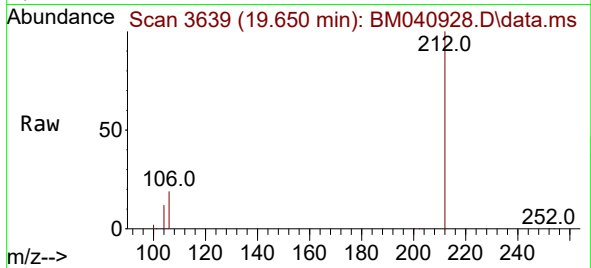

#26
Benzo(a)pyrene
Concen: 0.094 ng/ul
RT: 23.670 min Scan# 4906
Delta R.T. -0.053 min
Lab File: BM040928.D
Acq: 17 Jul 2023 18:43

Tgt Ion:252 Resp: 2504
Ion Ratio Lower Upper
252 100
253 54.3 22.9 34.3#
125 57.2 21.0 31.4#

