
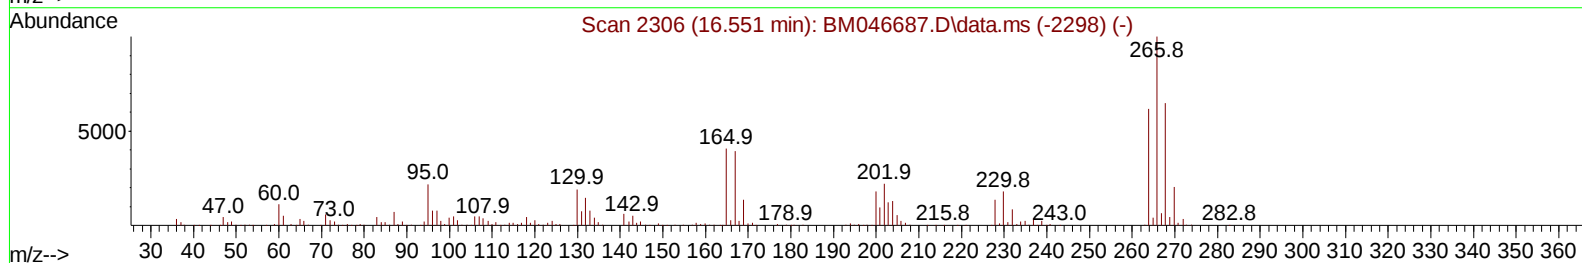
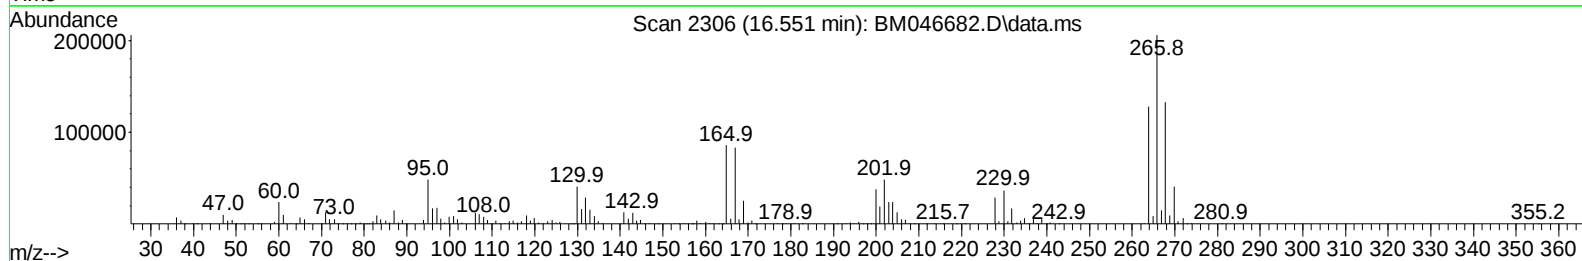


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071724\
Data File : BM046682.D
Acq On : 17 Jul 2024 23:53
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 21 Sample Multiplier: 1

Quant Time: Jul 18 06:27:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 18 06:01:46 2024
Response via : Initial Calibration

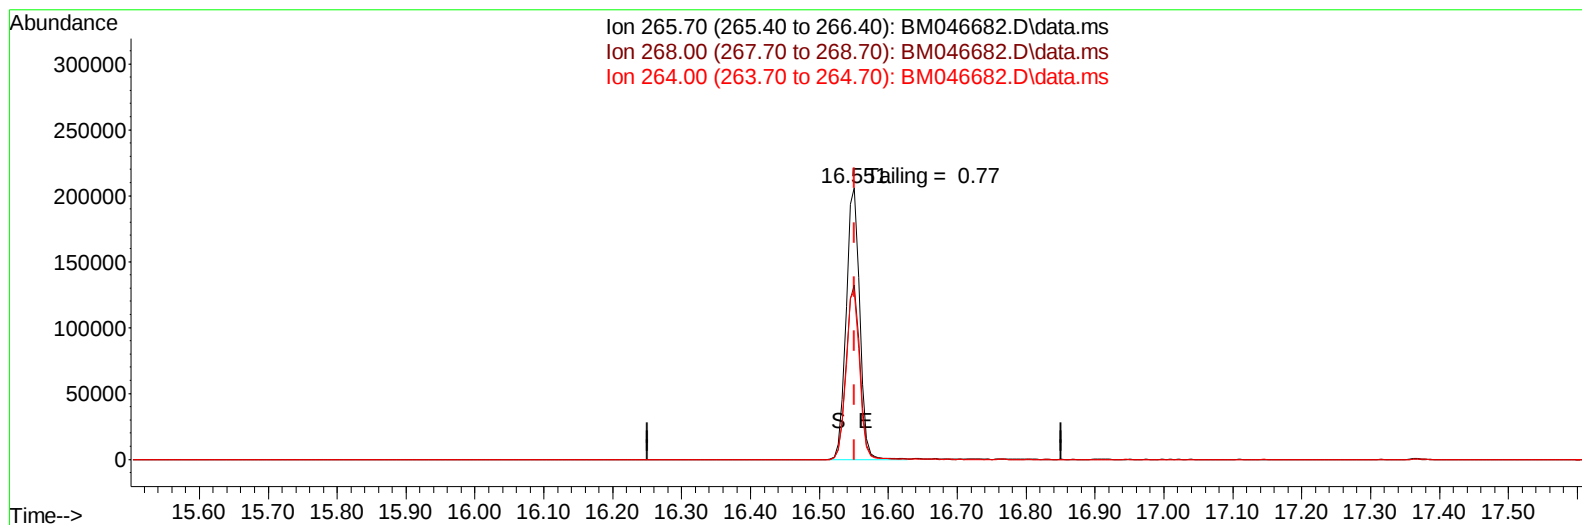

TIC: BM046682.D\data.ms

(70) Pentachlorophenol (C)




16.551min (-0.000) 0.00 ng

response 280843

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.80	64.36
264.00	61.80	61.98
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071724\
Data File : BM046682.D
Acq On : 17 Jul 2024 23:53
Operator : MA/JU
Sample : DFTTP
Misc :
ALS Vial : 21 Sample Multiplier: 1

Quant Time: Jul 18 06:27:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 18 06:01:46 2024
Response via : Initial Calibration

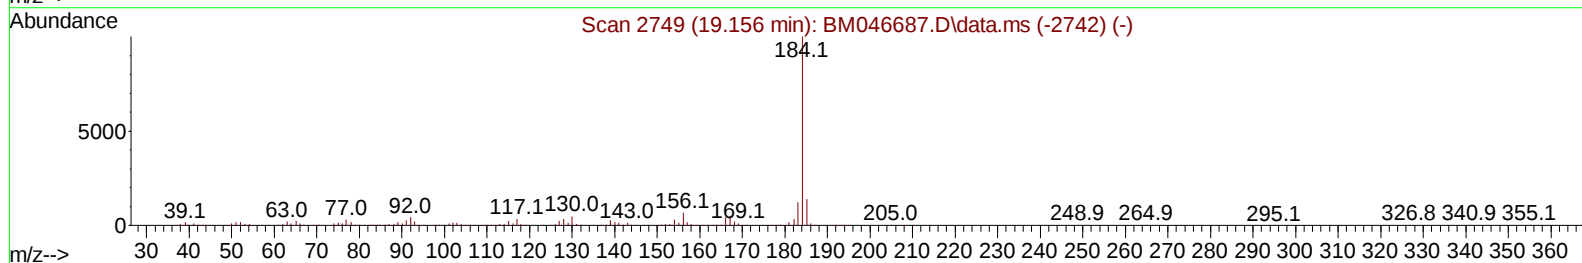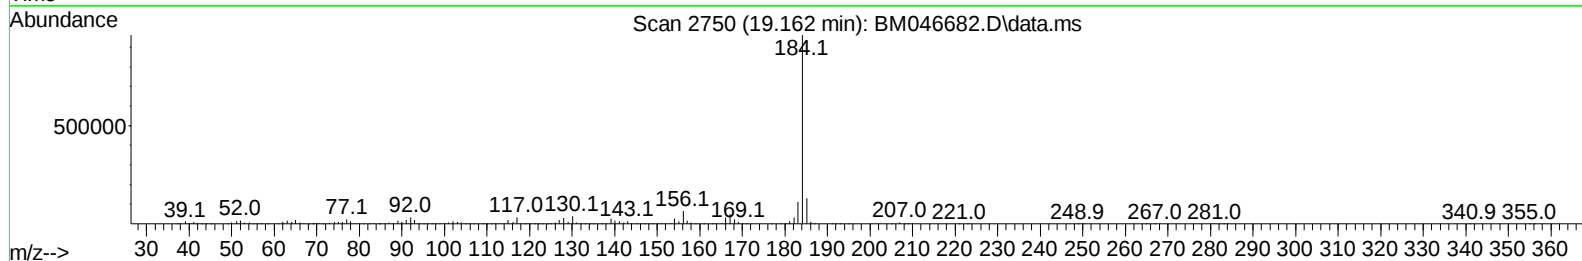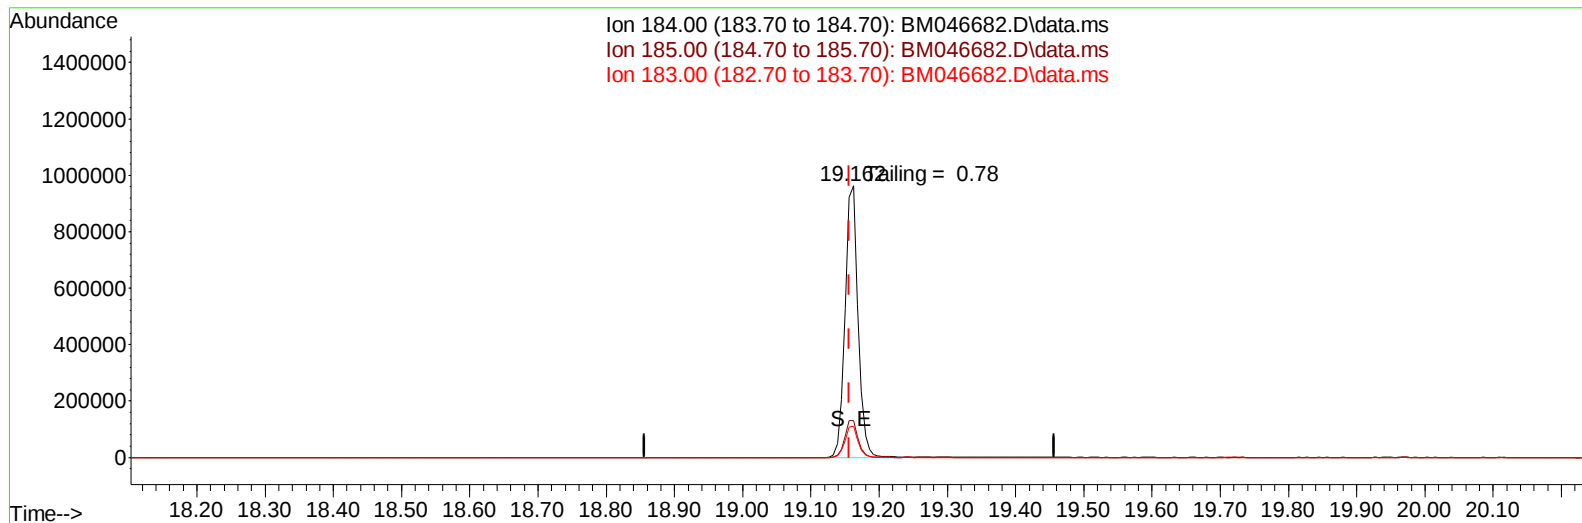

TIC: BM046682.D\data.ms

(77) Benzidine**19.162min (+ 0.006) 349805.78 ng****response 1266936**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	13.69
183.00	12.30	11.50
0.00	0.00	0.00