
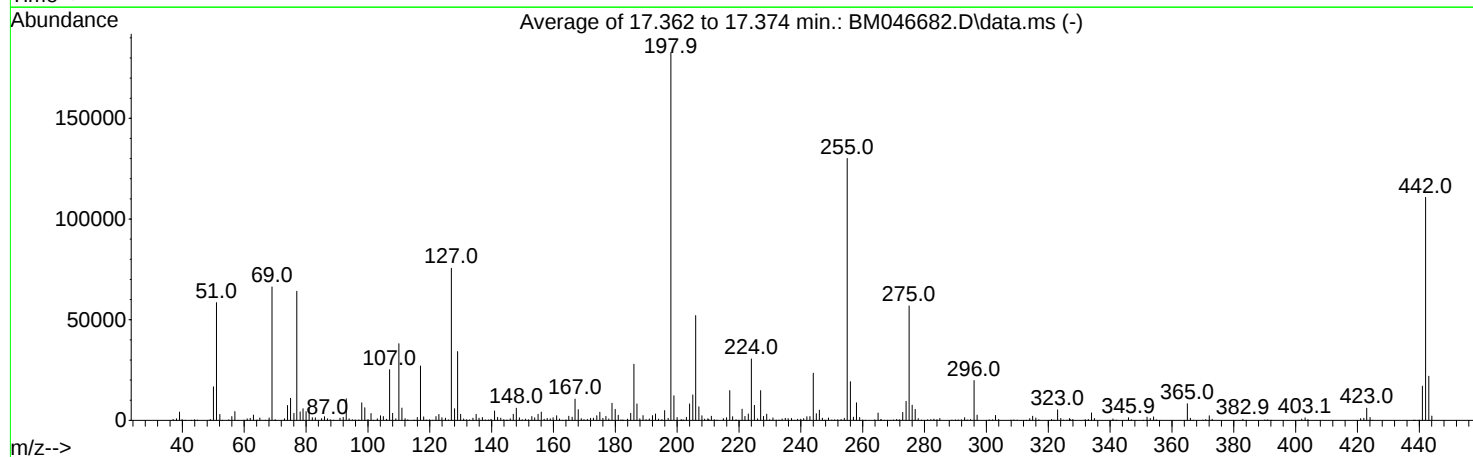


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071724\
Data File : BM046682.D
Acq On : 17 Jul 2024 23:53
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071724.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Jul 18 06:01:46 2024

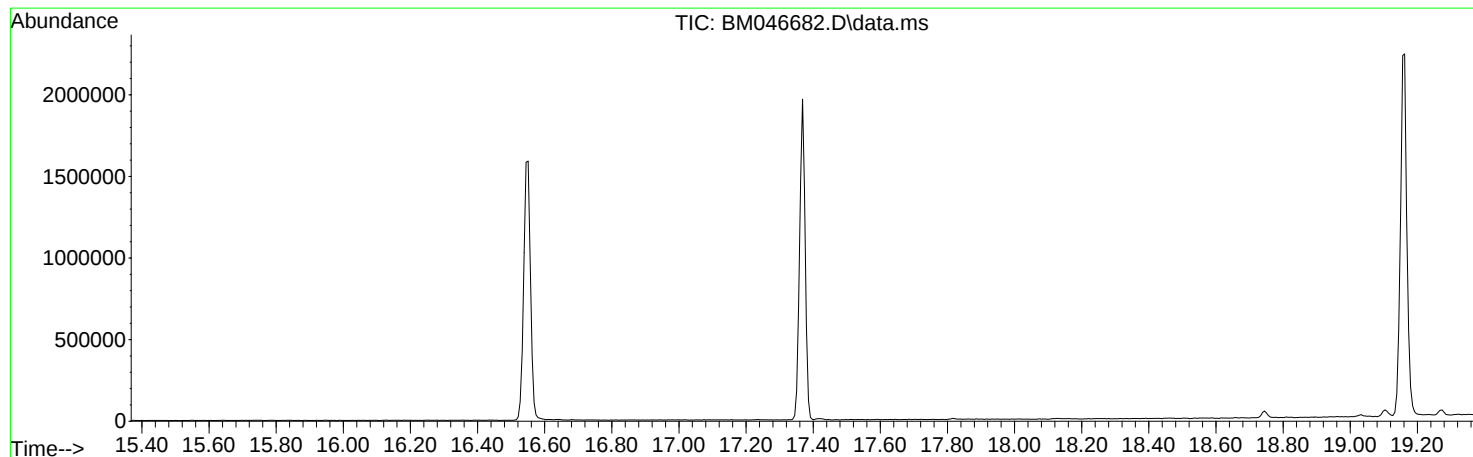




AutoFind: Scans 2444, 2445, 2446; Background Corrected with Scan 2437

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.0	58483	PASS
68	69	0.00	2	1.8	1179	PASS
69	198	0.00	100	36.3	66251	PASS
70	69	0.00	2	0.4	234	PASS
127	198	10	80	41.4	75555	PASS
197	198	0.00	2	0.6	1025	PASS
198	198	100	100	100.0	182699	PASS
199	198	5	9	6.7	12276	PASS
275	198	10	60	31.1	56824	PASS
365	198	1	100	4.5	8262	PASS
441	198	0.01	100	9.3	16999	PASS
442	442	50	100	100.0	110776	PASS
443	442	15	24	19.8	21953	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071724\
Data File : BM046682.D
Acq On : 17 Jul 2024 23:53
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jul 18 06:27:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 18 06:01:46 2024
Response via : Initial Calibration

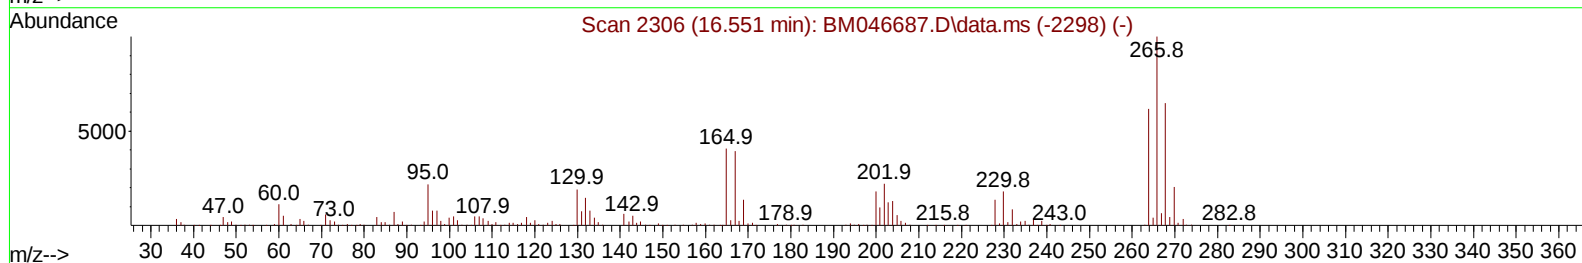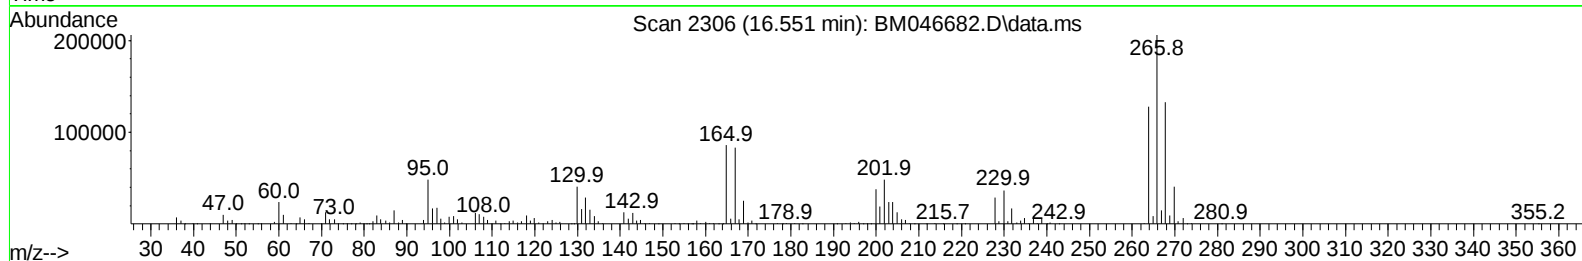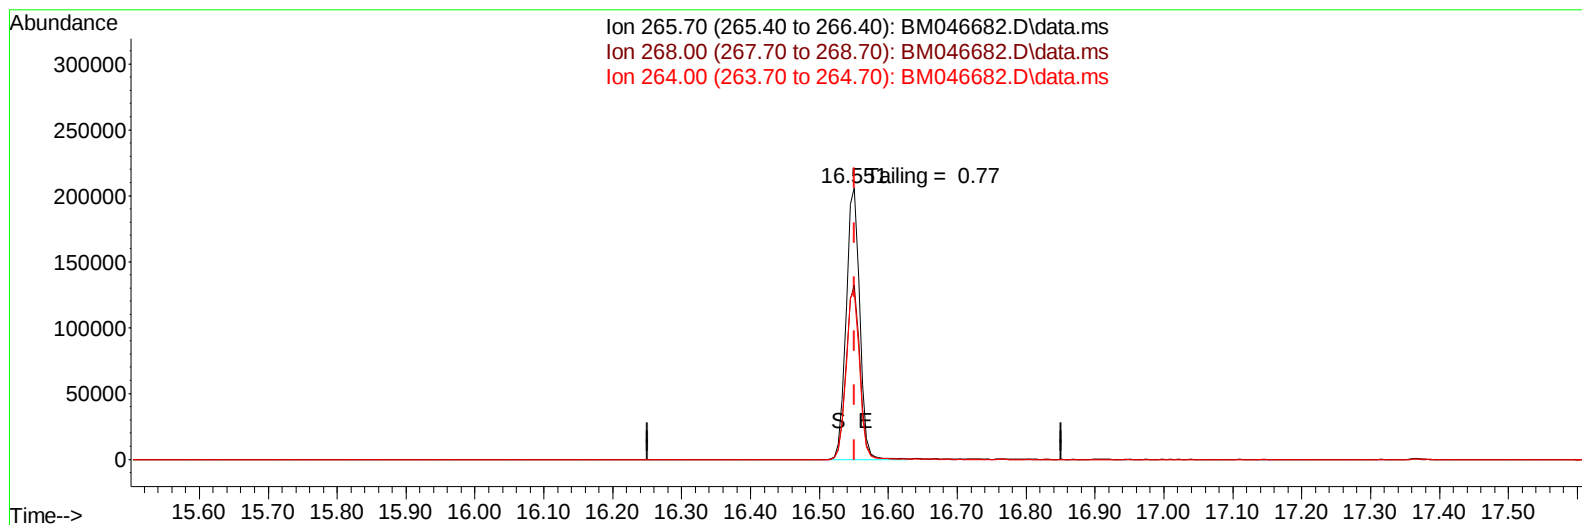

TIC: BM046682.D\data.ms

(70) Pentachlorophenol (C)

16.551min (-0.000) 0.00 ng




response 280843

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.80	64.36
264.00	61.80	61.98
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071724\
Data File : BM046682.D
Acq On : 17 Jul 2024 23:53
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jul 18 06:27:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM071724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 18 06:01:46 2024
Response via : Initial Calibration

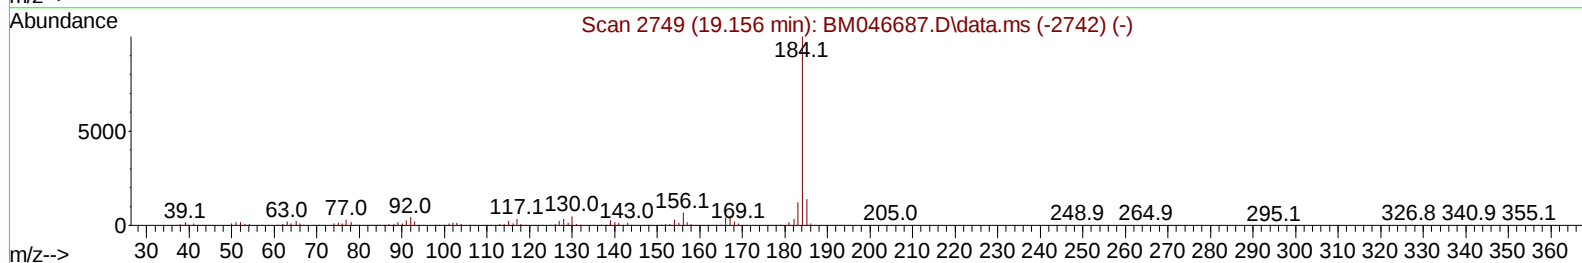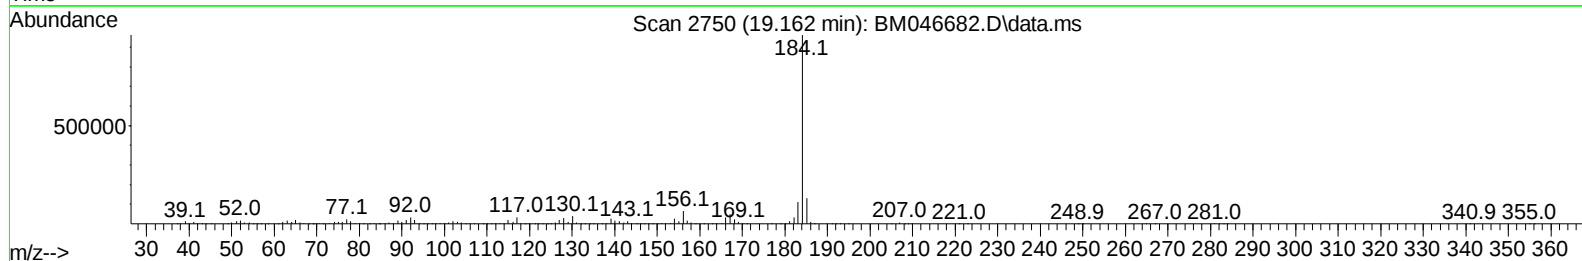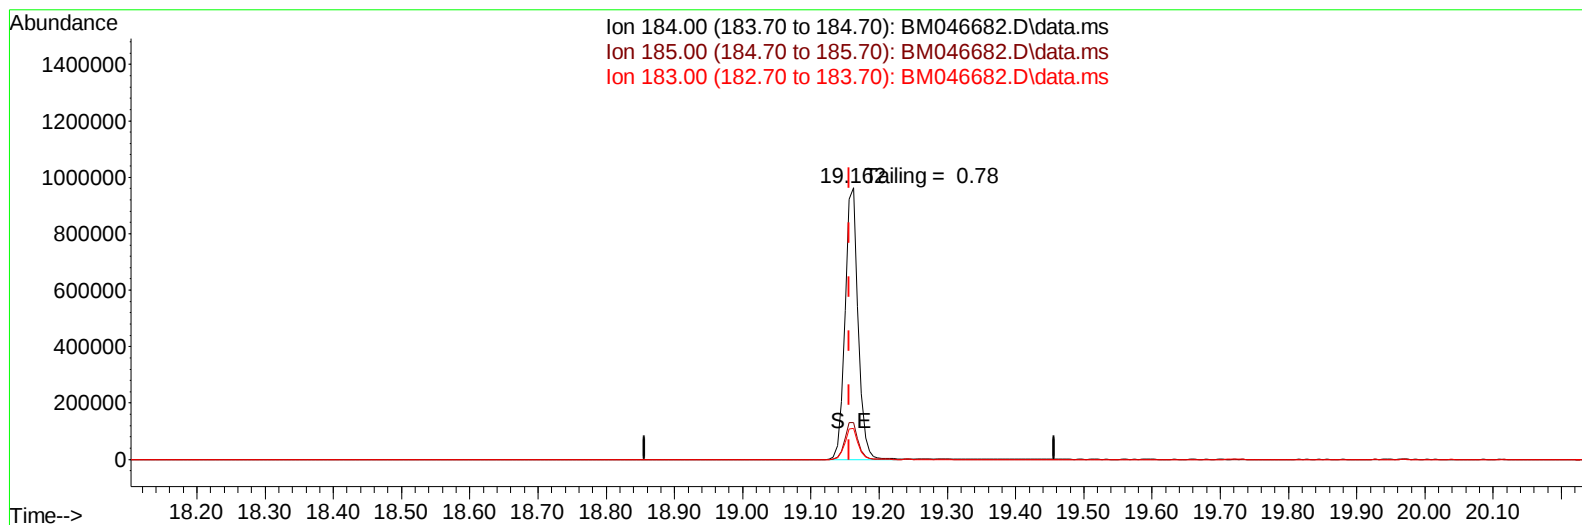

TIC: BM046682.D\data.ms

(77) Benzidine

19.162min (+ 0.006) 349805.78 ng

response 1266936

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	13.69
183.00	12.30	11.50
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/17/2024	BNA_M	<u>BM046682.D</u>
Compound Name	Response	Retention Time
DDT	480294	20.403
DDD	166773	19.962
DDE	1449	19.456
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
168222	648516	25.94

Instrument :
BNA_M
ClientSampleId :
DFTPP