
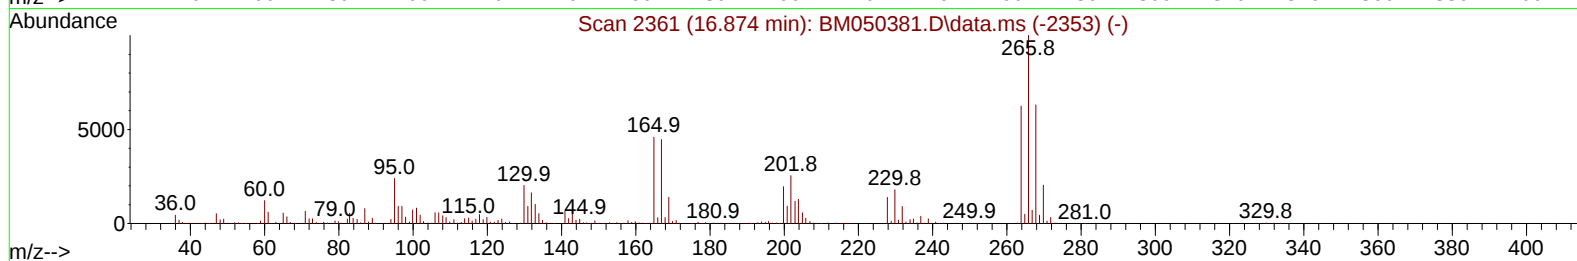
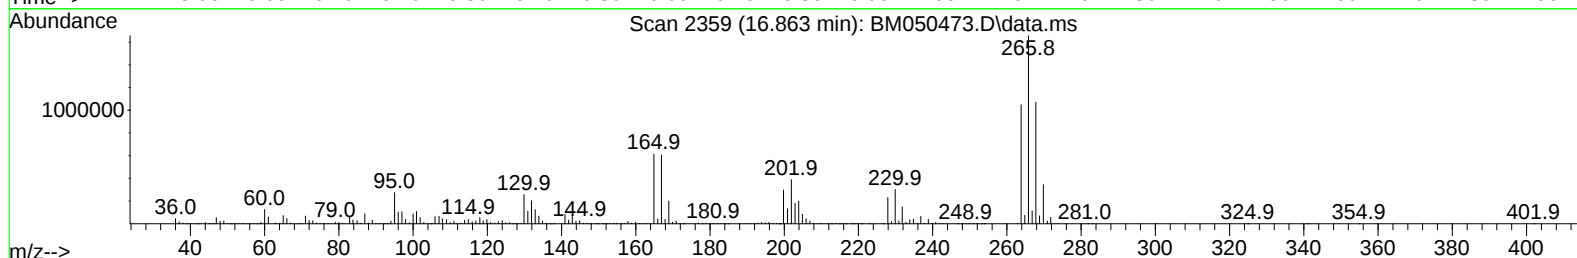


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071725\
Data File : BM050473.D
Acq On : 17 Jul 2025 13:02
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 17 16:24:15 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM070925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 17 16:20:15 2025
Response via : Initial Calibration

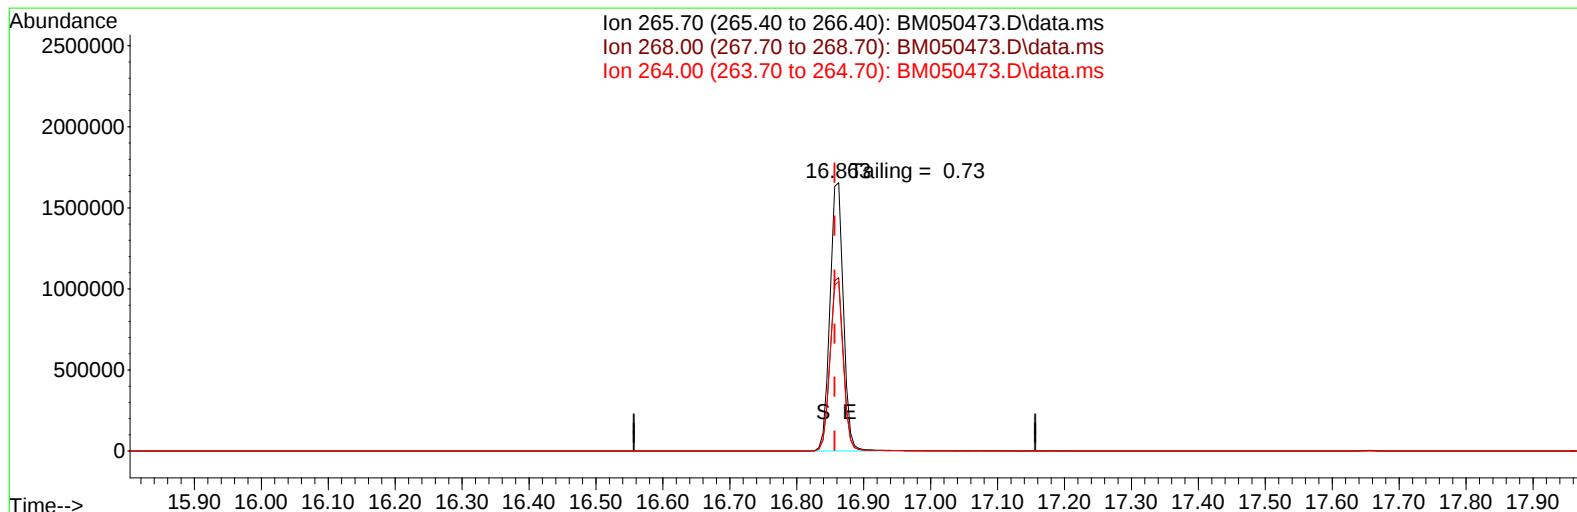

TIC: BM050473.D\data.ms

(70) Pentachlorophenol (C)




16.863min (+ 0.006) 343417.56 ng

response 2320091

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	64.56
264.00	62.40	63.28
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM071725\
Data File : BM050473.D
Acq On : 17 Jul 2025 13:02
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 17 16:24:15 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM070925.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 17 16:20:15 2025
Response via : Initial Calibration

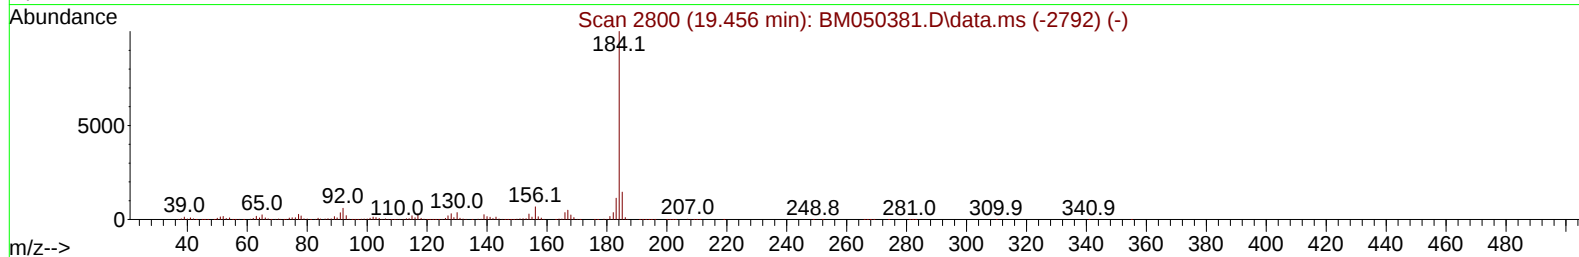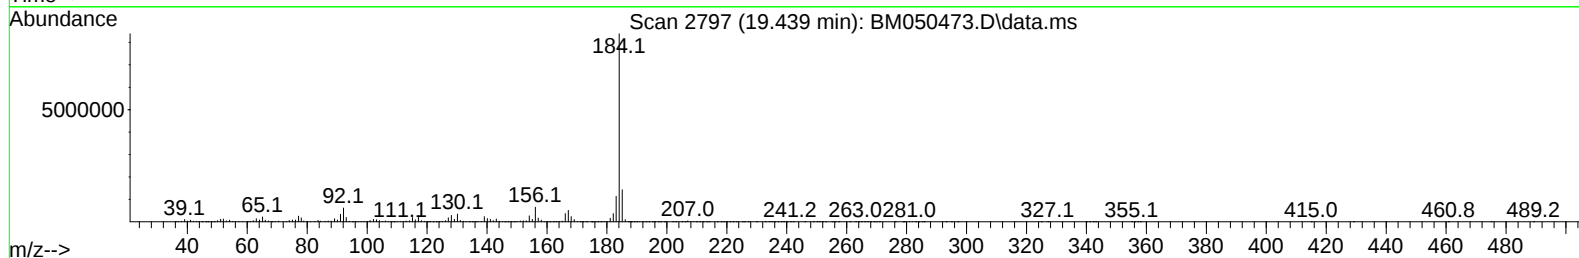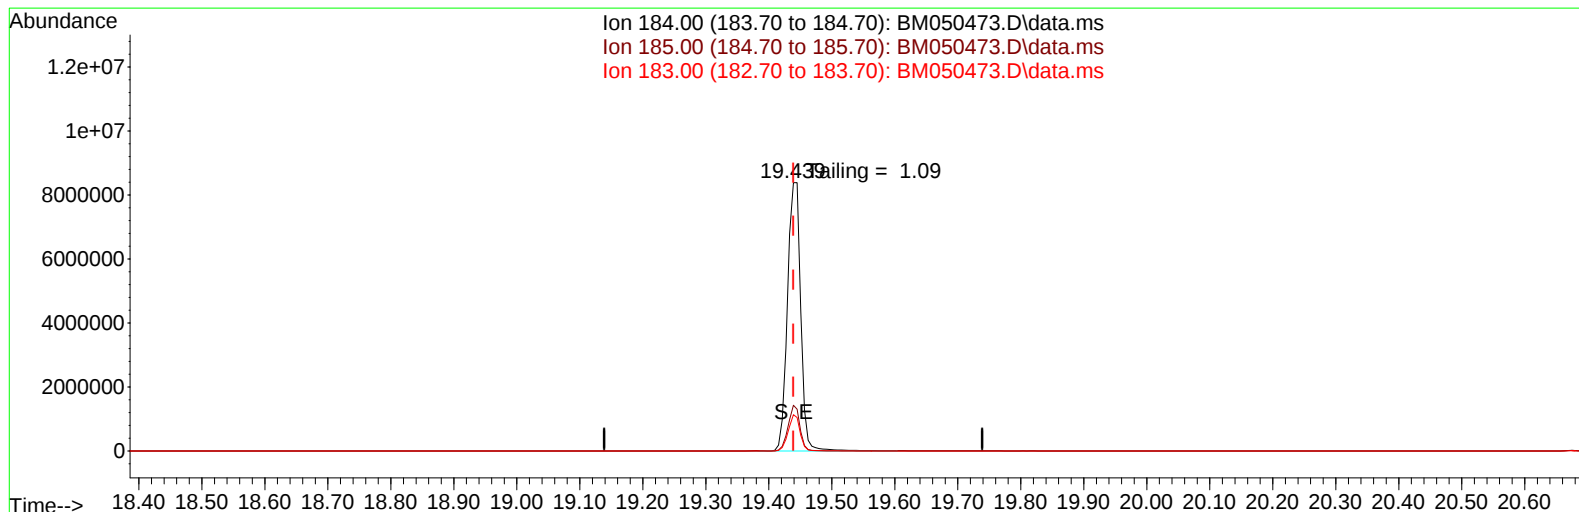

TIC: BM050473.D\data.ms

(77) Benzidine**19.439min (+ 0.000) 121383.09 ng****response 12309874**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	17.04
183.00	11.30	13.56#
0.00	0.00	0.00