


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM071919\
Data File : BM021557.D
Acq On : 19 Jul 2019 14:36
Operator : HP/JU
Sample : DFTPP28
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Integration File: LSCINT.P

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM070819MA.M
Title : SVOA CALIBRATION
Last Update : Sat Jul 20 05:03:12 2019

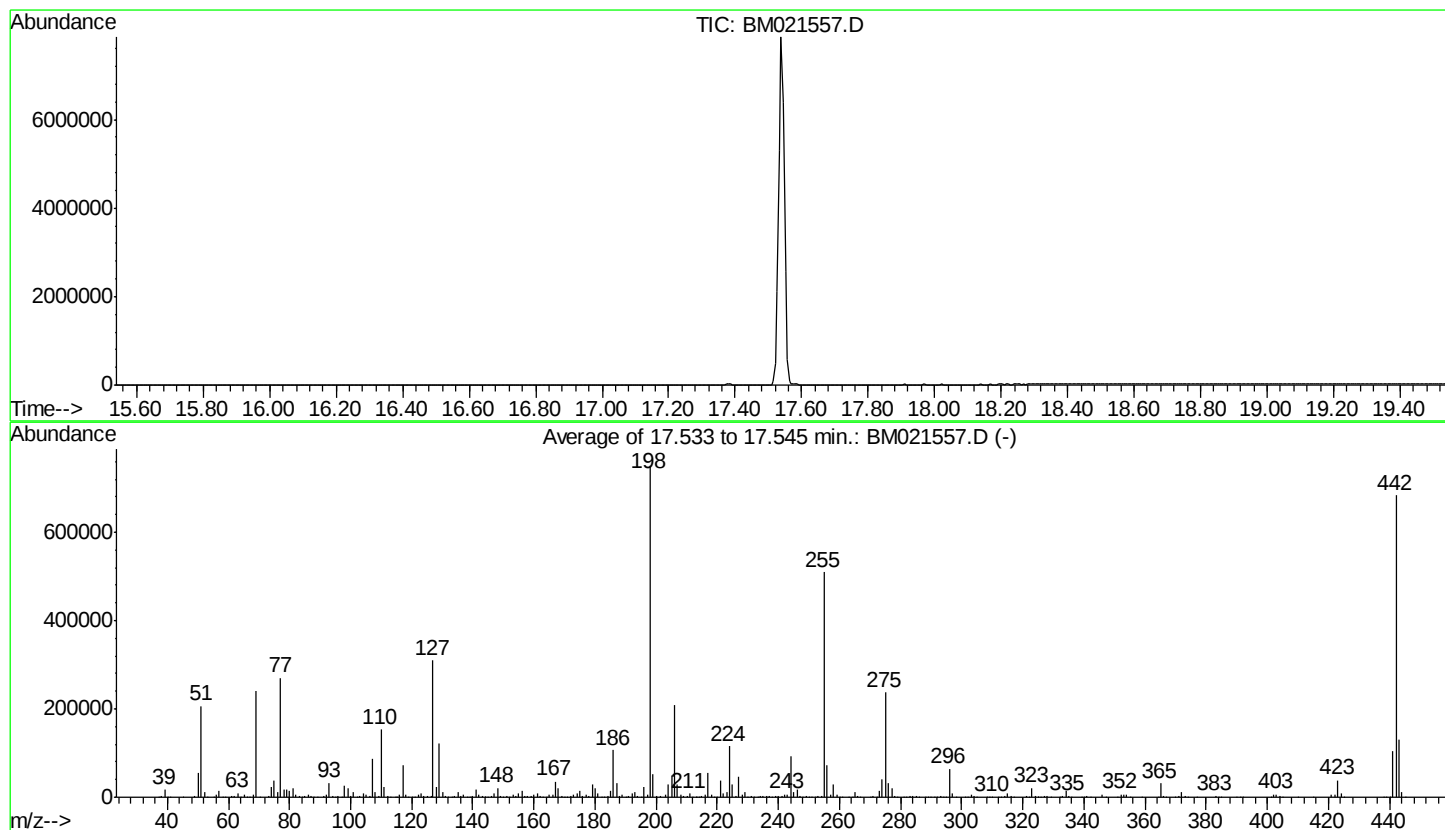

AutoFind: Scans 2473, 2474, 2475; Background Corrected with Scan 2467

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.6	207018	PASS
68	69	0.00	2	1.9	4601	PASS
69	198	0.00	100	32.1	241301	PASS
70	69	0.00	2	0.5	1237	PASS
127	198	10	80	41.2	309034	PASS
197	198	0.00	2	0.7	4921	PASS
198	198	100	100	100.0	750805	PASS
199	198	5	9	6.8	51306	PASS
275	198	10	60	31.6	237354	PASS
365	198	1	100	4.1	30544	PASS
441	198	0.01	100	14.1	105690	PASS
442	198	50	100	91.0	683008	PASS
443	442	15	24	19.2	130973	PASS