

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM071919\
 Data File : BM021566.D
 Acq On : 19 Jul 2019 20:14
 Operator : HP/JU
 Sample : K3823-08
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A52K8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM070819MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.887	659	663	674	rVB	152655	276666	5.66%	0.729%
2	7.057	687	692	703	rVB	479071	756626	15.48%	1.994%
3	7.245	718	724	731	rBV	590536	914062	18.70%	2.409%
4	7.710	797	803	812	rBV	519117	827343	16.92%	2.180%
5	8.416	917	923	935	rVB	424043	698571	14.29%	1.841%
6	8.875	994	1001	1009	rBV	639373	1053884	21.56%	2.777%
7	9.586	1116	1122	1133	rVB	497652	821158	16.80%	2.164%
8	10.122	1206	1213	1229	rBV	718321	1341740	27.45%	3.536%
9	10.492	1269	1276	1284	rVB	680839	1131560	23.15%	2.982%
10	10.663	1300	1305	1316	rBV	44445	94991	1.94%	0.250%
11	11.851	1503	1507	1514	rVB2	4923	6145	0.13%	0.016%
12	12.104	1545	1550	1557	rBV2	7779	15309	0.31%	0.040%
13	13.716	1820	1824	1828	rBV3	3321	6893	0.14%	0.018%
14	13.769	1828	1833	1839	rVV	1375359	2051391	41.96%	5.406%
15	13.821	1839	1842	1852	rVB	106553	147547	3.02%	0.389%
16	14.051	1874	1881	1894	rBV	1669940	2506190	51.26%	6.605%
17	14.357	1926	1933	1941	rBV2	1001728	1463407	29.93%	3.856%
18	14.427	1941	1945	1955	rVB7	7949	18925	0.39%	0.050%
19	14.598	1967	1974	1987	rBV2	49196	124281	2.54%	0.328%
20	15.110	2057	2061	2066	rBV	16857	26098	0.53%	0.069%
21	15.198	2070	2076	2079	rBV3	4856	6079	0.12%	0.016%
22	15.351	2096	2102	2113	rBV	2339001	3410754	69.77%	8.988%
23	15.492	2119	2126	2138	rBV	448920	683432	13.98%	1.801%
24	15.592	2138	2143	2148	rVB2	20172	29560	0.60%	0.078%
25	15.827	2180	2183	2187	rVV	7750	10595	0.22%	0.028%
26	15.868	2187	2190	2196	rVB2	7374	11673	0.24%	0.031%
27	16.098	2224	2229	2232	rVV2	6770	9967	0.20%	0.026%
28	16.139	2232	2236	2240	rVV3	6789	9102	0.19%	0.024%
29	16.186	2240	2244	2248	rVV	11241	14678	0.30%	0.039%
30	16.245	2248	2254	2261	rVV3	18392	33631	0.69%	0.089%
31	16.310	2261	2265	2268	rVV3	10939	16132	0.33%	0.043%
32	16.351	2269	2272	2277	rVB3	6482	8652	0.18%	0.023%
33	16.404	2277	2281	2282	rBV3	5372	6466	0.13%	0.017%
34	16.504	2294	2298	2305	rVB5	11673	23271	0.48%	0.061%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM071919\
 Data File : BM021566.D
 Acq On : 19 Jul 2019 20:14
 Operator : HP/JU
 Sample : K3823-08
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A52K8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM070819MA.M
 Title : SVOA CALIBRATION

35	16.580	2305	2311	2314	rBV	10757	16892	0.35%	0.045%
36	16.645	2320	2322	2328	rVB3	6646	9056	0.19%	0.024%
37	16.704	2328	2332	2339	rBV6	4225	9527	0.19%	0.025%
38	16.898	2361	2365	2368	rBV2	4945	6939	0.14%	0.018%
39	17.109	2394	2401	2411	rBV	1249911	1781956	36.45%	4.696%
40	17.209	2411	2418	2429	rVV	2349375	3467544	70.93%	9.138%
41	17.998	2548	2552	2561	rBV3	60660	102297	2.09%	0.270%
42	19.139	2742	2746	2752	rBV	26825	37665	0.77%	0.099%
43	19.286	2767	2771	2776	rBV5	22670	34001	0.70%	0.090%
44	19.392	2786	2789	2794	rVB	20026	22088	0.45%	0.058%
45	19.503	2802	2808	2816	rBV	3219779	4288983	87.73%	11.303%
46	21.003	3060	3063	3071	rBV6	66143	117246	2.40%	0.309%
47	21.297	3108	3113	3121	rBV	1710741	2219447	45.40%	5.849%
48	23.403	3465	3471	3485	rVB	2697753	4888708	100.00%	12.883%
49	23.544	3489	3495	3508	rVB	1221047	2387551	48.84%	6.292%


Sum of corrected areas: 37946679

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM071919\
Data File : BM021566.D
Acq On : 19 Jul 2019 20:14
Operator : HP/JU
Sample : K3823-08
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A52K8

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM070819MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

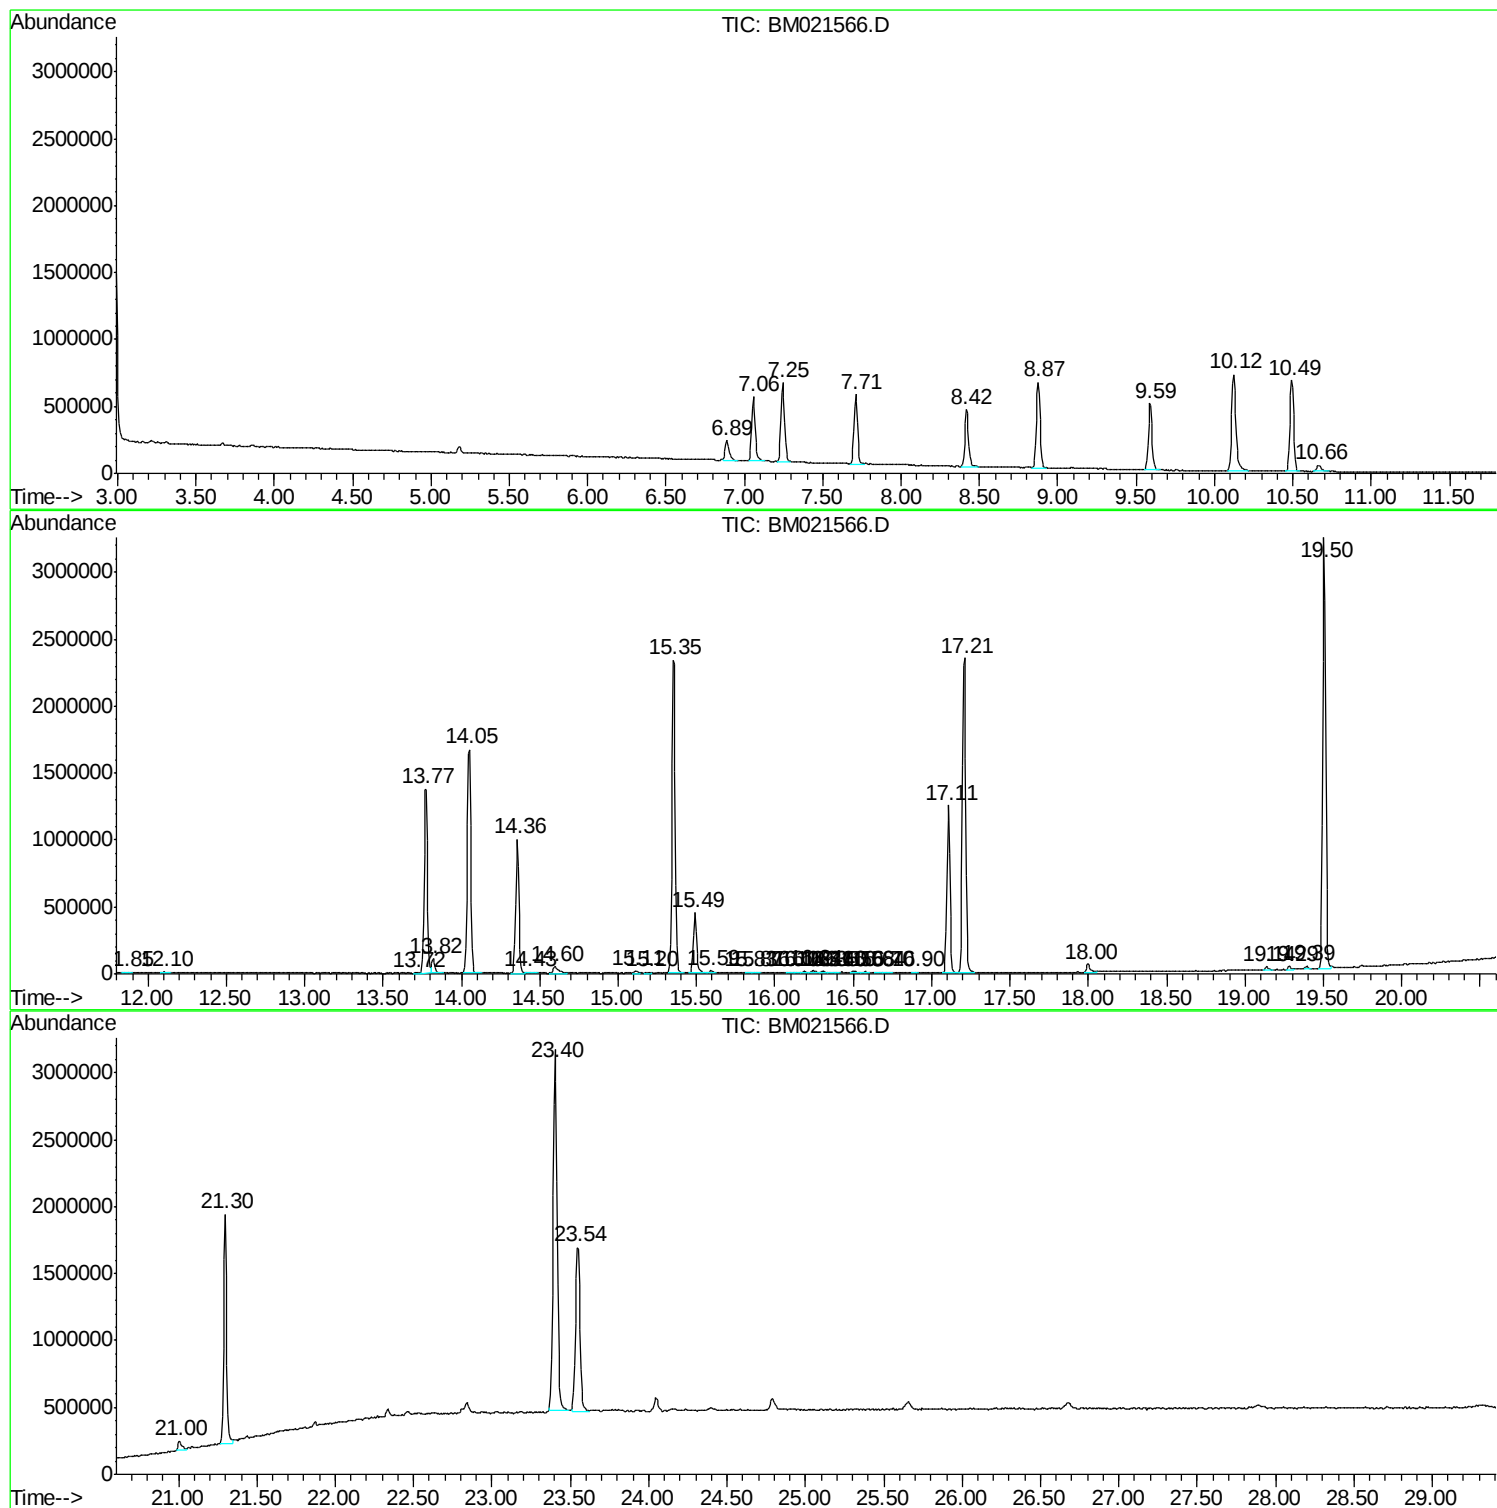

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM071919\
Data File : BM021566.D
Acq On : 19 Jul 2019 20:14
Operator : HP/JU
Sample : K3823-08
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A52K8

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM070819MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM071919\
Data File : BM021566.D
Acq On : 19 Jul 2019 20:14
Operator : HP/JU
Sample : K3823-08
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A52K8

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM070819MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc