

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM071919\
 Data File : BM021570.D
 Acq On : 19 Jul 2019 22:41
 Operator : HP/JU
 Sample : PB121510BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK10

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM070819MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.887	657	663	675	rVB	617683	999079	23.96%	2.682%
2	7.057	687	692	700	rBV	466416	741841	17.79%	1.992%
3	7.245	718	724	738	rVB	692456	1113088	26.69%	2.988%
4	7.710	797	803	811	rVB	535608	843804	20.23%	2.265%
5	8.416	917	923	938	rVB	750566	1254514	30.08%	3.368%
6	8.875	995	1001	1016	rVB	623814	1058131	25.37%	2.841%
7	9.586	1116	1122	1134	rVB	463977	798557	19.15%	2.144%
8	10.122	1206	1213	1229	rBV	753558	1336754	32.05%	3.589%
9	10.492	1270	1276	1286	rVB	700911	1153486	27.66%	3.097%
10	10.645	1295	1302	1322	rBV	634282	1275747	30.59%	3.425%
11	12.110	1546	1551	1558	rVB3	7891	14843	0.36%	0.040%
12	13.774	1827	1834	1846	rBV	1347551	1865772	44.74%	5.009%
13	14.045	1874	1880	1895	rBV	1558145	2313903	55.48%	6.212%
14	14.357	1926	1933	1942	rBV2	1004529	1467629	35.19%	3.940%
15	14.580	1965	1971	1992	rBV	274827	638190	15.30%	1.713%
16	15.357	2096	2103	2114	rBV	1989323	2873600	68.90%	7.715%
17	15.492	2120	2126	2140	rBV	350830	550219	13.19%	1.477%
18	15.592	2140	2143	2150	rVB2	19222	26554	0.64%	0.071%
19	16.139	2232	2236	2240	rVB3	5860	8369	0.20%	0.022%
20	16.898	2360	2365	2370	rBV4	3851	6064	0.15%	0.016%
21	17.109	2395	2401	2407	rBV	1241872	1744664	41.83%	4.684%
22	17.209	2411	2418	2433	rVV	2205643	3069341	73.59%	8.240%
23	19.145	2743	2747	2751	rBV3	14416	19264	0.46%	0.052%
24	19.392	2786	2789	2794	rBV	12462	18513	0.44%	0.050%
25	19.503	2802	2808	2818	rBV	2584057	3631847	87.08%	9.750%
26	21.297	3108	3113	3120	rBV	1542451	2046299	49.06%	5.494%
27	23.403	3464	3471	3486	rBV	2302487	4170610	100.00%	11.197%
28	23.550	3490	3496	3509	rVB2	1105659	2207496	52.93%	5.926%


Sum of corrected areas: 37248178

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM071919\
Data File : BM021570.D
Acq On : 19 Jul 2019 22:41
Operator : HP/JU
Sample : PB121510BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK10

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM070819MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

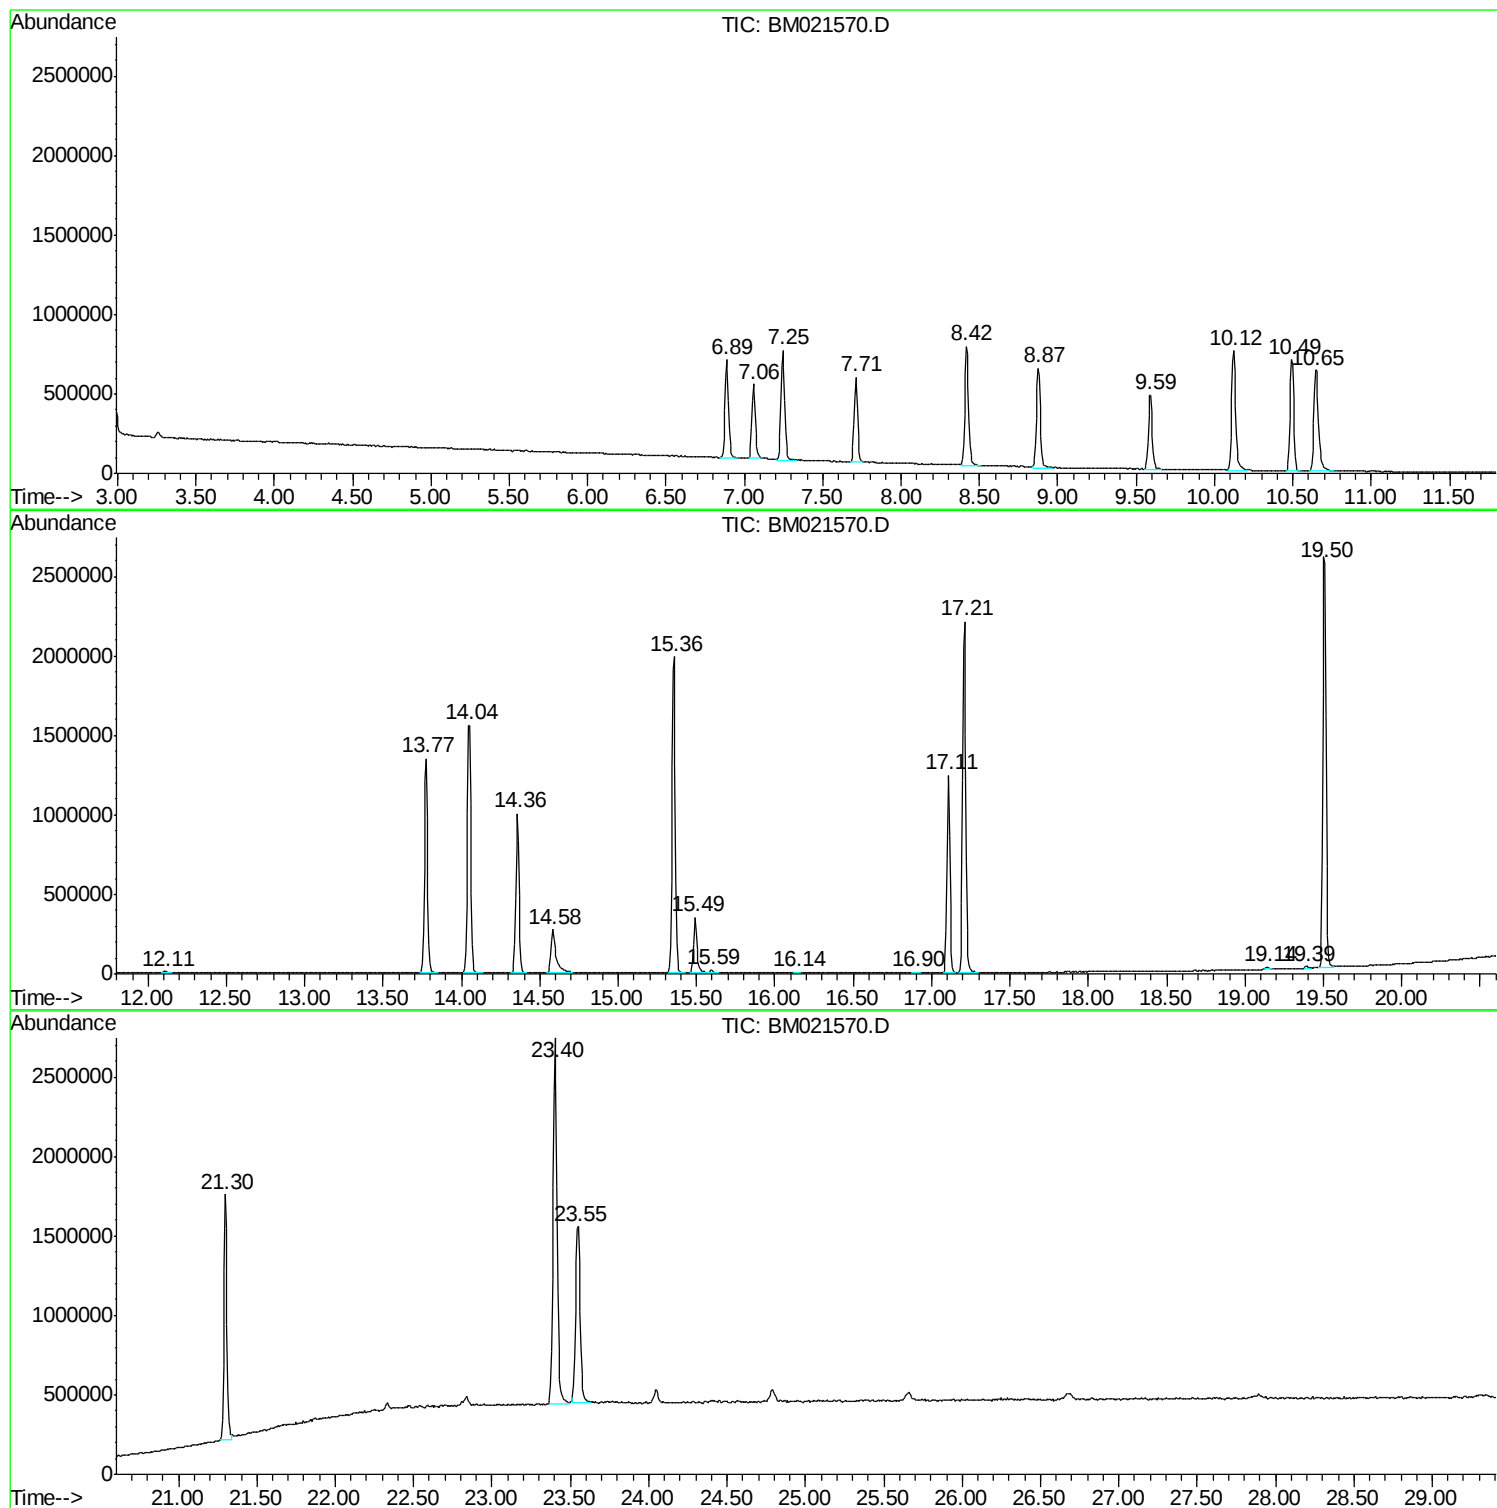

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM071919\
Data File : BM021570.D
Acq On : 19 Jul 2019 22:41
Operator : HP/JU
Sample : PB121510BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK10

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM070819MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM071919\
Data File : BM021570.D
Acq On : 19 Jul 2019 22:41
Operator : HP/JU
Sample : PB121510BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK10

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM070819MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc