

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM071919\
 Data File : BM021574.D
 Acq On : 20 Jul 2019 02:32
 Operator : HP/JU
 Sample : K3823-11
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A52L8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM070819MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.893	659	664	674	rVB	137586	253588	5.19%	0.662%
2	7.057	687	692	700	rBV	416987	657418	13.45%	1.716%
3	7.245	719	724	741	rVB	527931	844863	17.28%	2.206%
4	7.710	797	803	813	rVB	605013	963817	19.72%	2.516%
5	8.422	918	924	935	rVB	386186	654590	13.39%	1.709%
6	8.875	995	1001	1011	rBV	568128	933858	19.10%	2.438%
7	9.592	1116	1123	1135	rVB	441732	745520	15.25%	1.946%
8	10.122	1206	1213	1230	rBV	632462	1205561	24.66%	3.148%
9	10.492	1269	1276	1286	rBV	793339	1321652	27.04%	3.451%
10	10.669	1298	1306	1317	rBV	43531	98988	2.02%	0.258%
11	12.098	1545	1549	1557	rVB4	7371	13594	0.28%	0.035%
12	13.774	1827	1834	1839	rBV	1390850	1921160	39.30%	5.016%
13	13.822	1839	1842	1850	rVB	82396	117297	2.40%	0.306%
14	14.045	1874	1880	1895	rBV	1461971	2249816	46.02%	5.874%
15	14.357	1926	1933	1941	rBV2	1141049	1717862	35.14%	4.485%
16	14.421	1941	1944	1949	rBV2	19023	34153	0.70%	0.089%
17	14.598	1968	1974	1995	rVB2	51997	138867	2.84%	0.363%
18	15.110	2057	2061	2067	rBV	37543	54797	1.12%	0.143%
19	15.357	2096	2103	2117	rBV2	2112418	3176542	64.98%	8.294%
20	15.492	2120	2126	2137	rVV	473756	700974	14.34%	1.830%
21	15.598	2140	2144	2148	rVB	20148	25705	0.53%	0.067%
22	15.833	2180	2184	2187	rVV4	5936	7902	0.16%	0.021%
23	15.868	2187	2190	2196	rVB2	6384	8825	0.18%	0.023%
24	16.098	2226	2229	2232	rVV	6155	7018	0.14%	0.018%
25	16.139	2232	2236	2239	rVV3	6738	7973	0.16%	0.021%
26	16.186	2239	2244	2248	rVV	12879	15439	0.32%	0.040%
27	16.245	2248	2254	2260	rVB2	17247	31047	0.64%	0.081%
28	16.310	2260	2265	2268	rBV3	12986	18000	0.37%	0.047%
29	16.345	2268	2271	2277	rVB3	6120	9358	0.19%	0.024%
30	16.404	2277	2281	2282	rBV4	5407	5844	0.12%	0.015%
31	16.510	2294	2299	2306	rBV5	11877	22248	0.46%	0.058%
32	16.574	2306	2310	2314	rBV	9402	13751	0.28%	0.036%
33	16.645	2320	2322	2328	rVB2	5387	8636	0.18%	0.023%
34	16.704	2328	2332	2339	rBV6	3402	6558	0.13%	0.017%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM071919\
Data File : BM021574.D
Acq On : 20 Jul 2019 02:32
Operator : HP/JU
Sample : K3823-11
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A52L8

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM070819MA.M
Title : SVOA CALIBRATION

35	16.898	2360	2365	2371	rBV4	6722	10953	0.22%	0.029%
36	17.110	2394	2401	2409	rBV	1472578	2065160	42.25%	5.392%
37	17.210	2411	2418	2432	rVV	2437679	3471466	71.01%	9.064%
38	17.474	2458	2463	2466	rBV6	3347	5247	0.11%	0.014%
39	17.998	2547	2552	2561	rBV2	76418	111955	2.29%	0.292%
40	19.139	2743	2746	2754	rBV	25405	37059	0.76%	0.097%
41	19.280	2767	2770	2777	rBV4	28004	45414	0.93%	0.119%
42	19.392	2786	2789	2793	rVB	22265	23614	0.48%	0.062%
43	19.503	2802	2808	2817	rBV	3224032	4319314	88.36%	11.277%
44	21.003	3060	3063	3070	rBV4	68966	116129	2.38%	0.303%
45	21.297	3108	3113	3123	rBV	1899399	2531858	51.79%	6.610%
46	23.409	3465	3472	3482	rVB	2651568	4888507	100.00%	12.763%
47	23.550	3490	3496	3508	rVB2	1347015	2681520	54.85%	7.001%


Sum of corrected areas: 38301417

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM071919\
Data File : BM021574.D
Acq On : 20 Jul 2019 02:32
Operator : HP/JU
Sample : K3823-11
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A52L8

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM070819MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

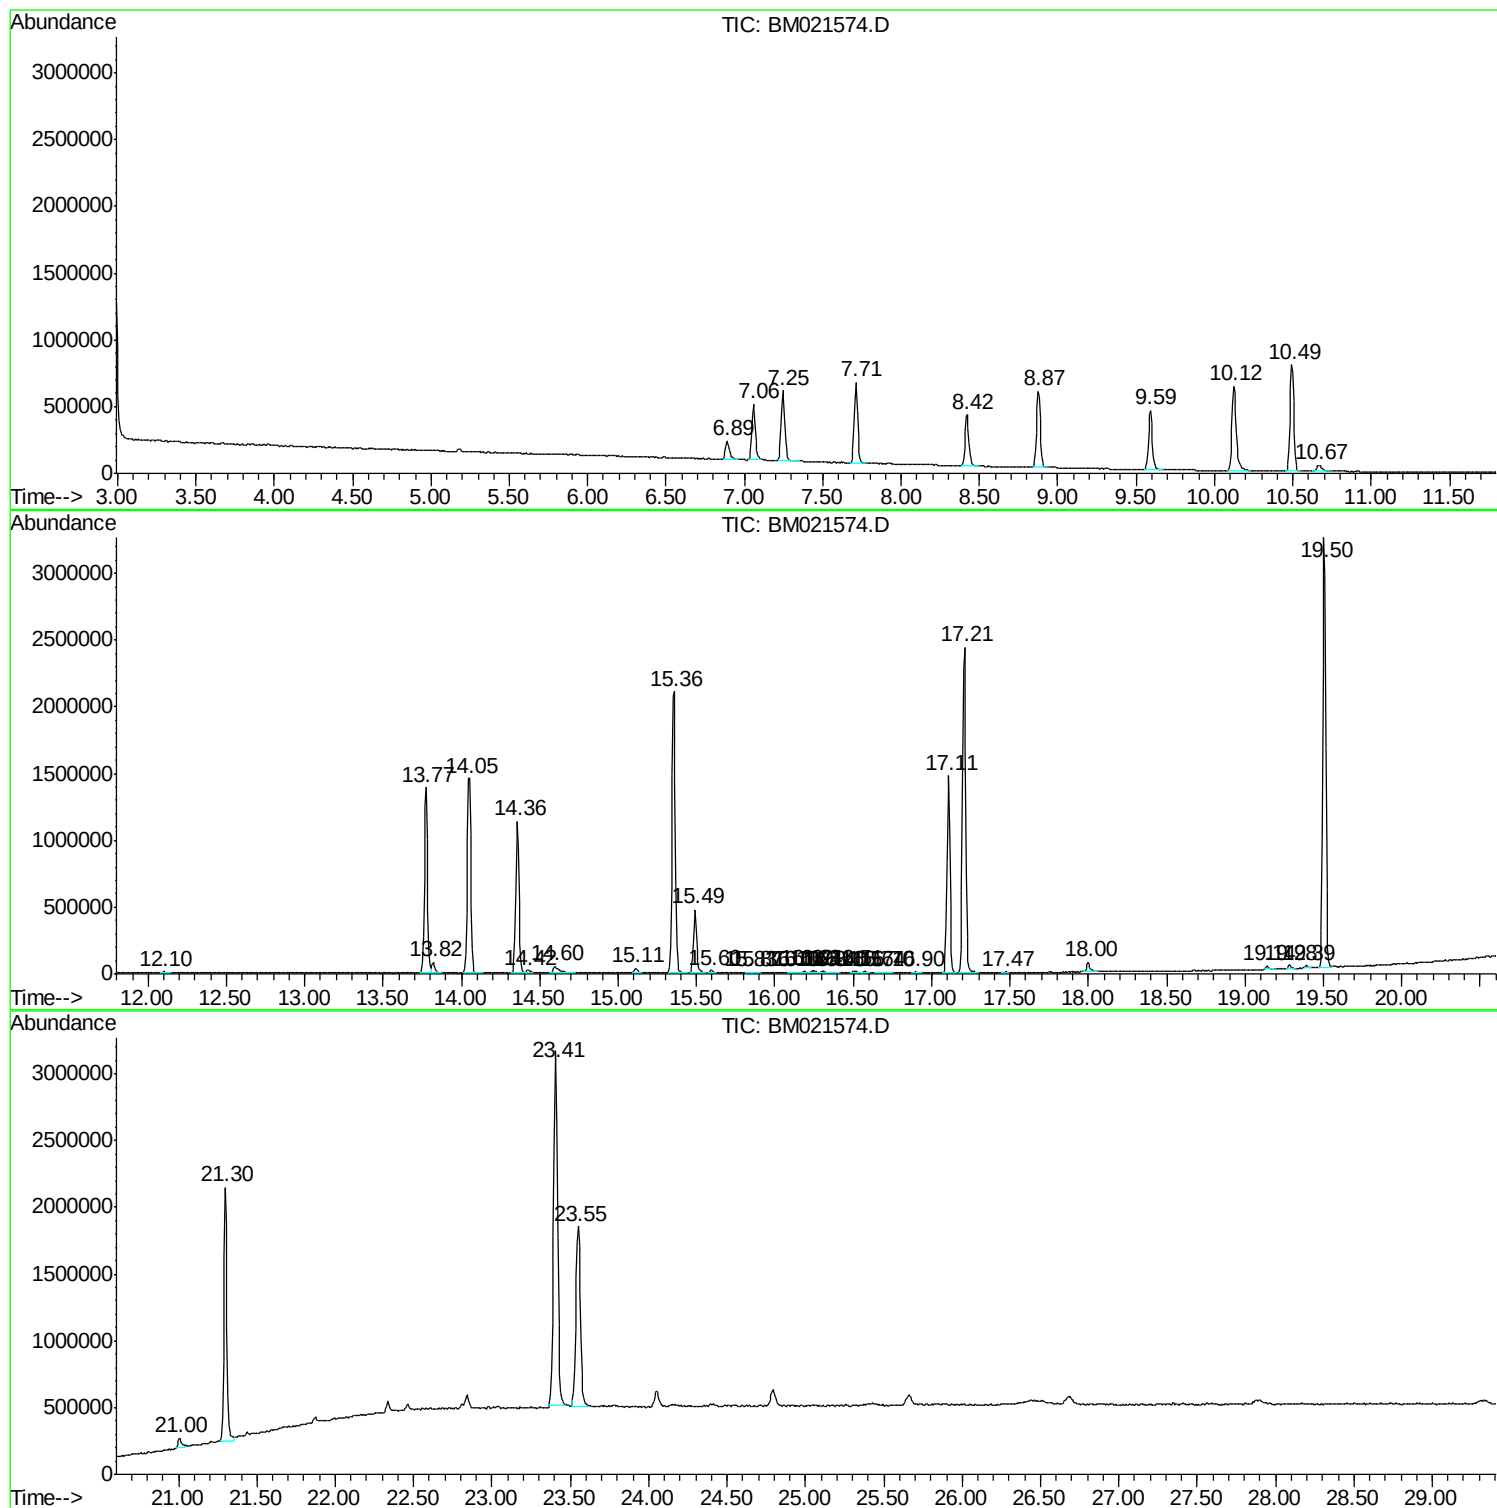

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM071919\
Data File : BM021574.D
Acq On : 20 Jul 2019 02:32
Operator : HP/JU
Sample : K3823-11
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A52L8

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM070819MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM071919\
Data File : BM021574.D
Acq On : 20 Jul 2019 02:32
Operator : HP/JU
Sample : K3823-11
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A52L8

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM070819MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc