


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072018\
 Data File : BM016012.D
 Acq On : 20 Jul 2018 10:40
 Operator : SJ/JU
 Sample : DFTPP32
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP32

Integration File: LSCINT.P

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM071318MA.M
 Title : SVOA CALIBRATION
 Last Update : Fri Jul 20 23:12:47 2018

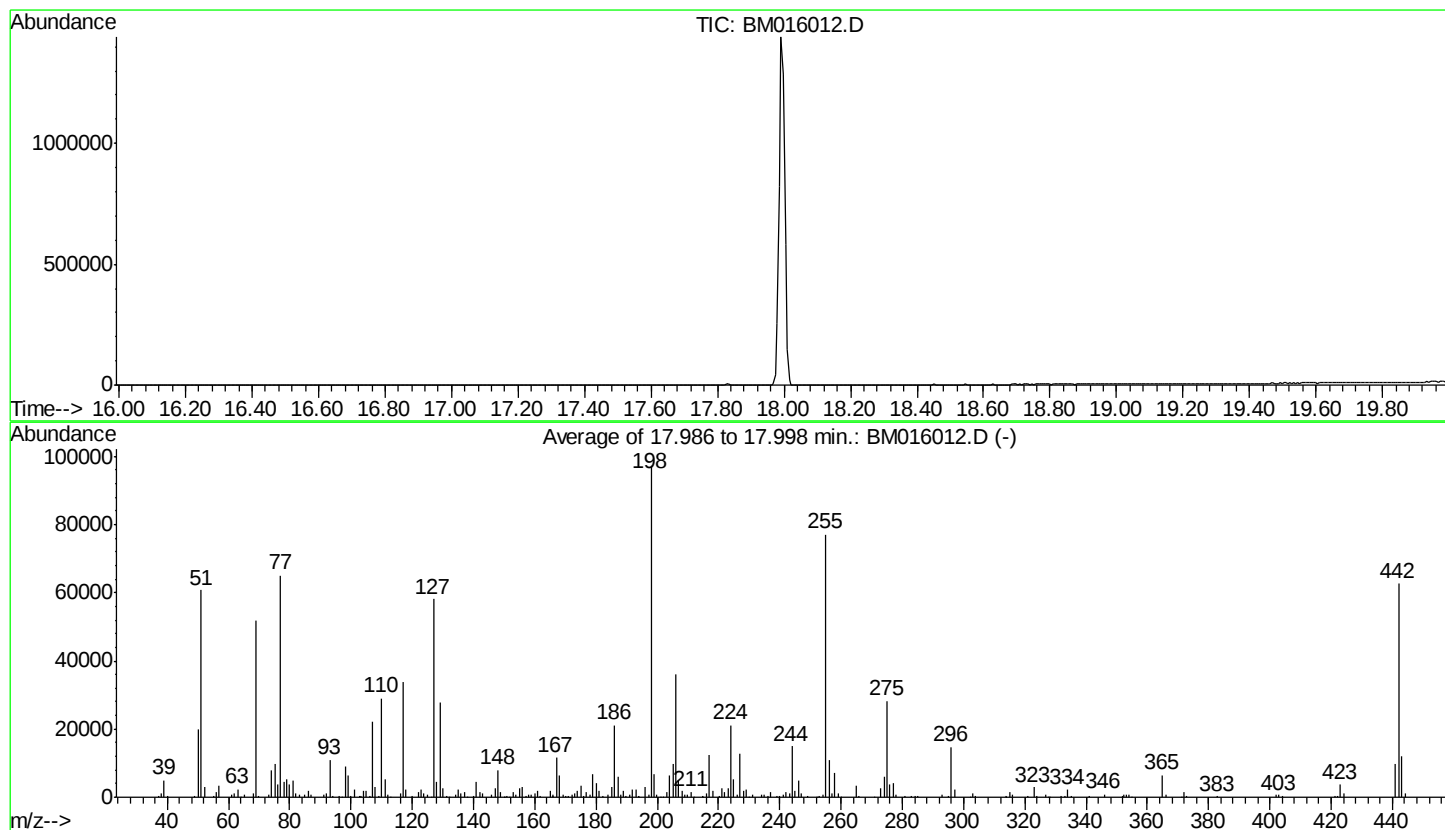

AutoFind: Scans 2499, 2500, 2501; Background Corrected with Scan 2494

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	62.5	60808	PASS
68	69	0.00	2	2.0	1041	PASS
69	198	0.00	100	53.1	51661	PASS
70	69	0.00	2	0.8	394	PASS
127	198	10	80	59.8	58157	PASS
197	198	0.00	2	0.8	762	PASS
198	198	100	100	100.0	97290	PASS
199	198	5	9	6.9	6740	PASS
275	198	10	60	29.0	28250	PASS
365	198	1	100	6.7	6485	PASS
441	198	0.01	100	10.2	9952	PASS
442	198	50	100	64.3	62594	PASS
443	442	15	24	19.1	11942	PASS

m/z	Abundance
37.00	330.0
38.00	1061.0
39.10	4285.0
40.00	365.0
50.10	15893.0
51.00	50152.0
52.10	2537.0
54.90	381.0
56.00	1499.0
57.00	2751.0
60.90	797.0
61.90	610.0
63.00	2131.0
65.00	701.0
67.90	975.0
69.00	40408.0
70.00	345.0
73.00	1049.0
74.00	6965.0
75.00	7780.0
76.00	3244.0
77.10	51832.0
78.00	3472.0
79.00	4386.0
80.00	3061.0
81.00	3867.0
82.00	921.0
83.00	605.0
85.00	495.0
86.00	1281.0
87.00	476.0
90.90	875.0
92.00	1139.0
93.00	8592.0
93.90	468.0
98.00	7532.0
99.00	5317.0
99.90	445.0
100.90	1923.0
102.90	645.0
104.00	1296.0
105.00	1164.0
105.90	458.0
107.00	17224.0
108.00	2490.0
109.10	366.0
110.00	21632.0
111.00	4101.0
111.90	423.0
116.10	1014.0
117.00	25624.0
118.00	1764.0
119.90	399.0
122.00	1276.0
123.00	2055.0
124.00	685.0
124.90	745.0
127.00	42928.0
128.00	3512.0
129.00	21176.0
130.00	2106.0
131.00	420.0
133.90	746.0
134.90	2000.0
135.90	885.0
137.00	1365.0
140.00	382.0
140.90	3415.0
142.00	1013.0
143.00	596.0
145.90	711.0
146.90	1685.0
148.00	6138.0
149.00	745.0
152.90	1190.0
153.90	690.0
155.00	1736.0
156.00	2192.0
157.10	423.0
158.00	541.0
158.90	593.0
160.00	902.0
161.00	1387.0
164.90	1155.0
165.90	914.0
167.00	8231.0
168.00	4756.0
169.00	516.0
171.00	325.0
172.00	488.0
173.00	715.0

Instrument :
BNA_M
ClientSampleId :
DFTPP32

173.90	1408.0
175.00	2309.0
176.10	530.0
177.00	1071.0
177.90	380.0
179.00	4948.0
179.90	3047.0
181.00	1451.0
183.90	452.0
185.00	2172.0
186.00	15017.0
187.00	4116.0
188.00	807.0
188.90	1073.0
190.90	676.0
191.90	1294.0
193.00	1572.0
193.80	361.0
196.00	1522.0
197.10	489.0
197.90	64760.0
198.90	4620.0
199.90	445.0
203.00	959.0
204.00	4138.0
205.00	6584.0
206.00	23488.0
207.00	3855.0
208.00	1280.0
208.90	590.0
210.00	533.0
211.10	977.0
214.80	389.0
215.90	784.0
217.00	9241.0
217.90	1086.0
220.90	1853.0
222.00	647.0
222.90	1389.0
224.00	13725.0
225.00	3382.0
226.00	431.0
227.00	7942.0
227.90	1019.0
228.90	1389.0
231.00	418.0
234.10	417.0
234.90	576.0
236.90	1228.0
240.00	351.0
240.90	347.0
242.10	785.0
243.00	776.0
244.00	9393.0
245.00	1273.0
246.00	3123.0
246.90	581.0
254.00	420.0
255.00	48096.0
256.00	7517.0
256.90	827.0
258.00	4598.0
258.90	544.0
264.90	2175.0
272.90	1580.0
274.00	3827.0
275.00	16167.0
276.00	2419.0
277.00	2194.0
278.00	726.0
280.90	417.0
285.00	419.0
293.00	475.0
296.00	8553.0
296.90	1574.0
303.00	824.0
313.80	356.0
315.00	993.0
316.00	315.0
323.00	1848.0
326.90	531.0
334.00	1266.0
346.00	399.0
351.90	635.0
353.00	466.0
354.00	473.0
365.00	3376.0
366.00	551.0
371.90	1058.0
402.00	329.0
402.90	526.0
421.10	370.0
423.00	1620.0
424.00	708.0
441.00	4438.0

Instrument :
BNA_M
ClientSampleId :
DFTPP32

442.1028888.0

443.006210.0

444.00448.0

Instrument :
BNA_M
ClientSampleId :
DFTPP32

m/z	Abundance
37.00	491.0
38.00	1249.0
39.10	6172.0
40.00	462.0
49.00	819.0
50.00	24368.0
51.10	74776.0
52.00	3607.0
55.00	528.0
56.00	1792.0
57.00	3983.0
61.00	945.0
62.00	1300.0
63.00	2601.0
64.10	394.0
65.00	1116.0
68.00	1269.0
69.00	65384.0
69.90	458.0
73.00	1512.0
74.00	8994.0
75.00	12102.0
76.10	4349.0
77.00	79104.0
78.10	6491.0
79.00	7006.0
80.00	4527.0
81.00	6303.0
81.90	1459.0
83.00	926.0
85.00	901.0
86.00	2563.0
87.00	902.0
91.00	1010.0
92.00	1571.0
93.00	13409.0
93.90	661.0
96.00	461.0
98.00	11044.0
99.00	8152.0
99.90	565.0
101.00	2752.0
102.90	881.0
104.00	2434.0
105.00	2396.0
106.00	664.0
107.00	26584.0
108.00	3656.0
109.10	749.0
110.00	36152.0
111.00	6456.0
111.90	861.0
116.00	1710.0
117.00	42320.0
118.00	2772.0
122.00	2114.0
123.00	2686.0
123.80	1244.0
124.90	1018.0
126.10	450.0
127.00	71240.0
128.00	5244.0
129.00	33768.0
130.00	3212.0
131.00	689.0
131.90	353.0
134.00	974.0
134.90	2795.0
136.00	1580.0
137.00	1969.0
140.00	602.0
140.90	5303.0
141.90	1752.0
142.90	1312.0
146.00	1057.0
147.00	3360.0
148.00	9353.0
149.00	1670.0
149.90	519.0
151.00	569.0
152.90	1703.0
154.00	959.0
155.00	3238.0
156.00	3912.0
156.90	620.0
157.90	988.0
158.90	803.0
160.00	1510.0
161.00	1992.0
161.90	547.0
164.90	2354.0

Instrument :
BNA_M
ClientSampleId :
DFTPP32

166.10	1310.0
167.00	14191.0
168.00	7291.0
169.10	958.0
170.00	435.0
171.00	466.0
172.00	1045.0
173.00	1295.0
173.90	1783.0
175.00	3936.0
176.00	709.0
176.90	1986.0
177.90	679.0
178.90	7603.0
180.00	4821.0
180.90	2422.0
182.00	453.0
184.00	701.0
185.00	3454.0
186.00	25768.0
187.00	7708.0
188.00	991.0
189.00	2048.0
189.90	433.0
190.90	1065.0
191.90	2858.0
193.00	2985.0
194.10	584.0
196.00	3832.0
197.00	962.0
197.90	119544.0
198.90	8097.0
200.00	852.0
203.00	1940.0
204.00	7243.0
205.00	12204.0
206.00	43976.0
207.00	6254.0
208.00	2219.0
208.90	981.0
209.90	839.0
211.00	2273.0
211.80	377.0
215.00	746.0
216.00	1568.0
217.00	14391.0
218.00	2596.0
220.10	349.0
221.00	3435.0
221.90	1919.0
223.00	2906.0
224.00	26088.0
225.00	6541.0
226.00	925.0
227.00	15442.0
228.00	1923.0
228.90	2457.0
229.90	435.0
231.00	709.0
234.00	1035.0
235.00	1134.0
235.90	914.0
237.00	1742.0
238.90	643.0
239.90	417.0
240.90	725.0
242.00	1970.0
243.00	1220.0
244.00	18104.0
245.00	2584.0
246.00	6488.0
246.90	1348.0
248.90	605.0
252.90	536.0
254.00	985.0
255.00	94808.0
256.00	13481.0
256.90	983.0
258.00	8634.0
259.00	1558.0
259.90	304.0
265.00	3833.0
265.90	480.0
270.80	301.0
272.90	2833.0
274.00	6829.0
275.00	35080.0
276.00	4806.0
277.00	4576.0
278.00	1115.0
281.00	361.0
282.90	522.0
283.90	334.0
284.90	593.0
292.90	885.0

Instrument :
BNA_M
ClientSampleId :
DFTPP32

295.10	324.0
296.00	17872.0
297.00	2989.0
303.00	1395.0
304.00	362.0
314.00	679.0
315.00	1903.0
315.90	853.0
321.10	450.0
323.00	2763.0
323.90	686.0
327.00	1008.0
327.80	458.0
331.90	416.0
333.00	560.0
334.00	2506.0
334.90	615.0
341.00	382.0
346.00	1066.0
352.10	1003.0
353.00	729.0
354.00	832.0
365.00	7441.0
365.90	935.0
372.00	1486.0
372.90	383.0
383.00	459.0
402.00	637.0
402.90	797.0
403.90	341.0
421.00	552.0
422.00	873.0
423.00	4470.0
424.10	1226.0
441.10	10584.0
442.10	70648.0
443.00	12337.0
444.00	1170.0

Instrument :
BNA_M
ClientSampleId :
DFTPP32

m/z	Abundance
38.00	1045.0
39.00	4331.0
40.00	349.0
49.10	655.0
50.00	18968.0
51.00	57496.0
52.10	3008.0
55.00	389.0
56.00	1503.0
57.00	3309.0
61.00	788.0
61.90	973.0
63.00	2329.0
65.00	747.0
68.00	879.0
69.00	49192.0
69.90	381.0
73.00	1128.0
74.00	7309.0
75.00	9910.0
76.00	3727.0
77.00	64304.0
78.10	4123.0
79.00	4625.0
80.00	3428.0
81.00	4404.0
82.00	1229.0
83.00	799.0
84.90	625.0
86.00	1600.0
87.00	667.0
90.90	859.0
92.00	1273.0
93.00	10950.0
93.90	520.0
95.90	350.0
97.00	342.0
98.00	8917.0
99.00	5508.0
100.00	392.0
101.00	2366.0
103.10	753.0
104.00	1958.0
105.00	1818.0
106.00	436.0
107.00	22200.0
108.00	2728.0
109.10	485.0
110.00	29032.0
111.00	5137.0
111.90	562.0
113.00	361.0
116.00	1254.0
117.00	33432.0
118.00	2295.0
120.00	325.0
121.90	1663.0
123.00	2379.0
123.90	967.0
124.90	914.0
127.00	60304.0
128.00	4838.0
129.00	28072.0
129.90	2536.0
131.00	550.0
134.00	931.0
135.00	2481.0
135.90	1021.0
137.00	1399.0
137.90	316.0
140.10	435.0
141.00	4365.0
142.00	1577.0
142.90	1073.0
145.90	934.0
147.00	2680.0
148.00	8306.0
148.90	1726.0
150.10	300.0
150.80	445.0
151.80	428.0
153.00	1292.0
154.00	1042.0
155.00	2481.0
156.00	2621.0
157.00	588.0
157.90	853.0
158.90	640.0
159.90	1256.0
161.00	2142.0
161.90	605.0

Instrument :
BNA_M
ClientSampleId :
DFTPP32

164.90	2290.0
166.00	1289.0
167.00	12258.0
168.00	6763.0
169.00	833.0
169.90	322.0
171.10	317.0
172.00	886.0
173.00	913.0
173.90	2054.0
175.00	3538.0
176.00	464.0
176.90	2001.0
177.90	767.0
179.00	7723.0
180.00	4575.0
181.00	2178.0
182.00	300.0
183.90	588.0
185.00	3397.0
186.00	22688.0
187.00	6708.0
188.00	878.0
188.90	2143.0
189.90	368.0
190.90	938.0
191.90	2823.0
193.00	2764.0
194.00	601.0
196.00	3209.0
197.00	836.0
197.90	107568.0
198.90	7504.0
200.00	687.0
201.10	382.0
201.70	379.0
203.00	1417.0
204.00	7259.0
205.00	10135.0
206.00	40512.0
207.00	5879.0
208.00	1972.0
209.00	956.0
210.00	709.0
211.00	1577.0
214.90	552.0
216.00	1367.0
216.90	13690.0
218.00	1858.0
220.20	380.0
221.00	2875.0
221.90	2037.0
222.90	3168.0
224.00	23528.0
225.00	5691.0
226.00	711.0
227.00	14970.0
228.00	2184.0
228.90	2665.0
230.90	856.0
233.90	952.0
234.90	1063.0
235.90	696.0
237.00	1401.0
238.90	757.0
239.90	491.0
241.00	791.0
242.00	1484.0
243.00	1486.0
244.00	17184.0
245.00	2149.0
246.00	5363.0
246.90	1203.0
249.00	628.0
251.80	304.0
253.00	495.0
254.10	628.0
255.00	88088.0
256.00	11936.0
257.00	1241.0
258.00	8756.0
258.90	1376.0
265.00	3612.0
265.90	485.0
273.00	3013.0
274.00	7432.0
275.00	33504.0
276.00	3796.0
277.00	5652.0
278.00	952.0
283.00	544.0
284.00	376.0
285.00	696.0
293.00	1043.0
295.00	341.0

Instrument :
BNA_M
ClientSampleId :
DFTPP32

296.00	18112.0
297.00	2391.0
302.10	333.0
303.00	1587.0
304.00	563.0
314.00	679.0
315.00	1986.0
316.00	875.0
320.90	524.0
323.00	3904.0
324.00	611.0
327.00	1128.0
328.00	511.0
331.90	336.0
333.00	420.0
334.00	2928.0
335.00	539.0
341.00	414.0
346.00	1026.0
352.10	1202.0
353.00	759.0
354.00	1076.0
354.90	408.0
365.00	8639.0
366.00	1015.0
371.00	348.0
372.00	1568.0
373.00	452.0
382.90	469.0
401.90	782.0
403.00	790.0
404.00	483.0
421.00	550.0
422.00	624.0
423.00	5085.0
423.90	1045.0
441.10	14834.0
442.00	88248.0
443.10	17280.0
444.10	1687.0

Instrument :
BNA_M
ClientSampleId :
DFTPP32

Scan 2494 (17.957 min): BM016012.D
DFTPP32

m/z	Abundance
73.00	575.0
207.10	606.0

Instrument :
BNA_M
ClientSampleId :
DFTPP32