

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072023\
 Data File : BM040985.D
 Acq On : 20 Jul 2023 17:21
 Operator : MA/JU
 Sample : PB154066BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Jul 20 21:38:35 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM071923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 20 05:08:42 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.866	152	3611	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.669	136	8774	0.400	ng/ul	#-0.01
9) Acenaphthene-d10	14.523	164	3735	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.274	188	6755	0.400	ng/ul	0.00
17) Chrysene-d12	21.472	240	4774	0.400	ng/ul	0.00
23) Perylene-d12	23.857	264	6865	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.280	96	24474	4.122	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.275	152	5631	0.482	ng/ul	0.00
18) Fluoranthene-d10	19.306	212	8128	0.405	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.668	202	956	0.038	ng/ul#	1
26) Benzo(a)pyrene	23.702	252	2252	0.099	ng/ul#	58


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072023\
Data File : BM040985.D
Acq On : 20 Jul 2023 17:21
Operator : MA/JU
Sample : PB154066BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Jul 20 21:38:35 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM071923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 20 05:08:42 2023
Response via : Initial Calibration

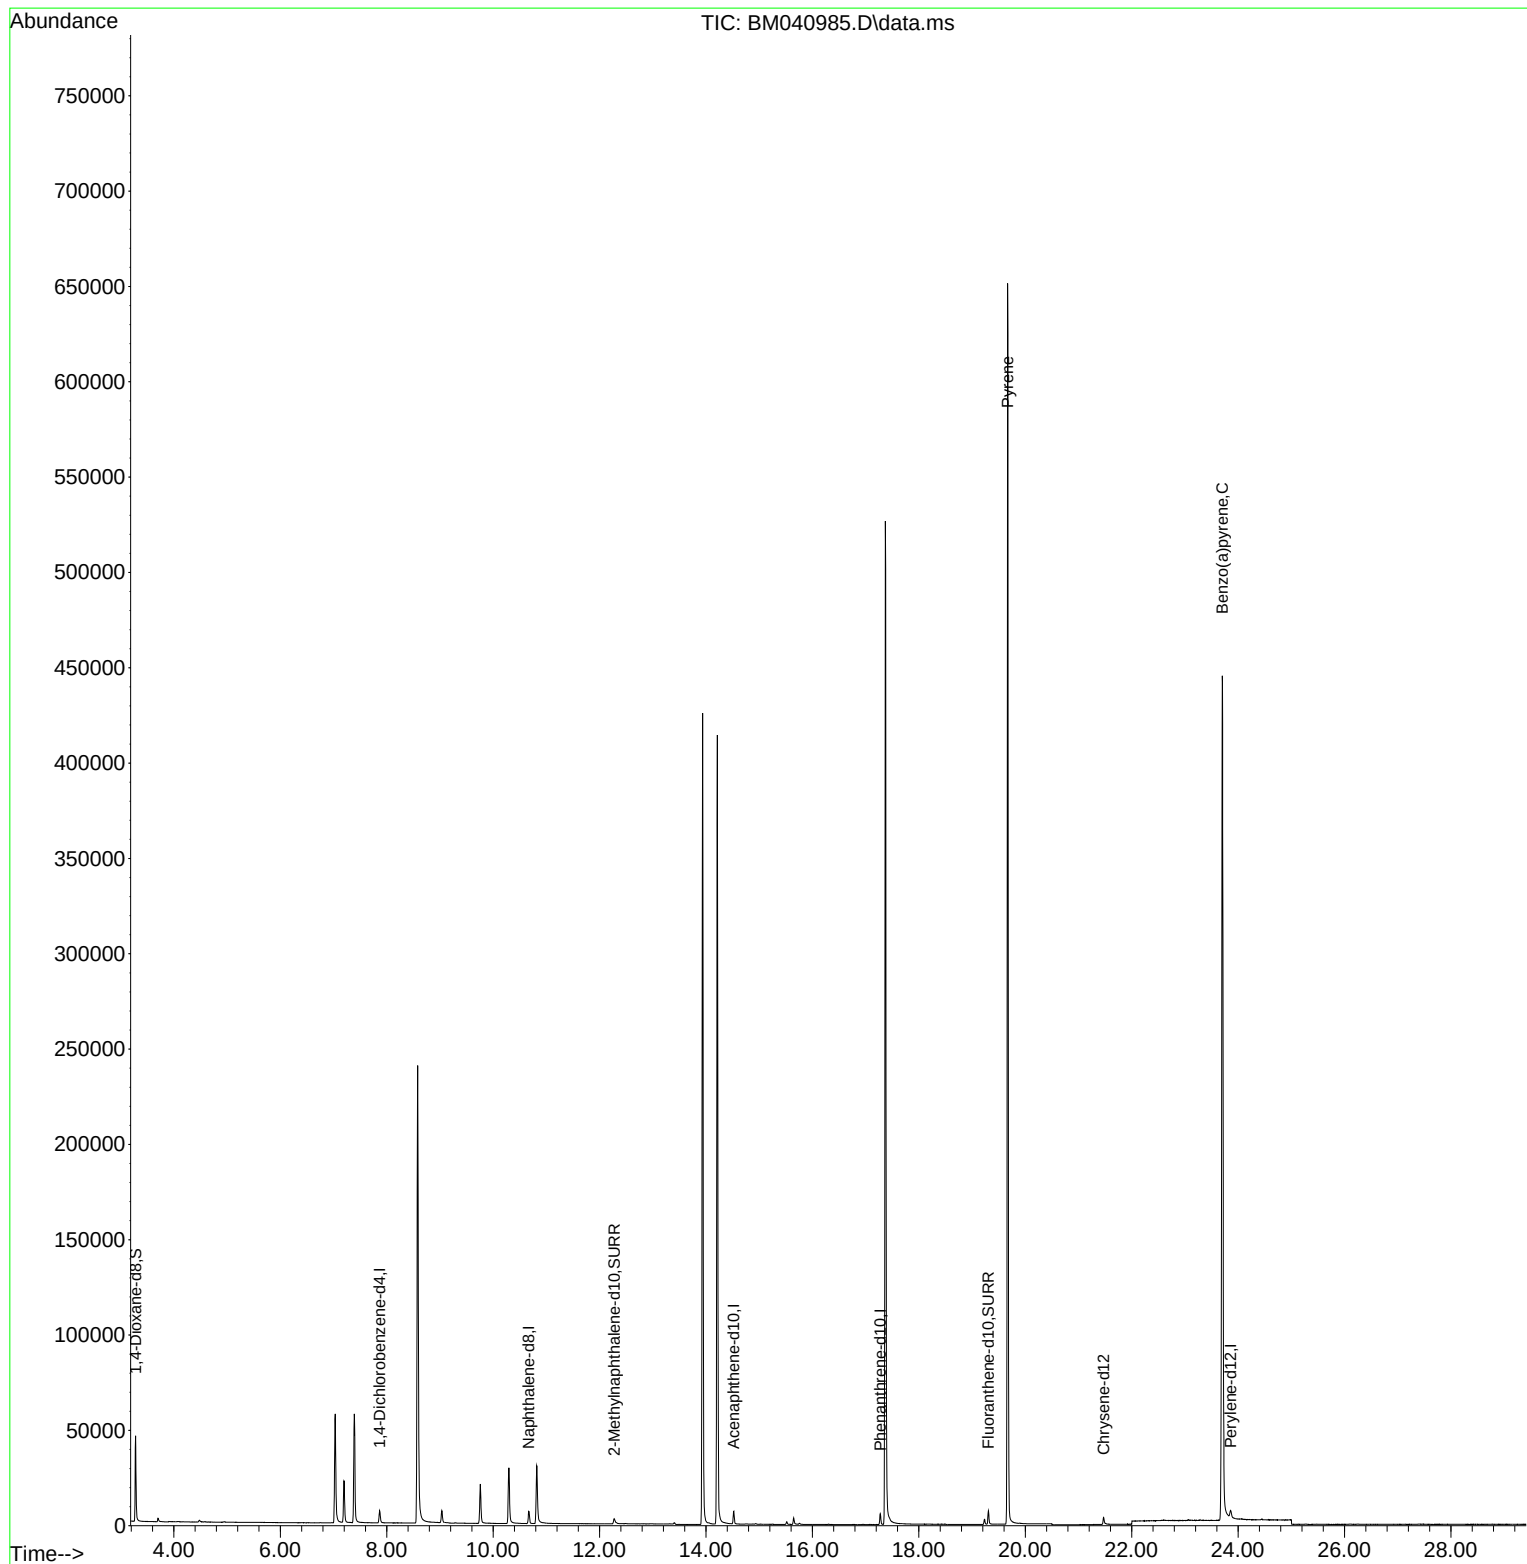

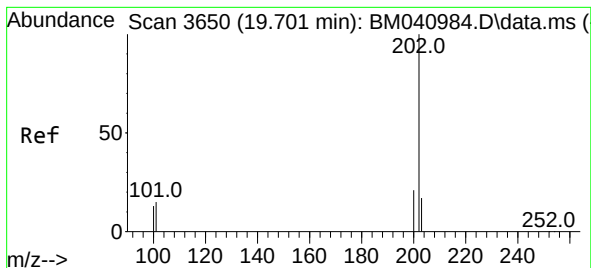

#20

Pyrene

Concen: 0.038 ng/ul

RT: 19.668 min Scan# 3

Delta R.T. -0.037 min


Lab File: BM040985.D

Acq: 20 Jul 2023 17:21




Instrument :

BNA_M

ClientSampleId :

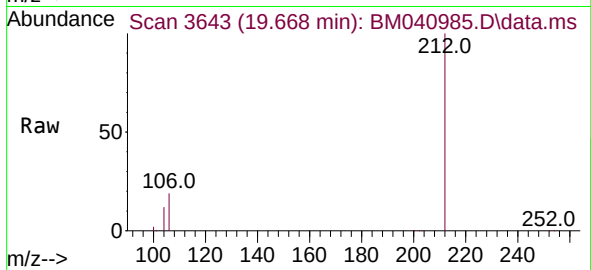

Tgt Ion:	202	Resp:	956
Ion	Ratio	Lower	Upper
202	100		
101	190.6	12.5	18.7#
100	1440.9	10.0	15.0#

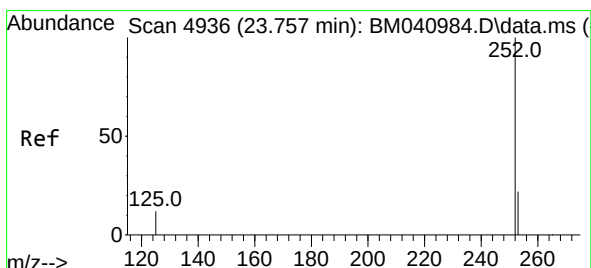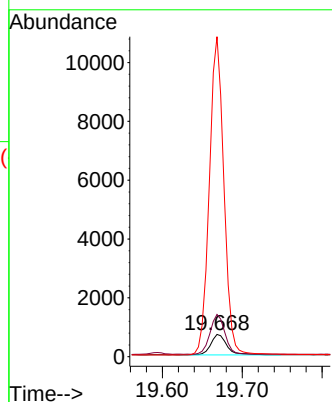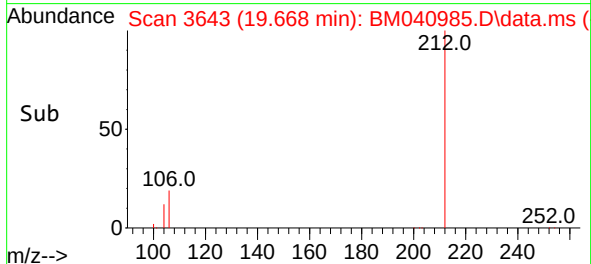

#26

Benzo(a)pyrene

Concen: 0.099 ng/ul

RT: 23.702 min Scan# 4917

Delta R.T. -0.061 min

Lab File: BM040985.D

Acq: 20 Jul 2023 17:21

Tgt Ion:	252	Resp:	2252
Ion	Ratio	Lower	Upper
252	100		
253	55.9	28.2	42.2#
125	59.1	25.2	37.8#

