

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072023\
 Data File : BM040989.D
 Acq On : 20 Jul 2023 19:51
 Operator : MA/JU
 Sample : 03452-08
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A46N5

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/20/2023
 Supervised By :Sohil Jodhani 07/20/2023

Quant Time: Jul 20 21:39:26 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM071923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 20 05:08:42 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.866	152	2945	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.669	136	8527	0.400	ng/ul	#-0.01
9) Acenaphthene-d10	14.518	164	3699	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.274	188	6972	0.400	ng/ul	0.00
17) Chrysene-d12	21.466	240	4803	0.400	ng/ul	0.00
23) Perylene-d12	23.857	264	4587	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.279	96	5375	1.110	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.264	152	2528	0.222	ng/ul	-0.02
18) Fluoranthene-d10	19.306	212	5229	0.259	ng/ul	0.00
Target Compounds						
						Qvalue
5) Naphthalene	10.724	128	3386	0.145	ng/ul#	92
7) 2-Methylnaphthalene	12.341	142	302	0.024	ng/ul	96
10) Acenaphthylene	14.240	152	578	0.037	ng/ul#	55
11) Acenaphthene	14.583	153	420	0.031	ng/ul#	92
12) Fluorene	15.573	166	378	0.027	ng/ul#	87
15) Phenanthrene	17.316	178	5987	0.287	ng/ul	97
16) Anthracene	17.409	178	563	0.035	ng/ul#	63
19) Fluoranthene	19.334	202	15184	0.612	ng/ul	100
20) Pyrene	19.696	202	16519	0.652	ng/ul	99
21) Benzo(a)anthracene	21.448	228	3943	0.269	ng/ul#	93
22) Chrysene	21.501	228	5085m	0.304	ng/ul	
24) Benzo(b)fluoranthene	23.129	252	6056	0.344	ng/ul	84
25) Benzo(k)fluoranthene	23.172	252	2626m	0.157	ng/ul	
26) Benzo(a)pyrene	23.748	252	773	0.051	ng/ul#	3
27) Indeno(1,2,3-cd)pyrene	26.330	276	2280	0.113	ng/ul#	95
28) Dibenzo(a,h)anthracene	26.344	278	693	0.045	ng/ul#	16

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072023\
Data File : BM040989.D
Acq On : 20 Jul 2023 19:51
Operator : MA/JU
Sample : 03452-08
Misc :
ALS Vial : 20 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
A46N5

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/20/2023
Supervised By :Sohil Jodhani 07/20/2023


Quant Time: Jul 20 21:39:26 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM071923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 20 05:08:42 2023
Response via : Initial Calibration

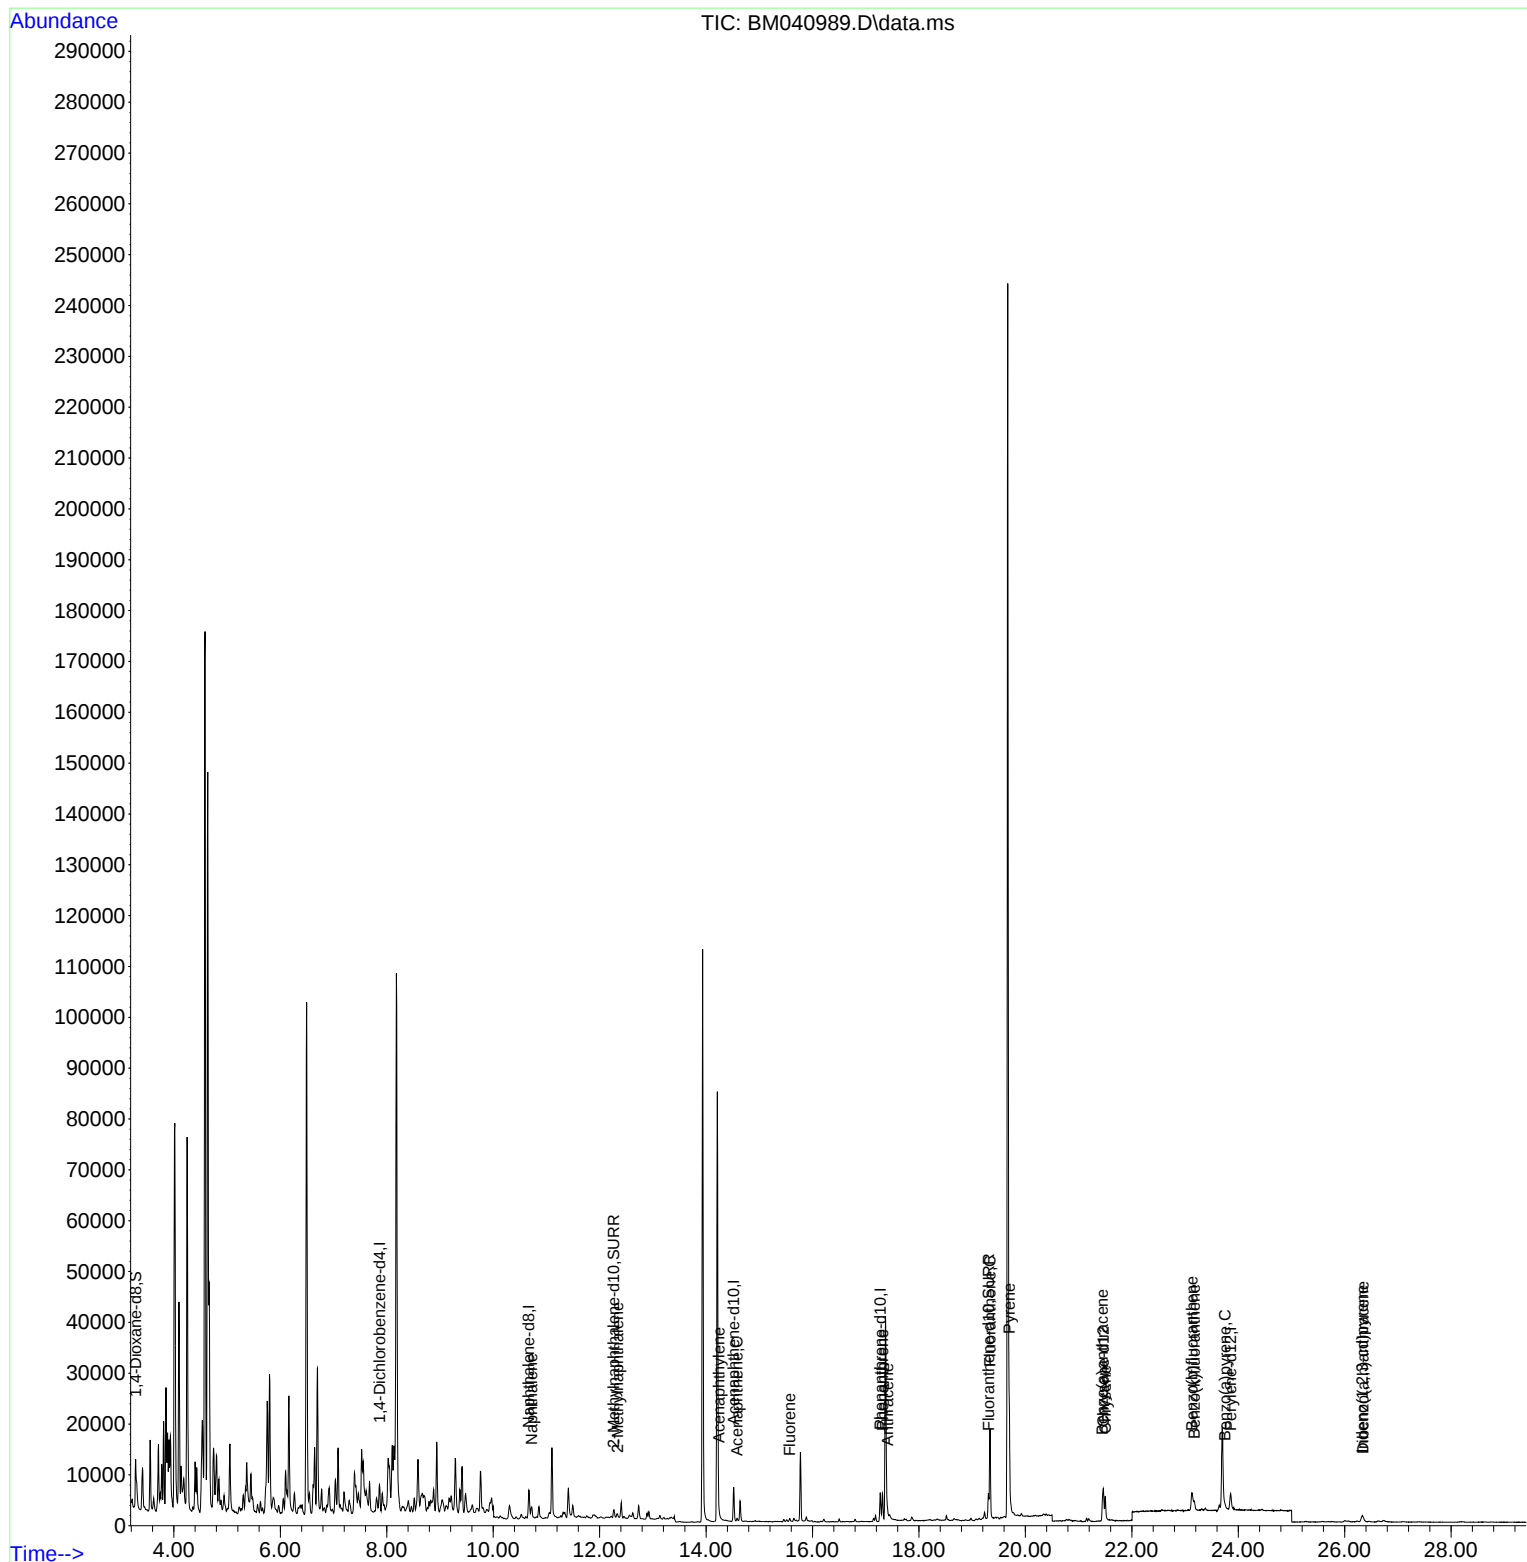



#5
Naphthalene
Concen: 0.145 ng/ul
RT: 10.724 min Scan# 1751
Delta R.T. -0.006 min
Lab File: BM040989.D
Acq: 20 Jul 2023 19:51




Instrument :
BNA_M
ClientSampleId :
A46N5

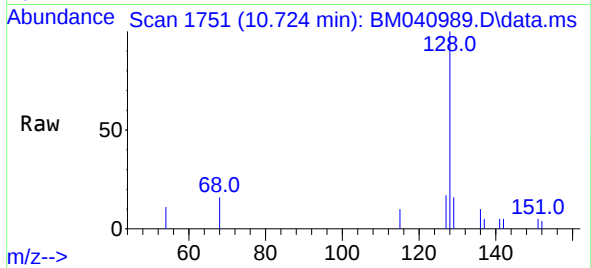

Tgt Ion:128 Resp: 3380
Ion Ratio Lower Upper
128 100
129 15.7 9.8 14.8
127 16.6 11.0 16.4




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 07/20/2023
Supervised By :Sohil Jodhani 07/20/2023

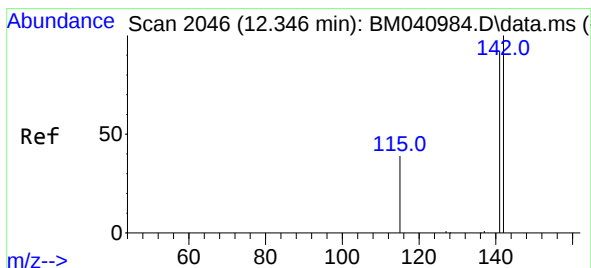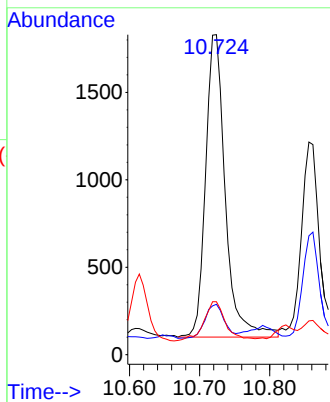

#7
2-Methylnaphthalene
Concen: 0.024 ng/ul
RT: 12.341 min Scan# 2045
Delta R.T. -0.011 min
Lab File: BM040989.D
Acq: 20 Jul 2023 19:51


Tgt Ion:142 Resp: 302
Ion Ratio Lower Upper
142 100
141 95.7 73.2 109.8

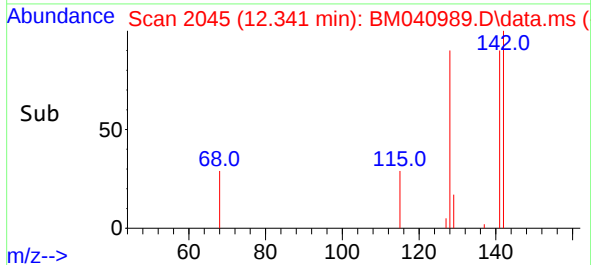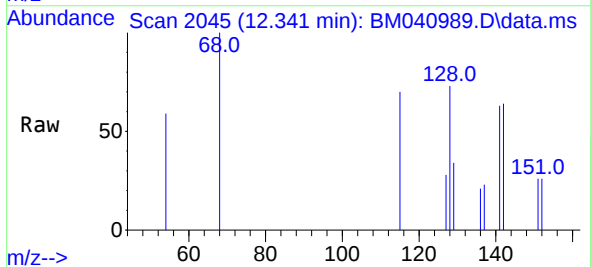



#10
Acenaphthylene
Concen: 0.037 ng/ul
RT: 14.240 min Scan# 2420
Delta R.T. -0.009 min
Lab File: BM040989.D
Acq: 20 Jul 2023 19:51




Instrument :
BNA_M
ClientSampleId :
A46N5



Tgt Ion:152 Resp: 578
Ion Ratio Lower Upper
152 100
151 42.1 16.8 25.2
153 32.6 11.6 17.4




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 07/20/2023
Supervised By :Sohil Jodhani 07/20/2023



#11
Acenaphthene
Concen: 0.031 ng/ul
RT: 14.583 min Scan# 2493
Delta R.T. -0.005 min
Lab File: BM040989.D
Acq: 20 Jul 2023 19:51


Tgt Ion:153 Resp: 420
Ion Ratio Lower Upper
153 100
152 61.9 41.0 61.6
154 88.6 68.2 102.2

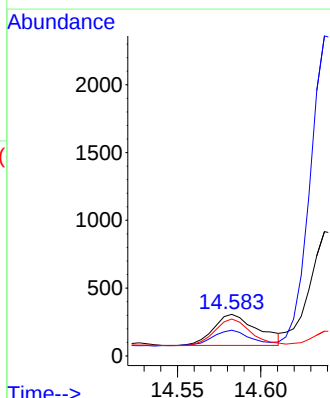



#12
Fluorene
Concen: 0.027 ng/ul
RT: 15.573 min Scan# 21
Delta R.T. -0.009 min
Lab File: BM040989.D
Acq: 20 Jul 2023 19:51




Instrument :
BNA_M
ClientSampleId :
A46N5



Tgt Ion:166 Resp: 378
Ion Ratio Lower Upper
166 100
165 108.2 80.3 120.5
167 35.1 11.7 17.5




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 07/20/2023
Supervised By :Sohil Jodhani 07/20/2023



#15
Phenanthrene
Concen: 0.287 ng/ul
RT: 17.316 min Scan# 3111
Delta R.T. -0.008 min
Lab File: BM040989.D
Acq: 20 Jul 2023 19:51


Tgt Ion:178 Resp: 5987
Ion Ratio Lower Upper
178 100
179 18.1 13.0 19.6
176 21.2 16.2 24.4

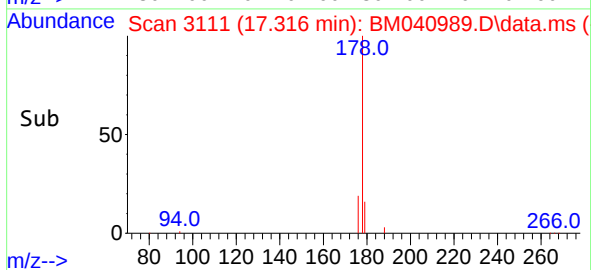



#16
 Anthracene
 Concen: 0.035 ng/u1
 RT: 17.409 min Scan# 3134
 Delta R.T. -0.013 min
 Lab File: BM040989.D
 Acq: 20 Jul 2023 19:51

Instrument :
 BNA_M
 ClientSampleId :
 A46N5






Tgt Ion:178 Resp: 561


Ion	Ratio	Lower	Upper
178	100		
179	39.2	13.7	20.5
176	32.2	16.4	24.6

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/20/2023
 Supervised By :Sohil Jodhani 07/20/2023






#19
 Fluoranthene
 Concen: 0.612 ng/u1
 RT: 19.334 min Scan# 3571
 Delta R.T. -0.009 min
 Lab File: BM040989.D
 Acq: 20 Jul 2023 19:51



Tgt Ion:202 Resp: 15184


Ion	Ratio	Lower	Upper
202	100		
101	13.7	11.0	16.4
100	10.6	8.3	12.5

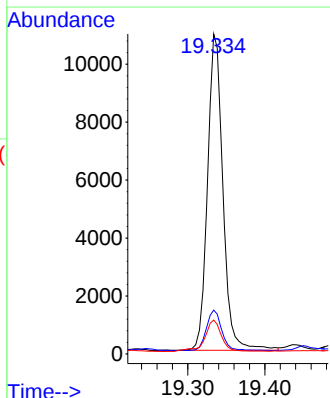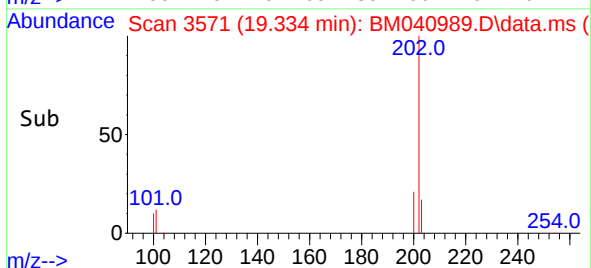



#20
Pyrene
Concen: 0.652 ng/ul
RT: 19.696 min Scan# 3649
Delta R.T. -0.009 min
Lab File: BM040989.D
Acq: 20 Jul 2023 19:51




Instrument :
BNA_M
ClientSampleId :
A46N5




Tgt Ion:202 Resp: 16519
Ion Ratio Lower Upper
202 100
101 14.6 12.5 18.7
100 12.3 10.0 15.0

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 07/20/2023
Supervised By :Sohil Jodhani 07/20/2023




#21
Benzo(a)anthracene
Concen: 0.269 ng/ul
RT: 21.448 min Scan# 4146
Delta R.T. -0.009 min
Lab File: BM040989.D
Acq: 20 Jul 2023 19:51




Tgt Ion:228 Resp: 3943
Ion Ratio Lower Upper
228 100
229 25.3 16.2 24.4#
226 30.4 22.3 33.5

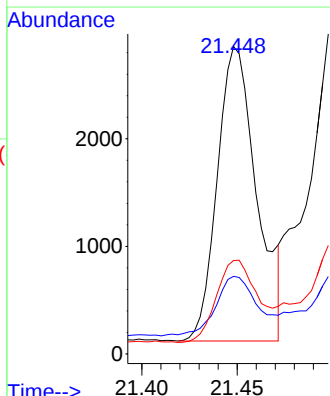



#22
Chrysene
Concen: 0.304 ng/ul m
RT: 21.501 min Scan# 4165
Delta R.T. -0.006 min
Lab File: BM040989.D
Acq: 20 Jul 2023 19:51




Instrument :
BNA_M
ClientSampleId :
A46N5

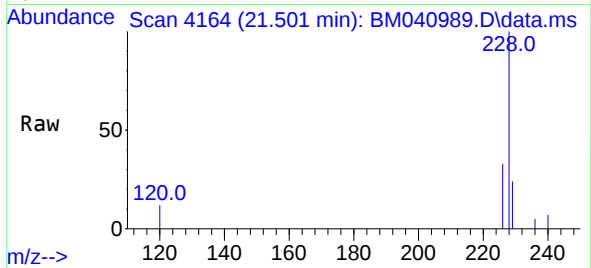

Tgt Ion:228 Resp: 5085
Ion Ratio Lower Upper
228 100
226 32.8 24.6 37.0
229 23.8 16.1 24.1




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 07/20/2023
Supervised By :Sohil Jodhani 07/20/2023

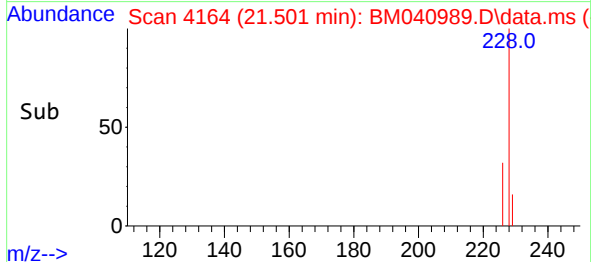

#24
Benzo(b)fluoranthene
Concen: 0.344 ng/ul
RT: 23.129 min Scan# 4721
Delta R.T. -0.006 min
Lab File: BM040989.D
Acq: 20 Jul 2023 19:51


Tgt Ion:252 Resp: 6056
Ion Ratio Lower Upper
252 100
253 34.4 0.0 57.4
125 33.5 0.0 45.2

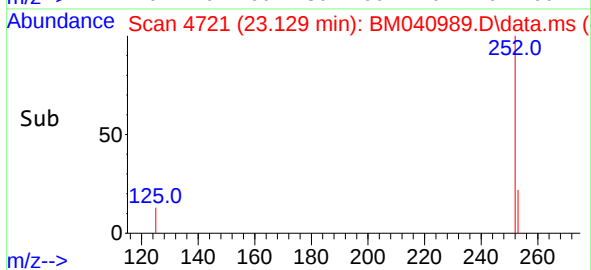



#25
Benzo(k)fluoranthene
Concen: 0.157 ng/ul m
RT: 23.172 min Scan# 4
Delta R.T. -0.015 min
Lab File: BM040989.D
Acq: 20 Jul 2023 19:51




Instrument :
BNA_M
ClientSampleId :
A46N5

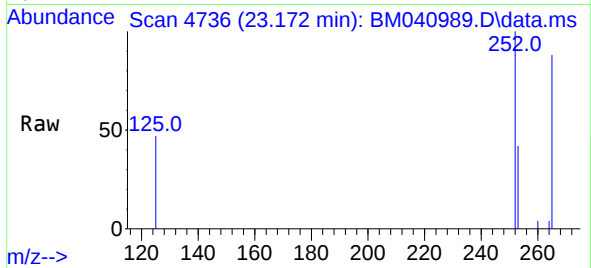


Tgt Ion:252 Resp: 2620
Ion Ratio Lower Upper
252 100
253 42.0 23.3 34.9#
125 47.3 18.2 27.2#

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 07/20/2023
Supervised By :Sohil Jodhani 07/20/2023

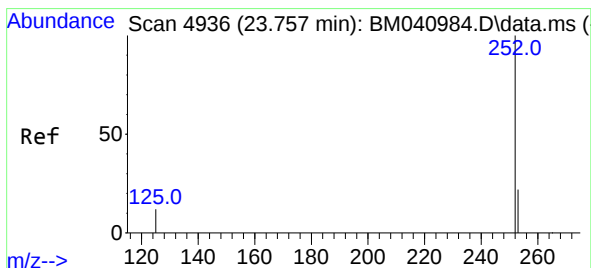


#26
Benzo(a)pyrene
Concen: 0.051 ng/ul
RT: 23.748 min Scan# 4933
Delta R.T. -0.015 min
Lab File: BM040989.D
Acq: 20 Jul 2023 19:51

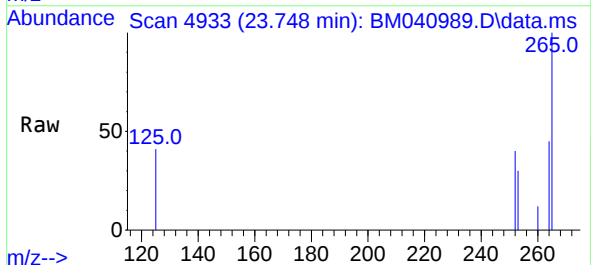


Tgt Ion:252 Resp: 773
Ion Ratio Lower Upper
252 100
253 75.7 28.2 42.2#
125 101.8 25.2 37.8#

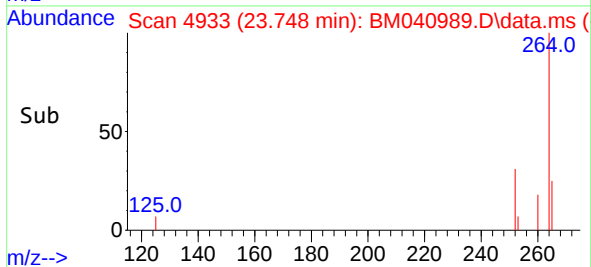



#27
Indeno(1,2,3-cd)pyrene
Concen: 0.113 ng/ul
RT: 26.330 min Scan# 5758
Delta R.T. -0.020 min
Lab File: BM040989.D
Acq: 20 Jul 2023 19:51




Instrument :
BNA_M
ClientSampleId :
A46N5

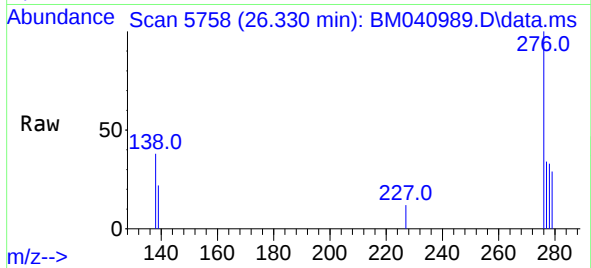


Tgt Ion:276 Resp: 2280
Ion Ratio Lower Upper
276 100
138 25.3 22.3 33.5
227 2.0 0.0 0.0

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/20/2023
Supervised By :Sohil Jodhani 07/20/2023

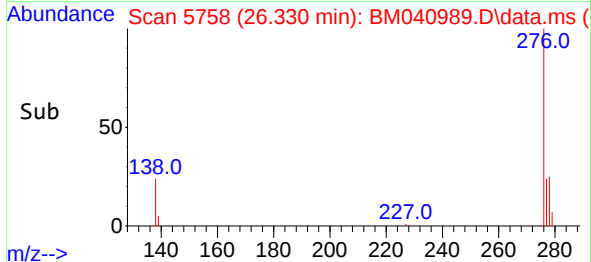

#28
Dibenzo(a,h)anthracene
Concen: 0.045 ng/ul
RT: 26.344 min Scan# 5762
Delta R.T. -0.024 min
Lab File: BM040989.D
Acq: 20 Jul 2023 19:51



Tgt Ion:278 Resp: 693
Ion Ratio Lower Upper
278 100
139 66.7 19.2 28.8#
279 80.6 27.0 40.6#

