

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072123\
 Data File : BM041026.D
 Acq On : 21 Jul 2023 20:38
 Operator : MA/JU
 Sample : PB154070BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Jul 21 23:51:21 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM071923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 21 18:20:46 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.862	152	4487	0.400	ng/ul	0.00
4) Naphthalene-d8	10.664	136	16331	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.518	164	9715	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.270	188	20920	0.400	ng/ul	0.00
17) Chrysene-d12	21.472	240	13920	0.400	ng/ul	0.00
23) Perylene-d12	23.854	264	16750	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.275	96	36966	5.011	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.269	152	7743	0.356	ng/ul	0.00
18) Fluoranthene-d10	19.306	212	17474	0.298	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.513	166	2960	0.080	ng/ul#	14
20) Pyrene	19.668	202	2439	0.033	ng/ul#	1
26) Benzo(a)pyrene	23.699	252	4263	0.077	ng/ul#	77


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072123\
Data File : BM041026.D
Acq On : 21 Jul 2023 20:38
Operator : MA/JU
Sample : PB154070BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Jul 21 23:51:21 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM071923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 21 18:20:46 2023
Response via : Initial Calibration




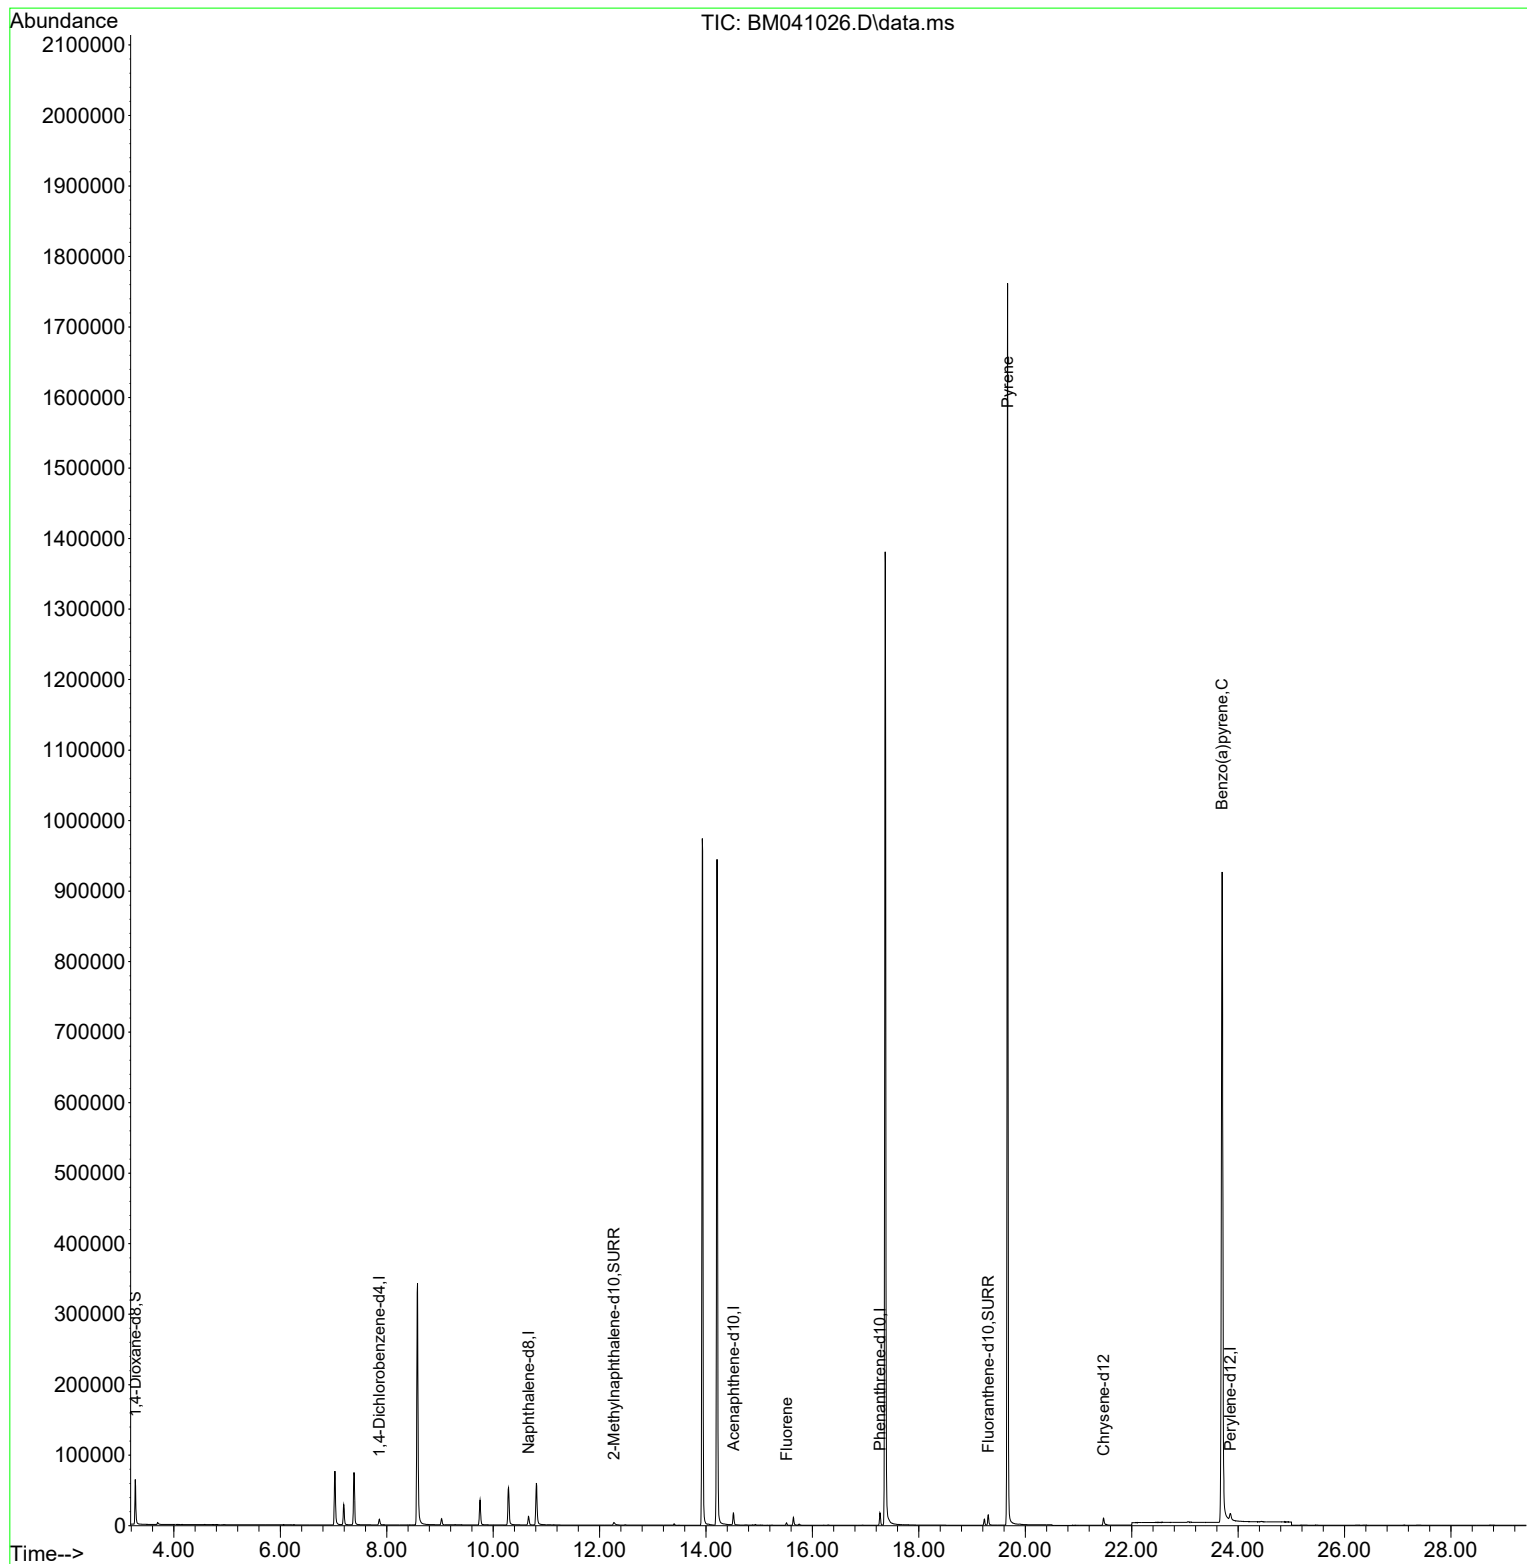


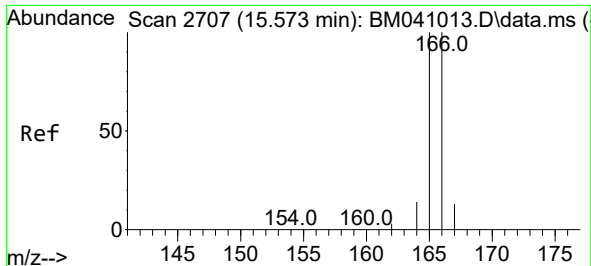

#12
Fluorene
Concen: 0.080 ng/ul
RT: 15.513 min Scan# 2
Delta R.T. -0.060 min
Lab File: BM041026.D
Acq: 21 Jul 2023 20:38




Instrument :
BNA_M
ClientSampleId :


Tgt Ion:166 Resp: 2960
Ion Ratio Lower Upper
166 100
165 7.6 80.3 120.5#
167 32.8 11.7 17.5#

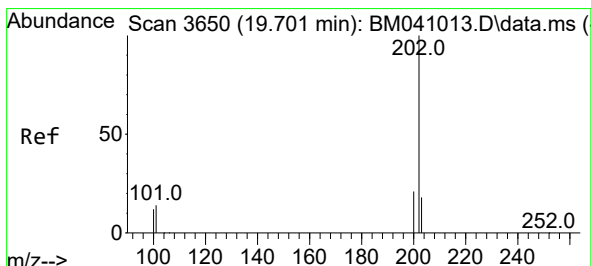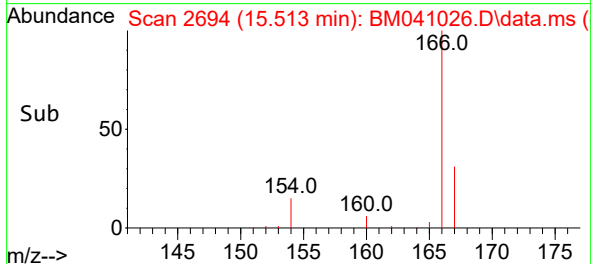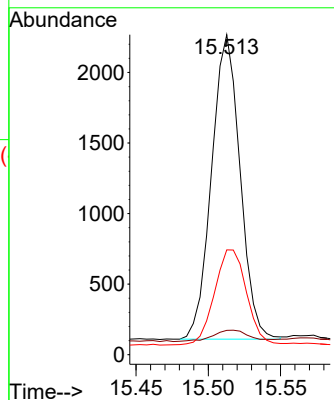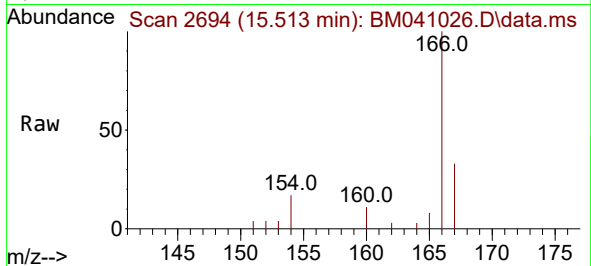

#20
Pyrene
Concen: 0.033 ng/ul
RT: 19.668 min Scan# 3643
Delta R.T. -0.033 min
Lab File: BM041026.D
Acq: 21 Jul 2023 20:38


Tgt Ion:202 Resp: 2439
Ion Ratio Lower Upper
202 100
101 152.9 12.5 18.7#
100 1126.3 10.0 15.0#

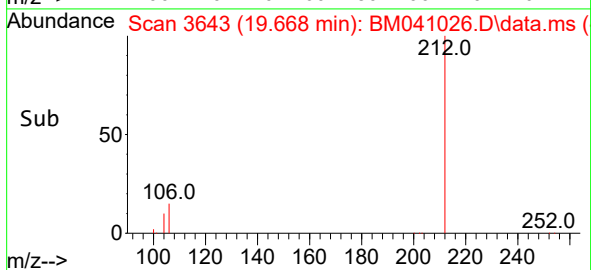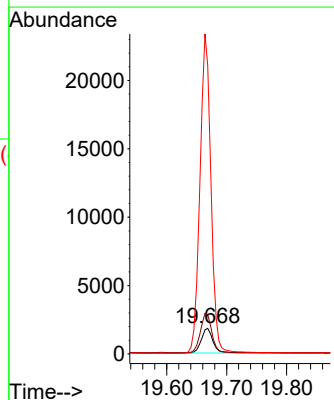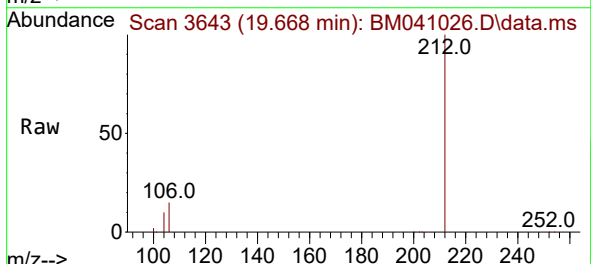

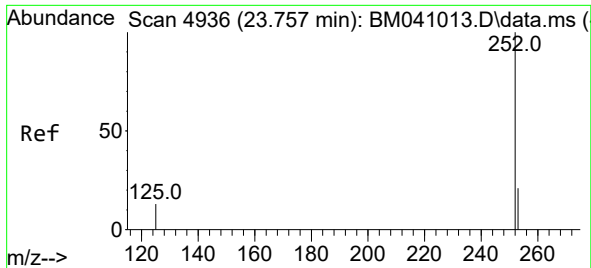

#26
Benzo(a)pyrene
Concen: 0.077 ng/ul
RT: 23.699 min Scan# 4916
Delta R.T. -0.058 min
Lab File: BM041026.D
Acq: 21 Jul 2023 20:38

Instrument :
BNA_M
ClientSampleId :

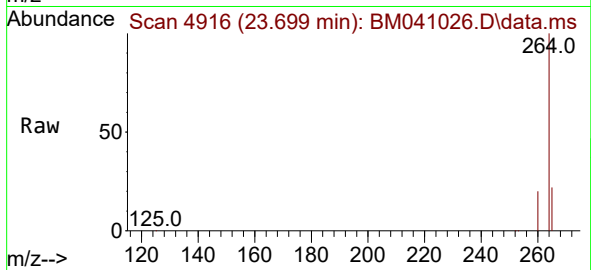

Tgt Ion:252 Resp: 4263
Ion Ratio Lower Upper
252 100
253 50.1 28.2 42.2#
125 42.6 25.2 37.8#

