

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072123\
 Data File : BM041043.D
 Acq On : 22 Jul 2023 07:48
 Operator : MA/JU
 Sample : PB154169BL
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Jul 22 22:35:03 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM071923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jul 22 22:33:48 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.857	152	4208	0.400	ng/ul	0.00
4) Naphthalene-d8	10.664	136	15705	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.513	164	9455	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.265	188	19041	0.400	ng/ul	0.00
17) Chrysene-d12	21.469	240	12232	0.400	ng/ul	0.00
23) Perylene-d12	23.851	264	16151	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.275	96	34684	5.013	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.264	152	7584	0.362	ng/ul	0.00
18) Fluoranthene-d10	19.301	212	15310	0.298	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.508	166	2786	0.077	ng/ul#	13
20) Pyrene	19.664	202	2197	0.034	ng/ul#	1
26) Benzo(a)pyrene	23.693	252	4341	0.081	ng/ul#	80


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072123\
Data File : BM041043.D
Acq On : 22 Jul 2023 07:48
Operator : MA/JU
Sample : PB154169BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :


Quant Time: Jul 22 22:35:03 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM071923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jul 22 22:33:48 2023
Response via : Initial Calibration

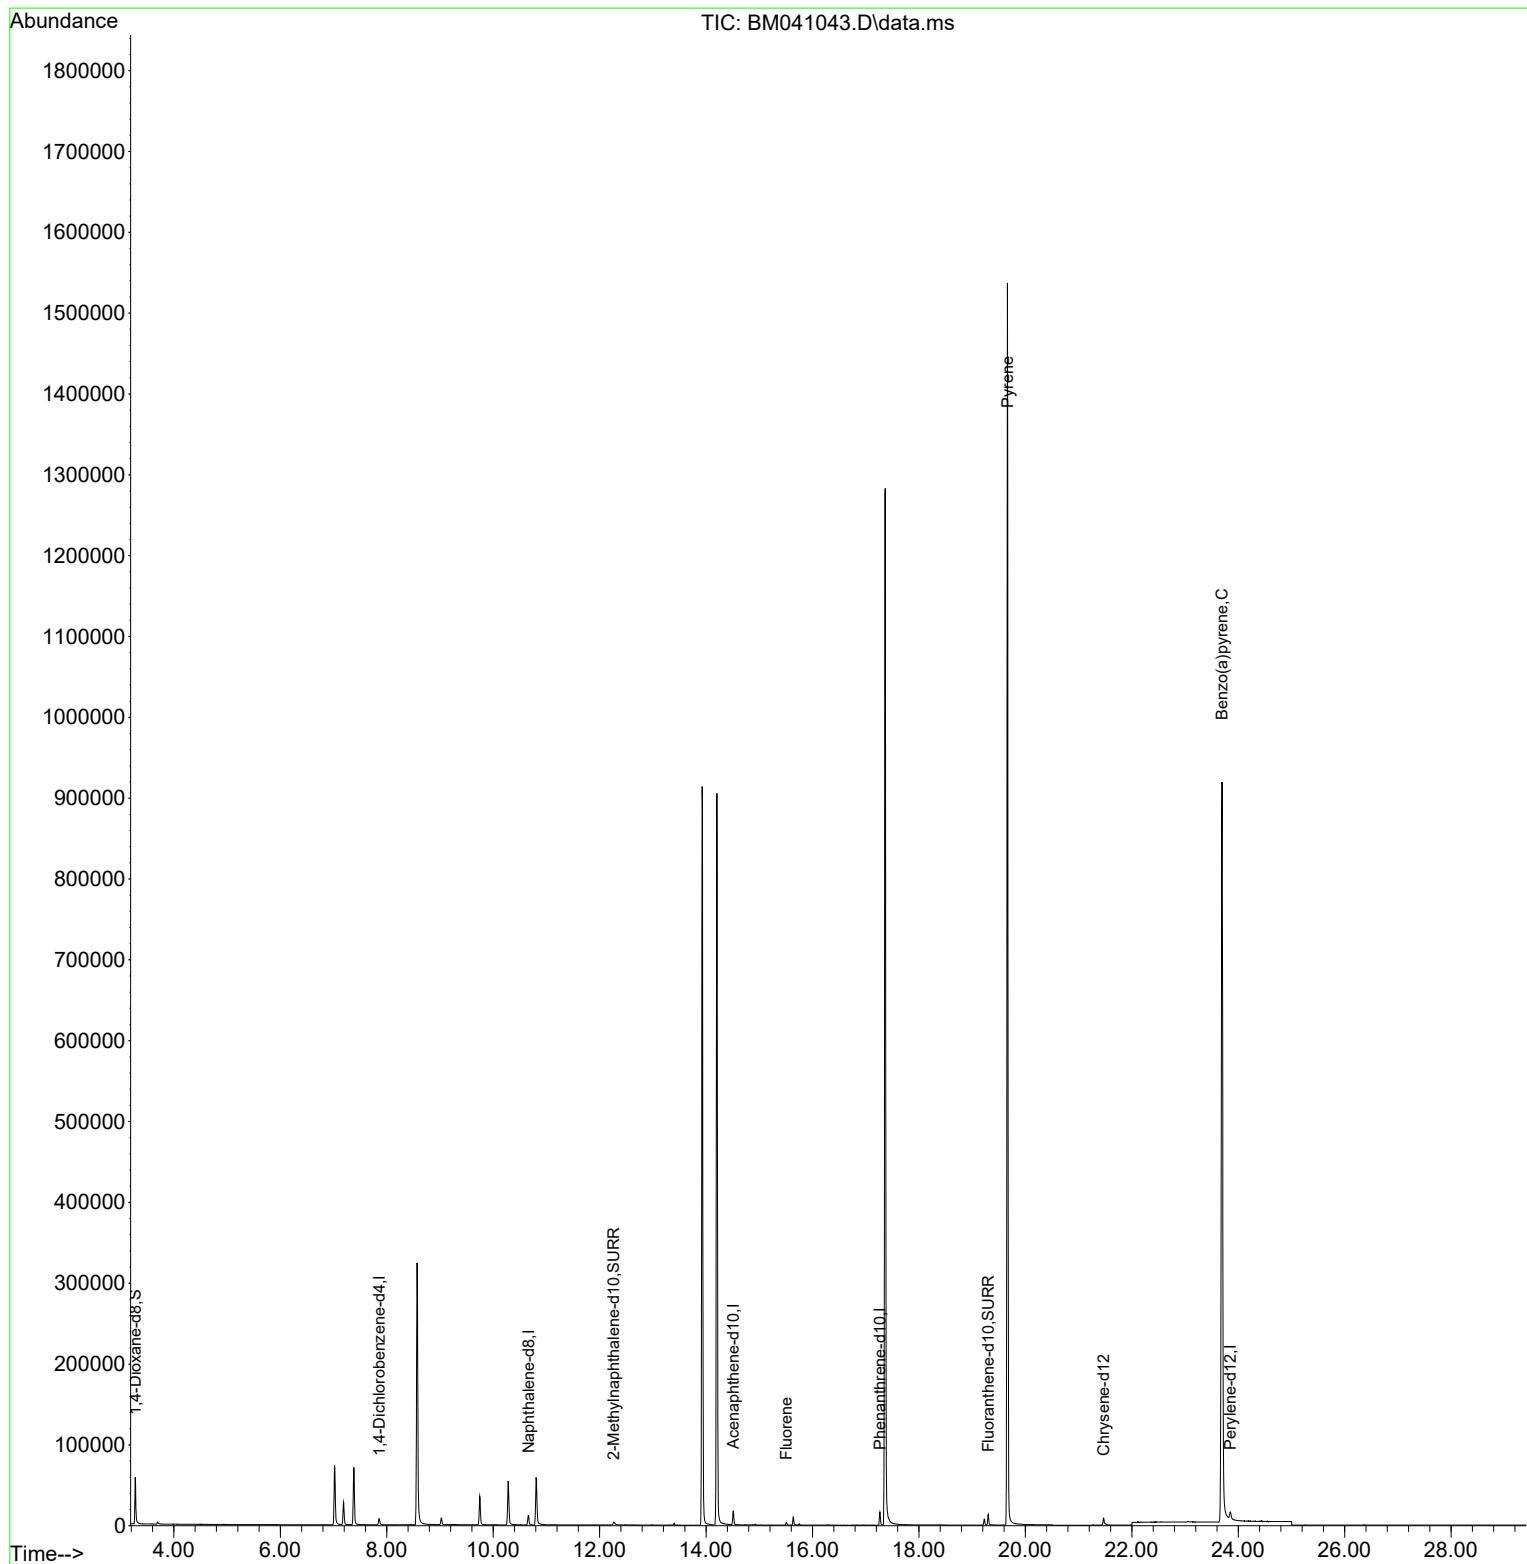



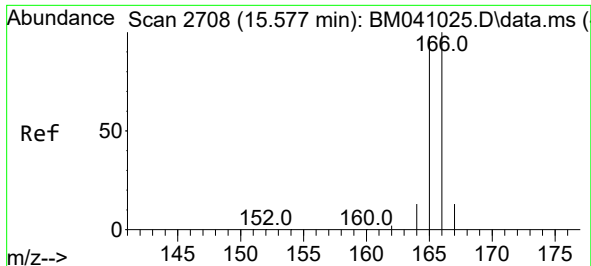


#12
Fluorene
Concen: 0.077 ng/ul
RT: 15.508 min Scan# 2708
Delta R.T. -0.065 min
Lab File: BM041043.D
Acq: 22 Jul 2023 07:48

Instrument :
BNA_M
ClientSampleId :



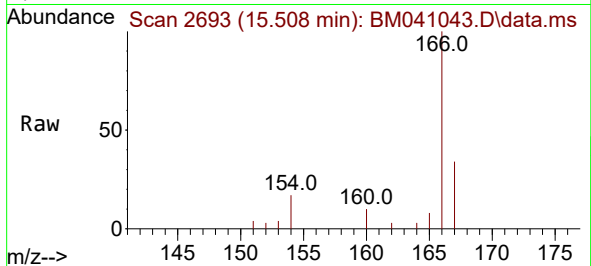



Tgt Ion:166 Resp: 2786
Ion Ratio Lower Upper
166 100
165 7.7 80.3 120.5#
167 33.7 11.7 17.5#

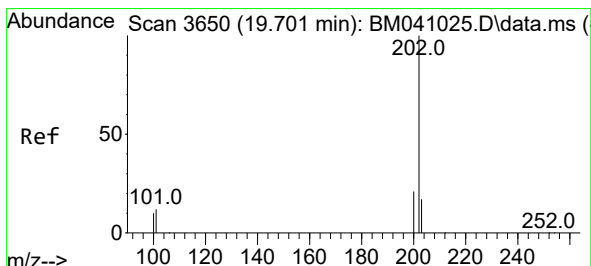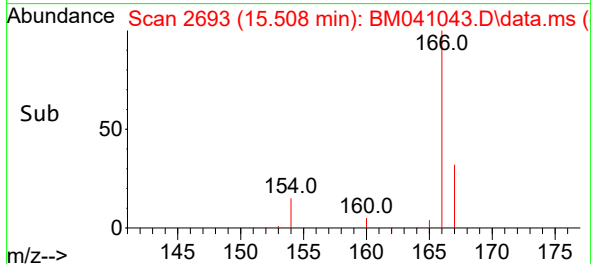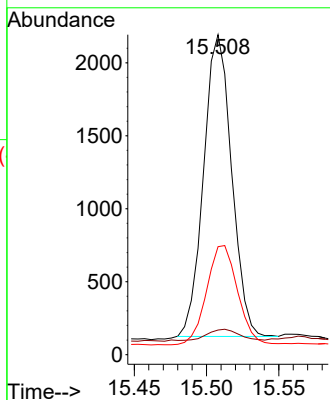

#20
Pyrene
Concen: 0.034 ng/ul
RT: 19.664 min Scan# 3642
Delta R.T. -0.033 min
Lab File: BM041043.D
Acq: 22 Jul 2023 07:48


Tgt Ion:202 Resp: 2197
Ion Ratio Lower Upper
202 100
101 160.1 12.5 18.7#
100 1191.6 10.0 15.0#

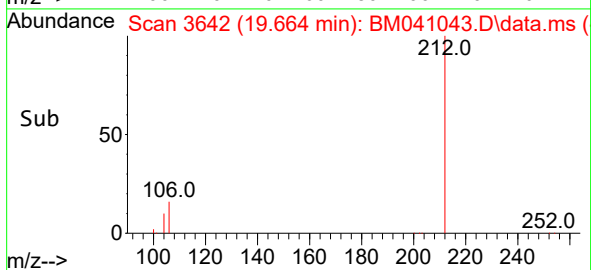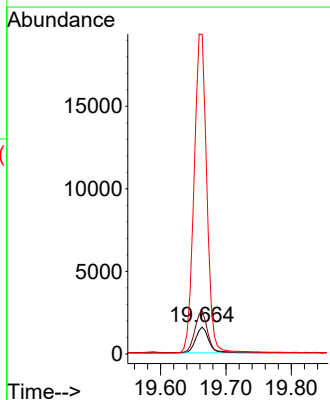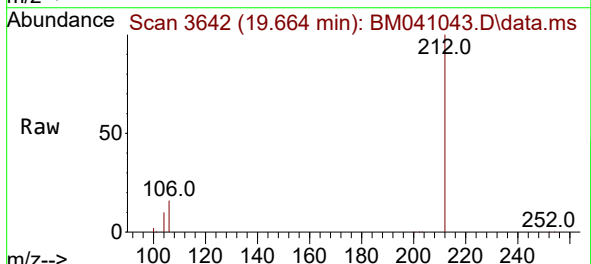

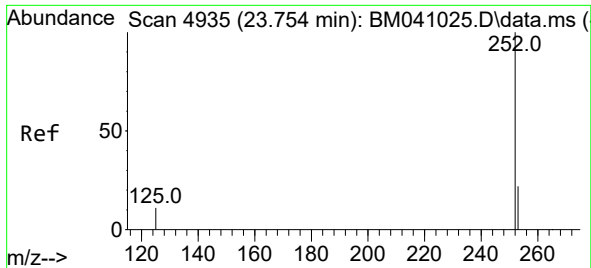

#26
Benzo(a)pyrene
Concen: 0.081 ng/ul
RT: 23.693 min Scan# 4914
Delta R.T. -0.056 min
Lab File: BM041043.D
Acq: 22 Jul 2023 07:48

Instrument :
BNA_M
ClientSampleId :

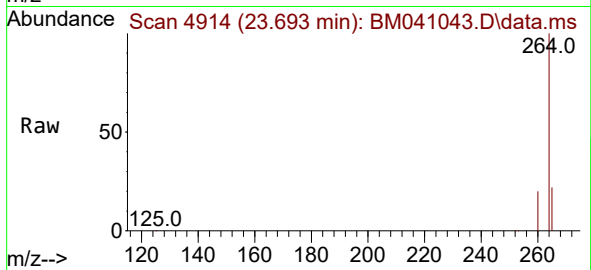

Tgt Ion:252 Resp: 4341
Ion Ratio Lower Upper
252 100
253 48.5 28.2 42.2#
125 41.1 25.2 37.8#

