

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072123\
 Data File : BM041051.D
 Acq On : 22 Jul 2023 12:43
 Operator : MA/JU
 Sample : PB154169BL
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Jul 22 22:36:26 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM071923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jul 22 22:33:48 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.857	152	4315	0.400	ng/ul	0.00
4) Naphthalene-d8	10.664	136	15674	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.513	164	8997	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.265	188	17084	0.400	ng/ul	0.00
17) Chrysene-d12	21.466	240	13807	0.400	ng/ul	0.00
23) Perylene-d12	23.851	264	19124	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.275	96	34172	4.817	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.264	152	7630	0.365	ng/ul	0.00
18) Fluoranthene-d10	19.301	212	14644	0.252	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.664	202	2119	0.029	ng/ul#	1
26) Benzo(a)pyrene	23.696	252	4613	0.073	ng/ul#	68


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072123\
Data File : BM041051.D
Acq On : 22 Jul 2023 12:43
Operator : MA/JU
Sample : PB154169BL
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Jul 22 22:36:26 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM071923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jul 22 22:33:48 2023
Response via : Initial Calibration

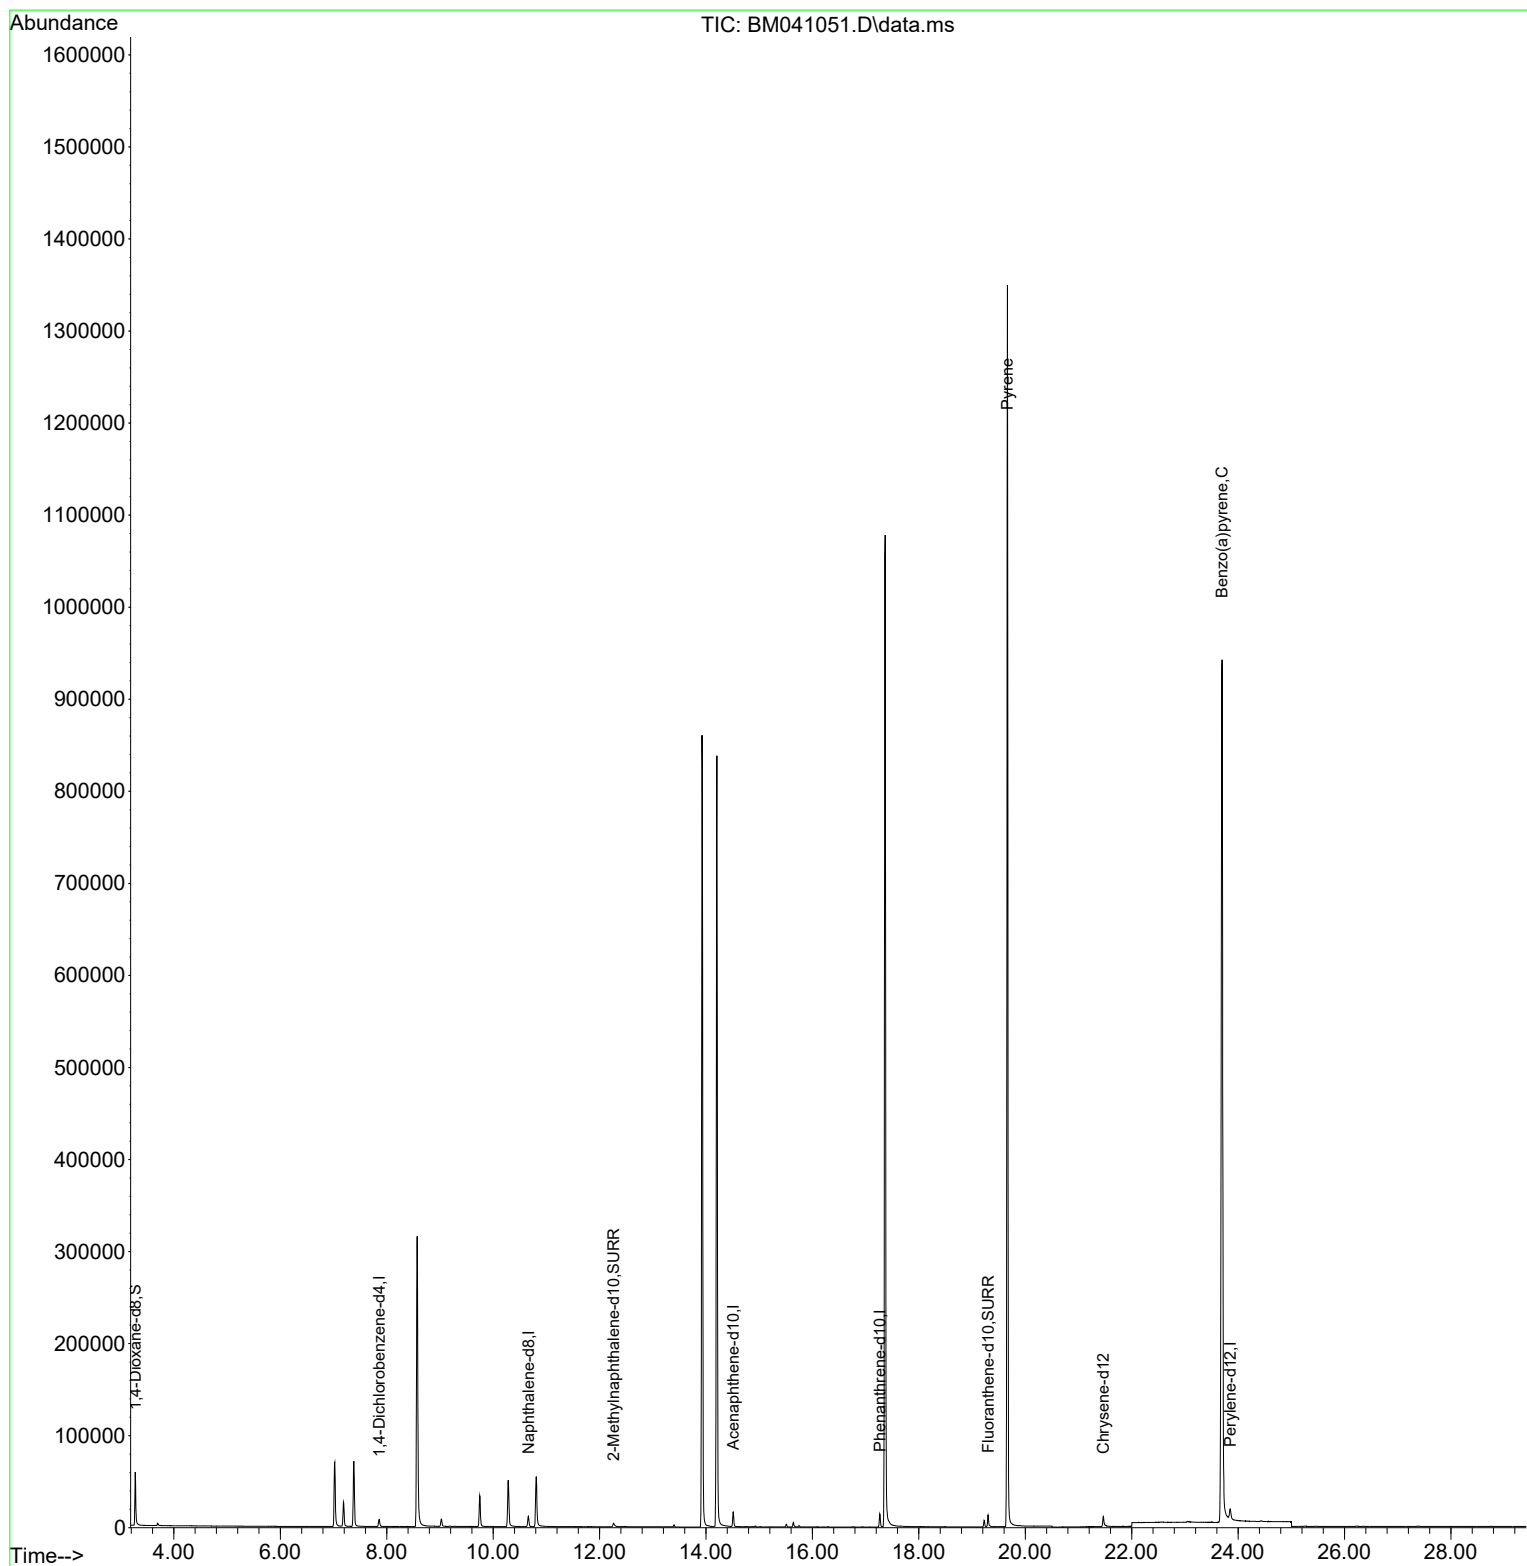

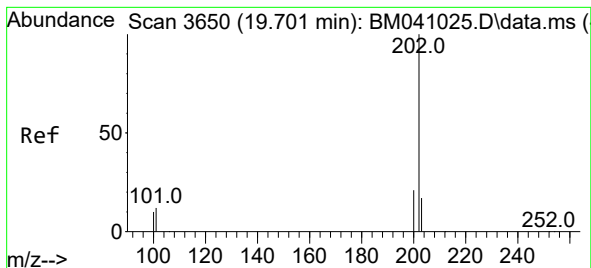

#20

Pyrene

Concen: 0.029 ng/ul

RT: 19.664 min Scan# 3

Delta R.T. -0.032 min


Lab File: BM041051.D

Acq: 22 Jul 2023 12:43

Instrument :




BNA_M

ClientSampleId :

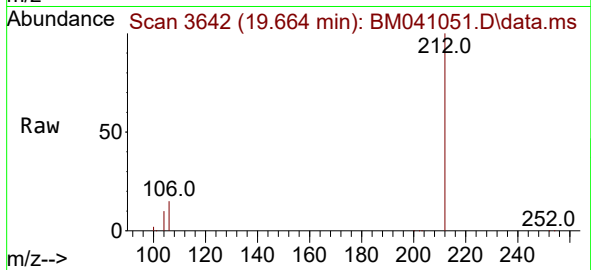

Tgt Ion:202 Resp: 2119

Ion	Ratio	Lower	Upper
202	100		
101	146.2	12.5	18.7#
100	1091.1	10.0	15.0#

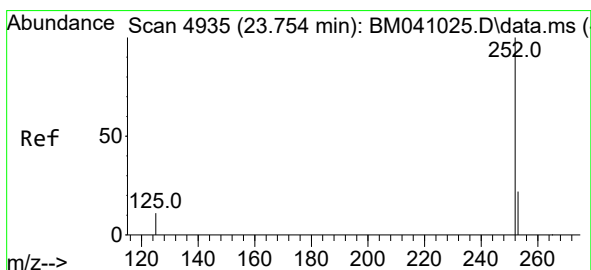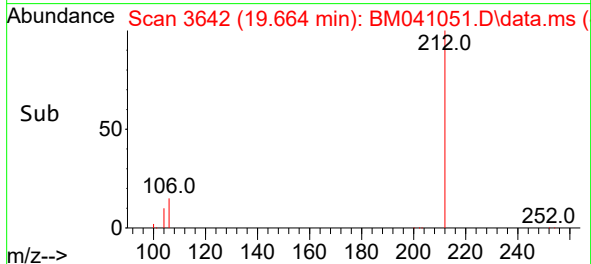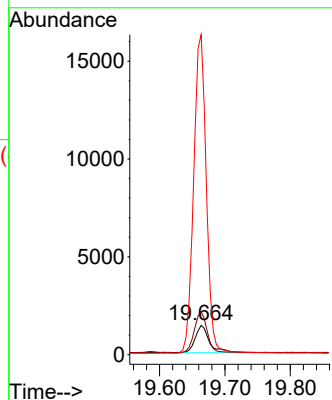

#26

Benzo(a)pyrene

Concen: 0.073 ng/ul

RT: 23.696 min Scan# 4915

Delta R.T. -0.053 min

Lab File: BM041051.D

Acq: 22 Jul 2023 12:43

Tgt Ion:252 Resp: 4613

Ion	Ratio	Lower	Upper
252	100		
253	53.5	28.2	42.2#
125	49.7	25.2	37.8#

