

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072123\
 Data File : BM041058.D
 Acq On : 22 Jul 2023 17:34
 Operator : MA/JU
 Sample : PB154124BL
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Jul 22 22:37:26 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM071923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jul 22 22:33:48 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.857	152	3897	0.400	ng/ul	0.00
4) Naphthalene-d8	10.658	136	13436	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.514	164	7396	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.265	188	14927	0.400	ng/ul	0.00
17) Chrysene-d12	21.466	240	12209	0.400	ng/ul	0.00
23) Perylene-d12	23.848	264	16752	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.271	96	33016	5.153	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.264	152	6575	0.367	ng/ul	0.00
18) Fluoranthene-d10	19.301	212	12890	0.251	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.664	202	2009	0.031	ng/ul#	1
26) Benzo(a)pyrene	23.693	252	4084	0.074	ng/ul#	76


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072123\
Data File : BM041058.D
Acq On : 22 Jul 2023 17:34
Operator : MA/JU
Sample : PB154124BL
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Jul 22 22:37:26 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM071923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jul 22 22:33:48 2023
Response via : Initial Calibration

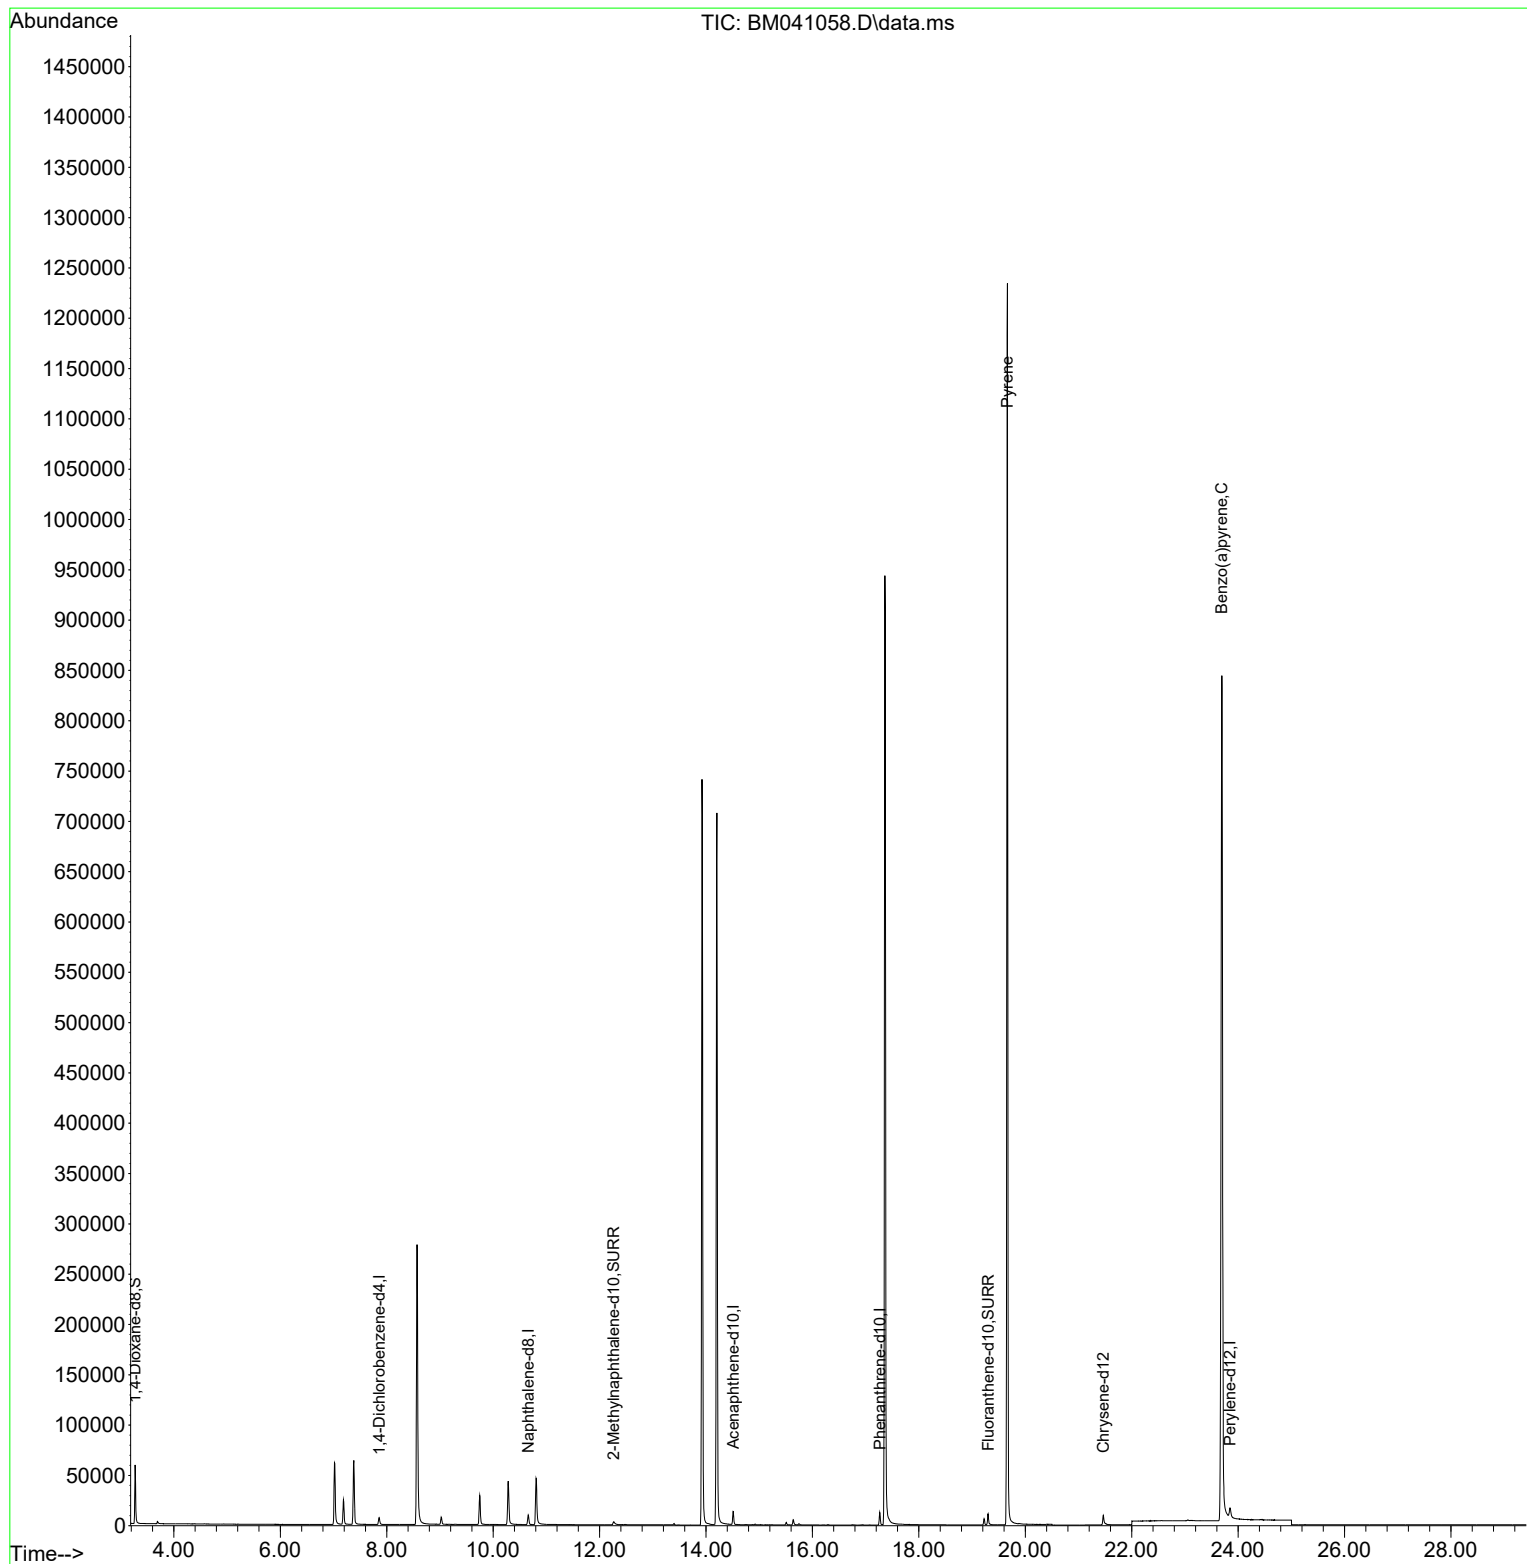

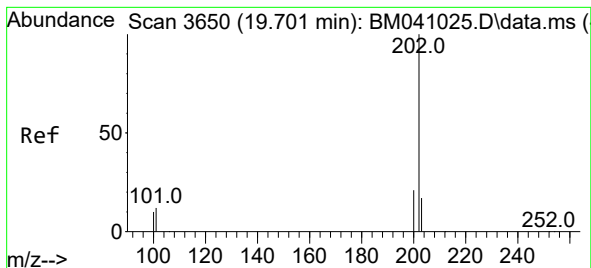

#20

Pyrene

Concen: 0.031 ng/ul

RT: 19.664 min Scan# 3

Delta R.T. -0.032 min


Lab File: BM041058.D

Acq: 22 Jul 2023 17:34

Instrument :

BNA_M

ClientSampleId :

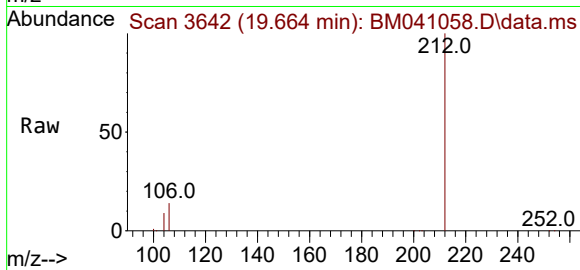




Tgt Ion:202 Resp: 2009

Ion Ratio Lower Upper

202 100

101 141.1 12.5 18.7#

100 1009.6 10.0 15.0#

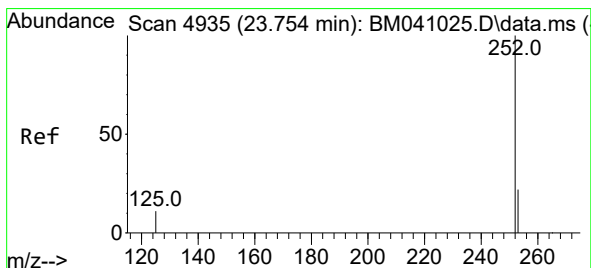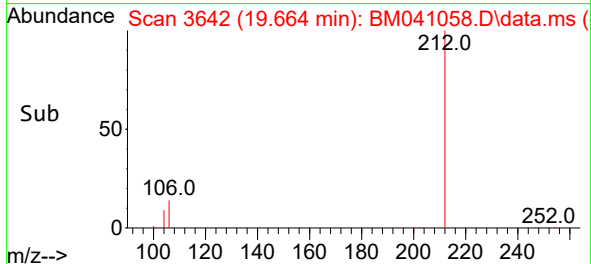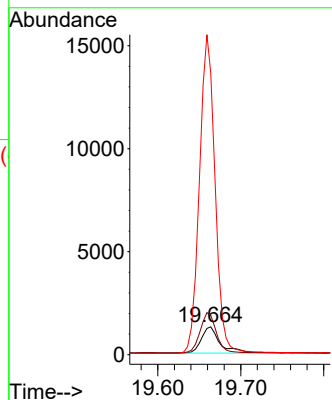

#26

Benzo(a)pyrene

Concen: 0.074 ng/ul

RT: 23.693 min Scan# 4914

Delta R.T. -0.055 min

Lab File: BM041058.D

Acq: 22 Jul 2023 17:34

Tgt Ion:252 Resp: 4084

Ion Ratio Lower Upper

252 100

253 51.2 28.2 42.2#

125 42.4 25.2 37.8#

