

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072123\
 Data File : BM041016.D
 Acq On : 21 Jul 2023 13:45
 Operator : MA/JU
 Sample : 03472-10
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A46Q4

Quant Time: Jul 21 16:40:58 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM071923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 21 16:33:57 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.862	152	3518	0.400	ng/ul	0.00
4) Naphthalene-d8	10.669	136	11758	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.518	164	5935	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.274	188	12646	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.469	240	10496	0.400	ng/ul	0.00
23) Perylene-d12	23.857	264	11991	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.280	96	16320	2.822	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.264	152	6235	0.398	ng/ul	0.00
18) Fluoranthene-d10	19.306	212	12816	0.290	ng/ul	0.00
Target Compounds						
					Qvalue	
19) Fluoranthene	19.334	202	1188	0.022	ng/ul#	80


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072123\
Data File : BM041016.D
Acq On : 21 Jul 2023 13:45
Operator : MA/JU
Sample : 03472-10
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A46Q4


Quant Time: Jul 21 16:40:58 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM071923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 21 16:33:57 2023
Response via : Initial Calibration

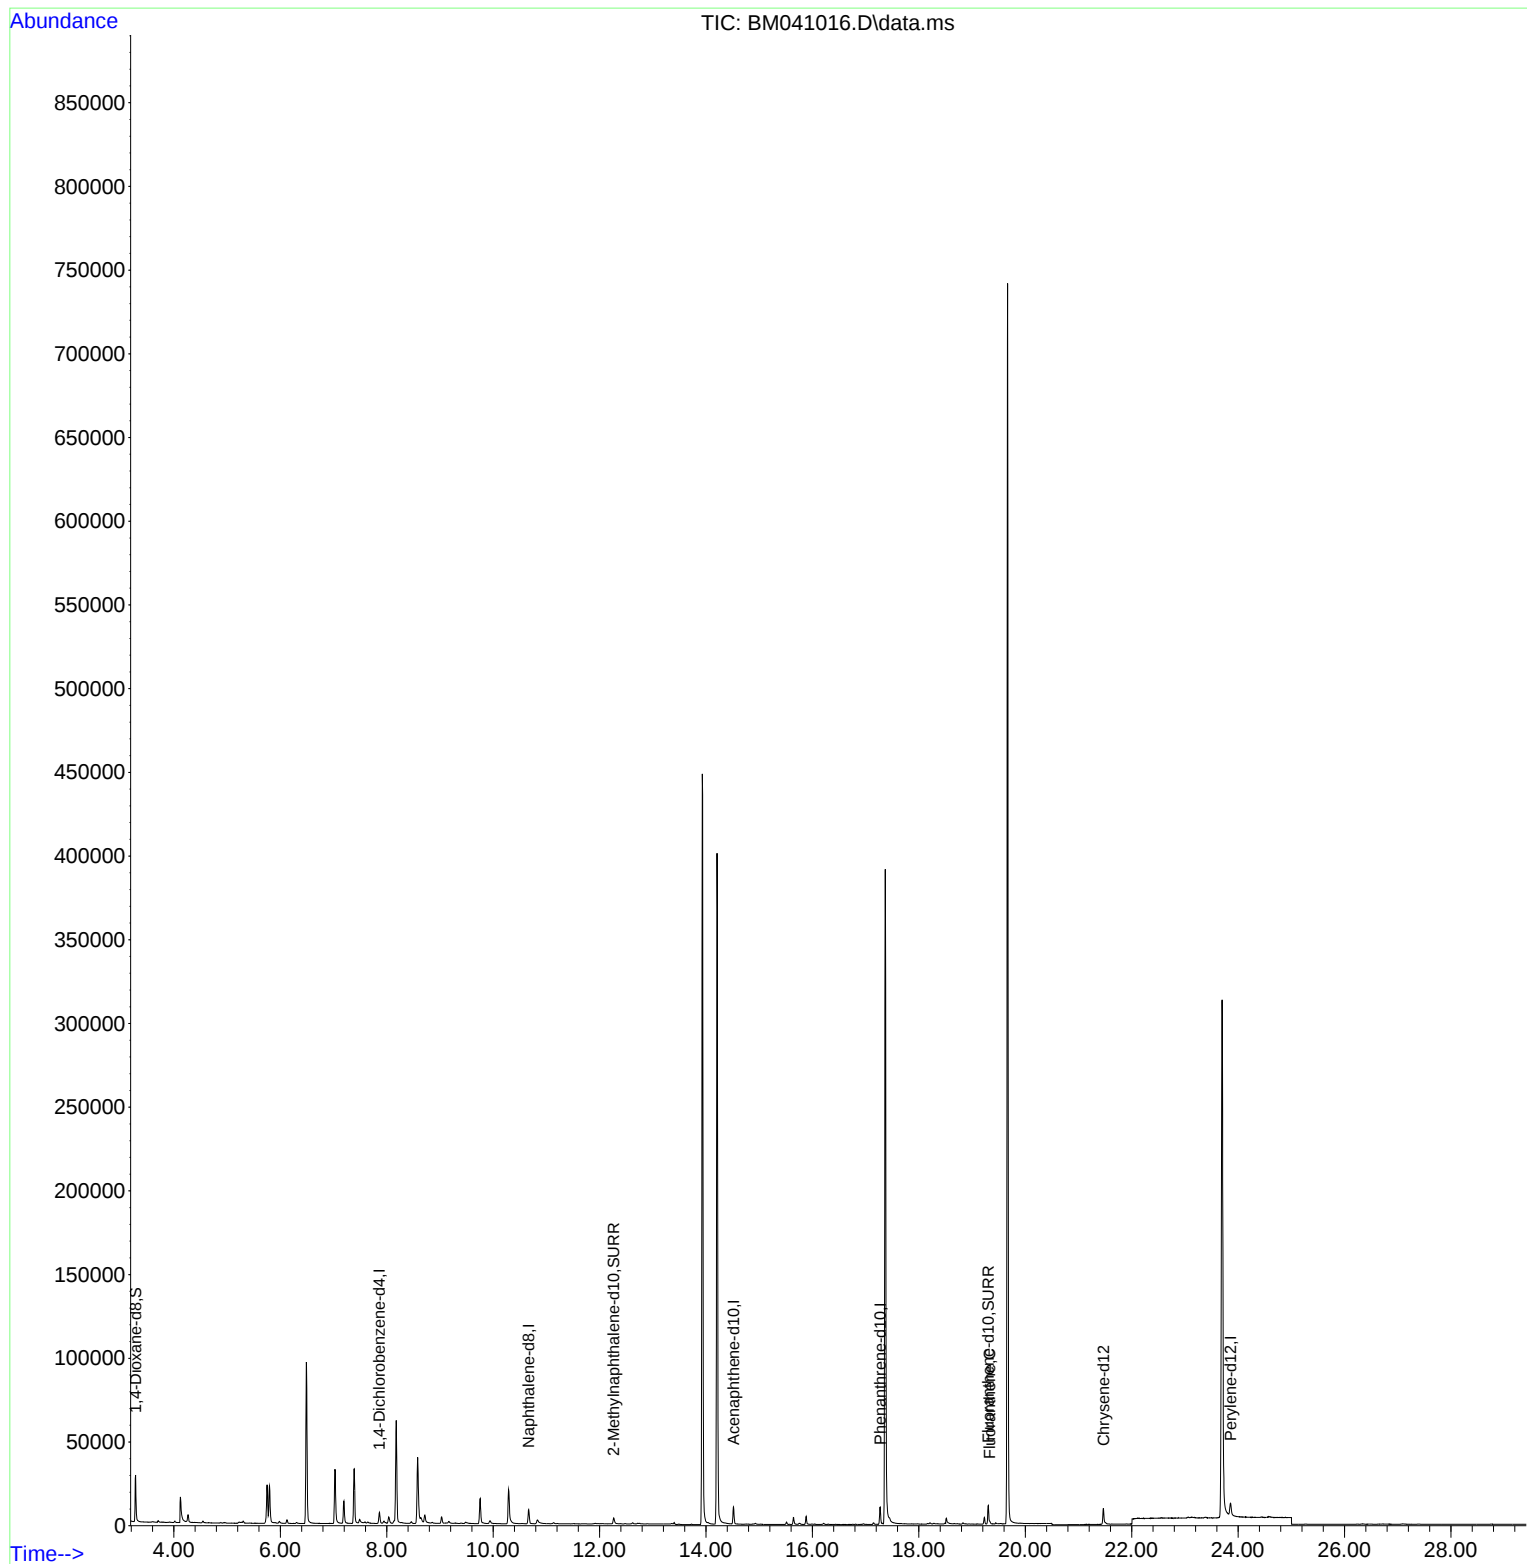

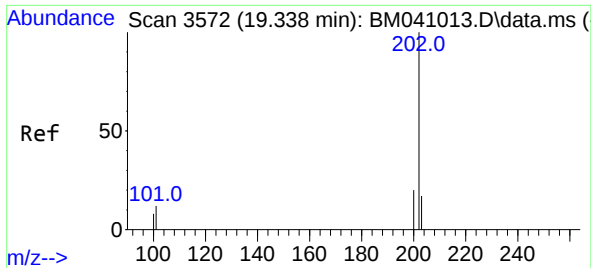

#19
Fluoranthene
Concen: 0.022 ng/ul
RT: 19.334 min Scan# 31
Delta R.T. -0.005 min
Lab File: BM041016.D
Acq: 21 Jul 2023 13:45

Instrument :
BNA_M
ClientSampleId :
A46Q4

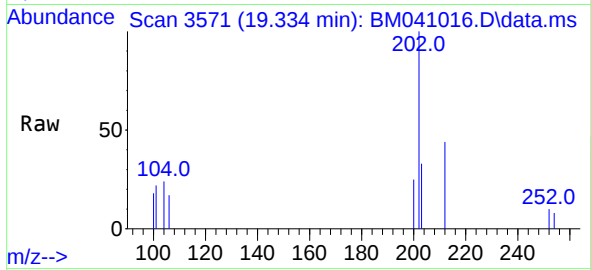

Tgt Ion:202 Resp: 1188
Ion Ratio Lower Upper
202 100
101 21.6 11.0 16.4#
100 18.0 8.3 12.5#

