

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM072219\
 Data File : BM021594.D
 Acq On : 22 Jul 2019 22:10
 Operator : HP/JU
 Sample : K3823-11
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A52L8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM070819MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.881	658	662	674	rVB	133916	240632	3.07%	0.474%
2	7.052	686	691	702	rVB	401535	653918	8.33%	1.289%
3	7.240	717	723	737	rVB	477717	794902	10.13%	1.567%
4	7.705	797	802	811	rVB	445156	720033	9.17%	1.420%
5	8.416	917	923	937	rVB	408307	685189	8.73%	1.351%
6	8.869	994	1000	1015	rVB	603142	1010591	12.88%	1.992%
7	9.587	1115	1122	1134	rVB	481679	815452	10.39%	1.608%
8	10.116	1205	1212	1227	rBV	699515	1313245	16.73%	2.589%
9	10.487	1269	1275	1283	rBV	693756	1157391	14.75%	2.282%
10	10.657	1298	1304	1317	rVB2	51071	119537	1.52%	0.236%
11	12.098	1544	1549	1555	rVB3	7834	14522	0.19%	0.029%
12	13.769	1826	1833	1838	rBV	1935788	2630369	33.51%	5.186%
13	13.816	1838	1841	1849	rVB	115003	159692	2.03%	0.315%
14	14.045	1872	1880	1896	rBV	1984307	2871360	36.59%	5.661%
15	14.351	1925	1932	1939	rBV	1302161	1875345	23.89%	3.697%
16	14.416	1939	1943	1963	rVB	38522	93620	1.19%	0.185%
17	14.586	1966	1972	1988	rBV2	94614	231581	2.95%	0.457%
18	14.775	2000	2004	2010	rBV6	7601	11845	0.15%	0.023%
19	15.110	2057	2061	2066	rBV	62630	81087	1.03%	0.160%
20	15.351	2095	2102	2117	rBV2	3035832	4286147	54.61%	8.450%
21	15.486	2119	2125	2139	rVV	828775	1209633	15.41%	2.385%
22	15.586	2139	2142	2148	rVB	26916	39718	0.51%	0.078%
23	15.822	2179	2182	2186	rVV2	9728	12357	0.16%	0.024%
24	15.863	2186	2189	2195	rVB2	8813	12021	0.15%	0.024%
25	16.092	2225	2228	2231	rVB2	8712	8999	0.11%	0.018%
26	16.128	2231	2234	2239	rVB3	9100	12621	0.16%	0.025%
27	16.186	2239	2244	2248	rBV	16877	24840	0.32%	0.049%
28	16.239	2249	2253	2259	rVB3	27806	45334	0.58%	0.089%
29	16.304	2259	2264	2267	rBV3	17418	25601	0.33%	0.050%
30	16.345	2267	2271	2275	rVB5	11740	17600	0.22%	0.035%
31	16.398	2275	2280	2281	rBV3	10197	10340	0.13%	0.020%
32	16.504	2293	2298	2304	rVB4	17301	32172	0.41%	0.063%
33	16.569	2304	2309	2314	rBV	16880	25288	0.32%	0.050%
34	16.651	2319	2323	2327	rVB2	7408	11583	0.15%	0.023%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM072219\
Data File : BM021594.D
Acq On : 22 Jul 2019 22:10
Operator : HP/JU
Sample : K3823-11
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A52L8

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM070819MA.M
Title : SVOA CALIBRATION

35	16.886	2360	2363	2368	rBV3	5246	8424	0.11%	0.017%
36	17.104	2394	2400	2408	rBV2	1796973	2463399	31.39%	4.857%
37	17.204	2410	2417	2428	rBV	3559580	4951065	63.08%	9.761%
38	17.463	2456	2461	2464	rBV5	5941	10454	0.13%	0.021%
39	17.992	2546	2551	2561	rBV	121875	192531	2.45%	0.380%
40	19.139	2741	2746	2750	rBV	40755	57150	0.73%	0.113%
41	19.280	2766	2770	2777	rBV4	53286	88342	1.13%	0.174%
42	19.386	2785	2788	2795	rVB	31811	43184	0.55%	0.085%
43	19.504	2801	2808	2820	rBV	4886065	6638241	84.58%	13.087%
44	21.004	3059	3063	3070	rBV2	112857	205574	2.62%	0.405%
45	21.292	3107	3112	3121	rBV	2525441	3326199	42.38%	6.558%
46	23.404	3464	3471	3483	rVB	4324992	7848450	100.00%	15.473%
47	23.545	3489	3495	3508	rVB	1949601	3634550	46.31%	7.166%


Sum of corrected areas: 50722128

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM072219\
Data File : BM021594.D
Acq On : 22 Jul 2019 22:10
Operator : HP/JU
Sample : K3823-11
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A52L8

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM070819MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

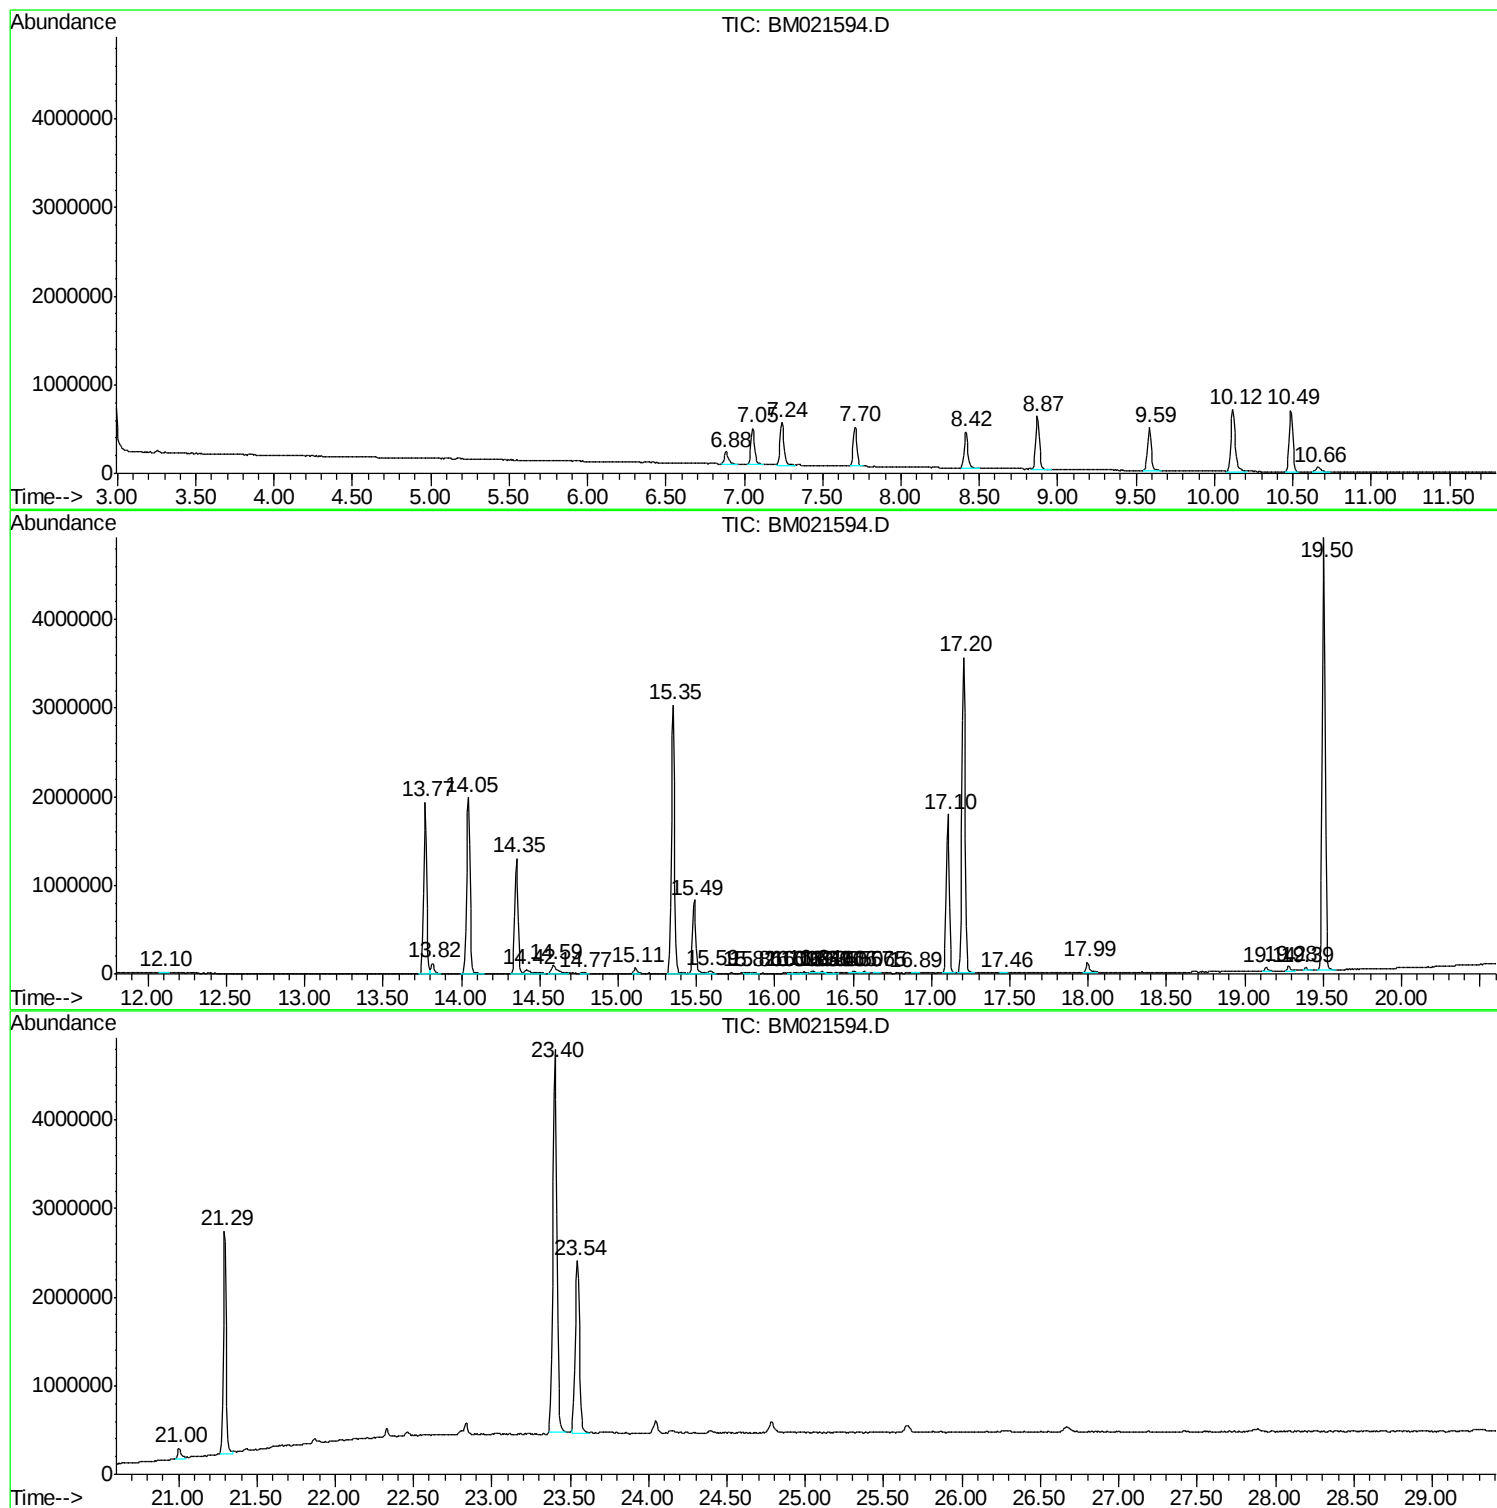

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM072219\
Data File : BM021594.D
Acq On : 22 Jul 2019 22:10
Operator : HP/JU
Sample : K3823-11
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A52L8

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM070819MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM072219\
Data File : BM021594.D
Acq On : 22 Jul 2019 22:10
Operator : HP/JU
Sample : K3823-11
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A52L8

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM070819MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc