

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072221\
 Data File : BM031060.D
 Acq On : 22 Jul 2021 11:00
 Operator : CG/JU
 Sample : M2971-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGE77

Quant Time: Jul 22 11:33:52 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM072221.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 22 10:17:09 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.639	152	1048	0.400	ng/ul	0.00
4) Naphthalene-d8	10.401	136	4135	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.265	164	3070	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.013	188	6487	0.400	ng/ul	0.00
17) Chrysene-d12	21.197	240	6448	0.400	ng/ul	0.00
23) Perylene-d12	23.375	264	6864	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.213	96	5264	4.782	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.993	152	2215	0.305	ng/ul	0.00
18) Fluoranthene-d10	19.043	212	6029	0.307	ng/ul	0.00
Target Compounds						
15) Phenanthrene	17.051	178	614	0.030	ng/ul#	Qvalue 76


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072221\
Data File : BM031060.D
Acq On : 22 Jul 2021 11:00
Operator : CG/JU
Sample : M2971-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGE77


Quant Time: Jul 22 11:33:52 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM072221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 22 10:17:09 2021
Response via : Initial Calibration

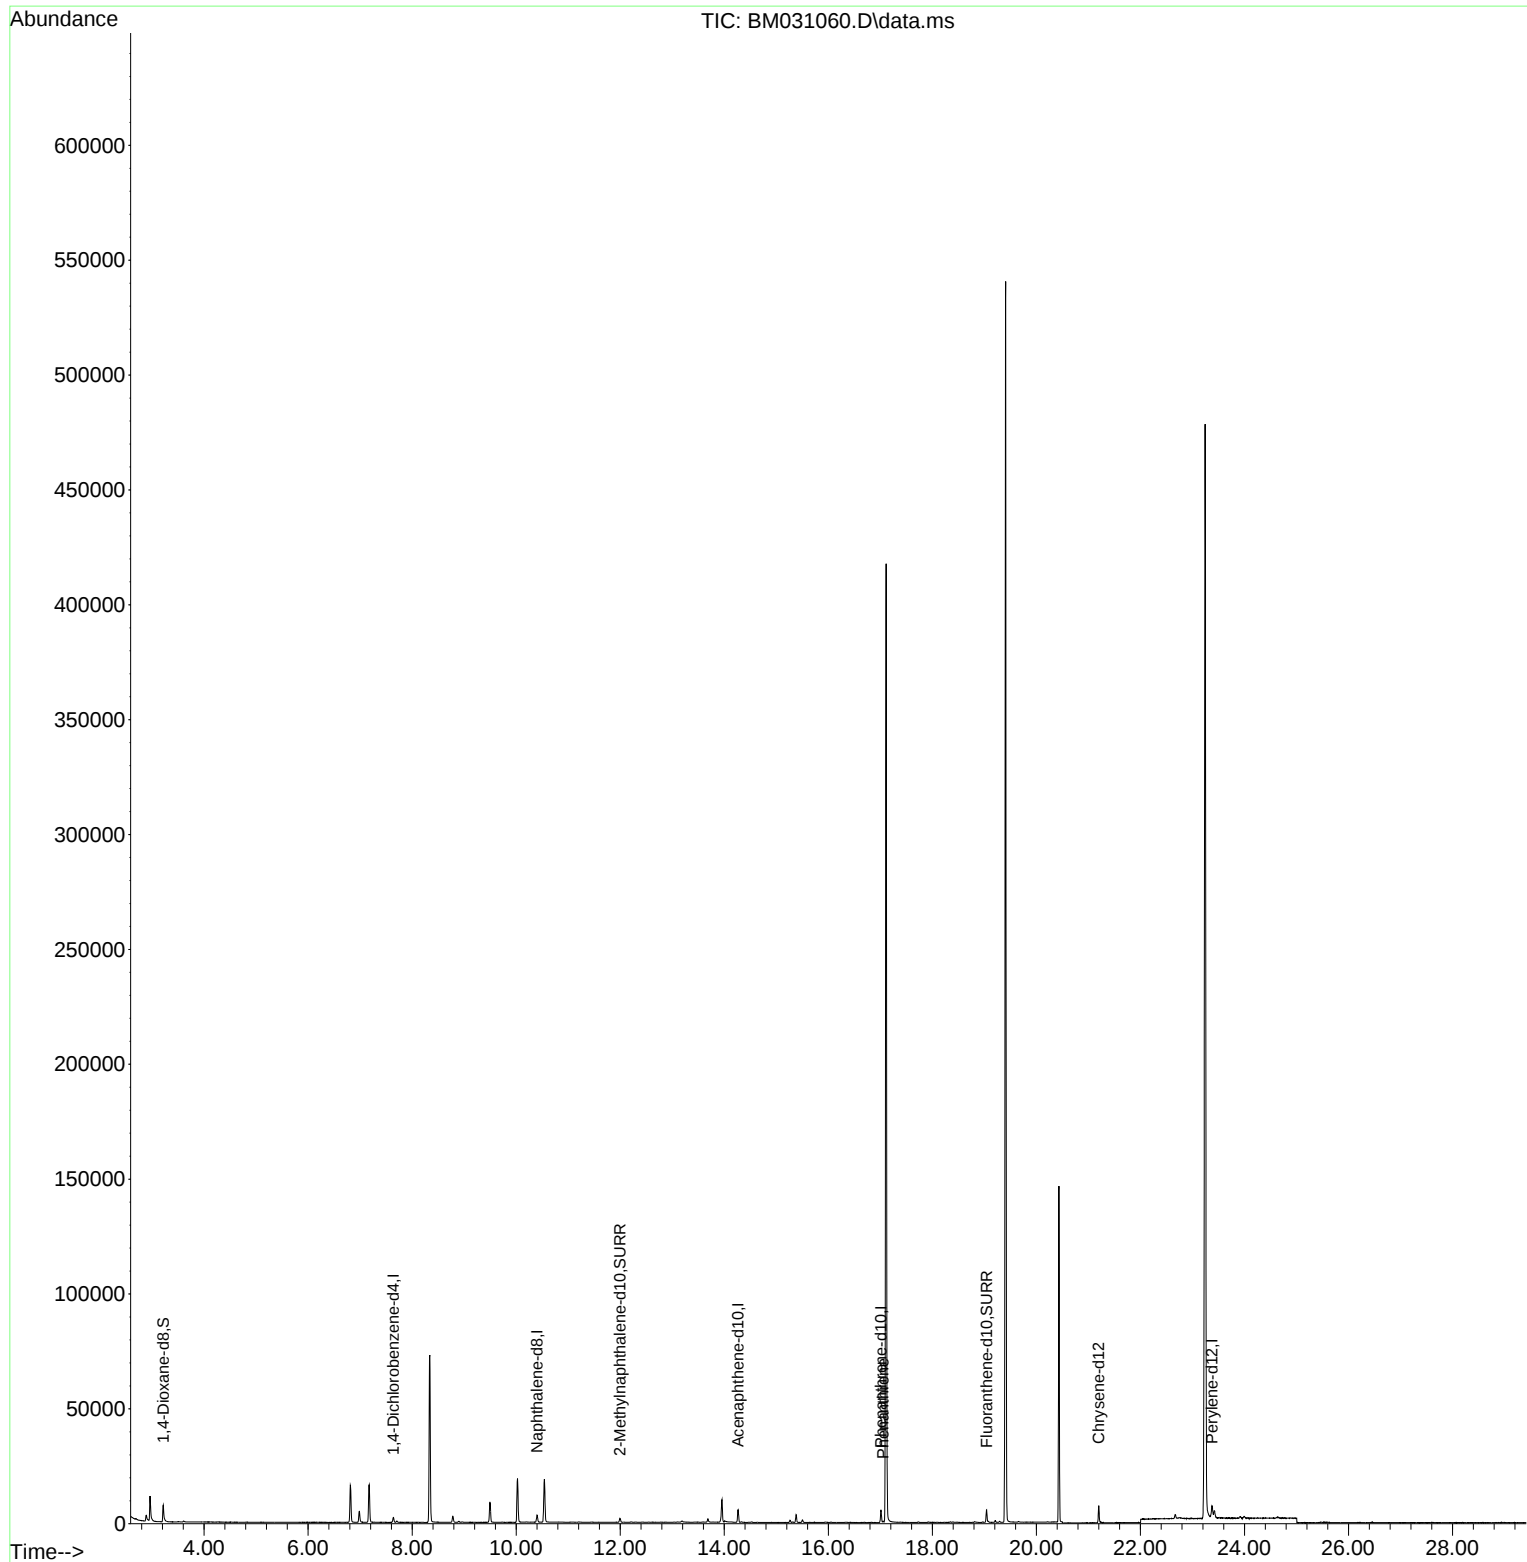

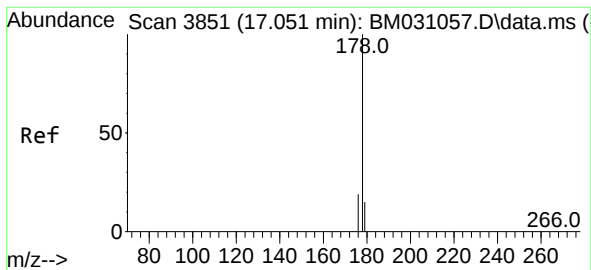

#15
 Phenanthrene
 Concen: 0.030 ng/ul
 RT: 17.051 min Scan# 3851
 Delta R.T. -0.000 min
 Lab File: BM031060.D
 Acq: 22 Jul 2021 11:00

Instrument :
 BNA_M
 ClientSampleId :
 BGE77

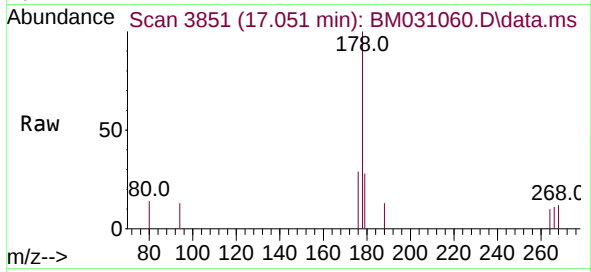

Tgt Ion:178 Resp: 614
 Ion Ratio Lower Upper
 178 100
 179 28.1 13.3 19.9#
 176 28.7 15.4 23.2#

