

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072221\
 Data File : BM031086.D
 Acq On : 23 Jul 2021 11:26
 Operator : CG/JU
 Sample : M2970-16DL 5X
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGE17DL

Manual Integrations
 APPROVED

mohammad
 7/26/2021 7:59:52 AM

Quant Time: Jul 23 11:57:54 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM072221.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 22 11:33:47 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.632	152	1966	0.400	ng/ul	0.00
4) Naphthalene-d8	10.397	136	7997	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.262	164	5424	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.010	188	11917	0.400	ng/ul	0.00
17) Chrysene-d12	21.198	240	11979	0.400	ng/ul	# 0.00
23) Perylene-d12	23.372	264	11844	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.213	96	1130	0.547	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.989	152	582	0.041	ng/ul	0.00
18) Fluoranthene-d10	19.039	212	1554	0.043	ng/ul	0.00
Target Compounds						
					Qvalue	
5) Naphthalene	10.446	128	8931	0.374	ng/ul	98
7) 2-Methylnaphthalene	12.065	142	1430	0.083	ng/ul	99
8) 1-Methylnaphthalene	12.286	142	375	0.022	ng/ul	100
10) Acenaphthylene	13.981	152	13944	0.629	ng/ul	97
11) Acenaphthene	14.326	153	9836	0.502	ng/ul	98
12) Fluorene	15.316	166	15390	0.667	ng/ul	99
15) Phenanthrene	17.051	178	407813	10.775	ng/ul	99
16) Anthracene	17.141	178	167047	4.711	ng/ul	97
19) Fluoranthene	19.070	202	865722	17.952	ng/ul	96
20) Pyrene	19.432	202	503991	10.237	ng/ul	96
21) Benzo(a)anthracene	21.183	228	495568	10.358	ng/ul	96
22) Chrysene	21.234	228	390440	7.540	ng/ul	98
24) Benzo(b)fluoranthene	22.730	252	442295m	7.943	ng/ul	
25) Benzo(k)fluoranthene	22.767	252	194413m	3.441	ng/ul	
26) Benzo(a)pyrene	23.280	252	168532	3.501	ng/ul#	91
27) Indeno(1,2,3-cd)pyrene	25.529	276	106954	1.696	ng/ul#	97
28) Dibenzo(a,h)anthracene	25.541	278	46973	0.928	ng/ul	98
29) Benzo(g,h,i)perylene	26.185	276	3678	0.069	ng/ul#	65

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072221\
Data File : BM031086.D
Acq On : 23 Jul 2021 11:26
Operator : CG/JU
Sample : M2970-16DL 5X
Misc :
ALS Vial : 31 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
BGE17DL

Manual Integrations
APPROVED

mohammad
7/26/2021 7:59:52 AM

Quant Time: Jul 23 11:57:54 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM072221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 22 11:33:47 2021
Response via : Initial Calibration

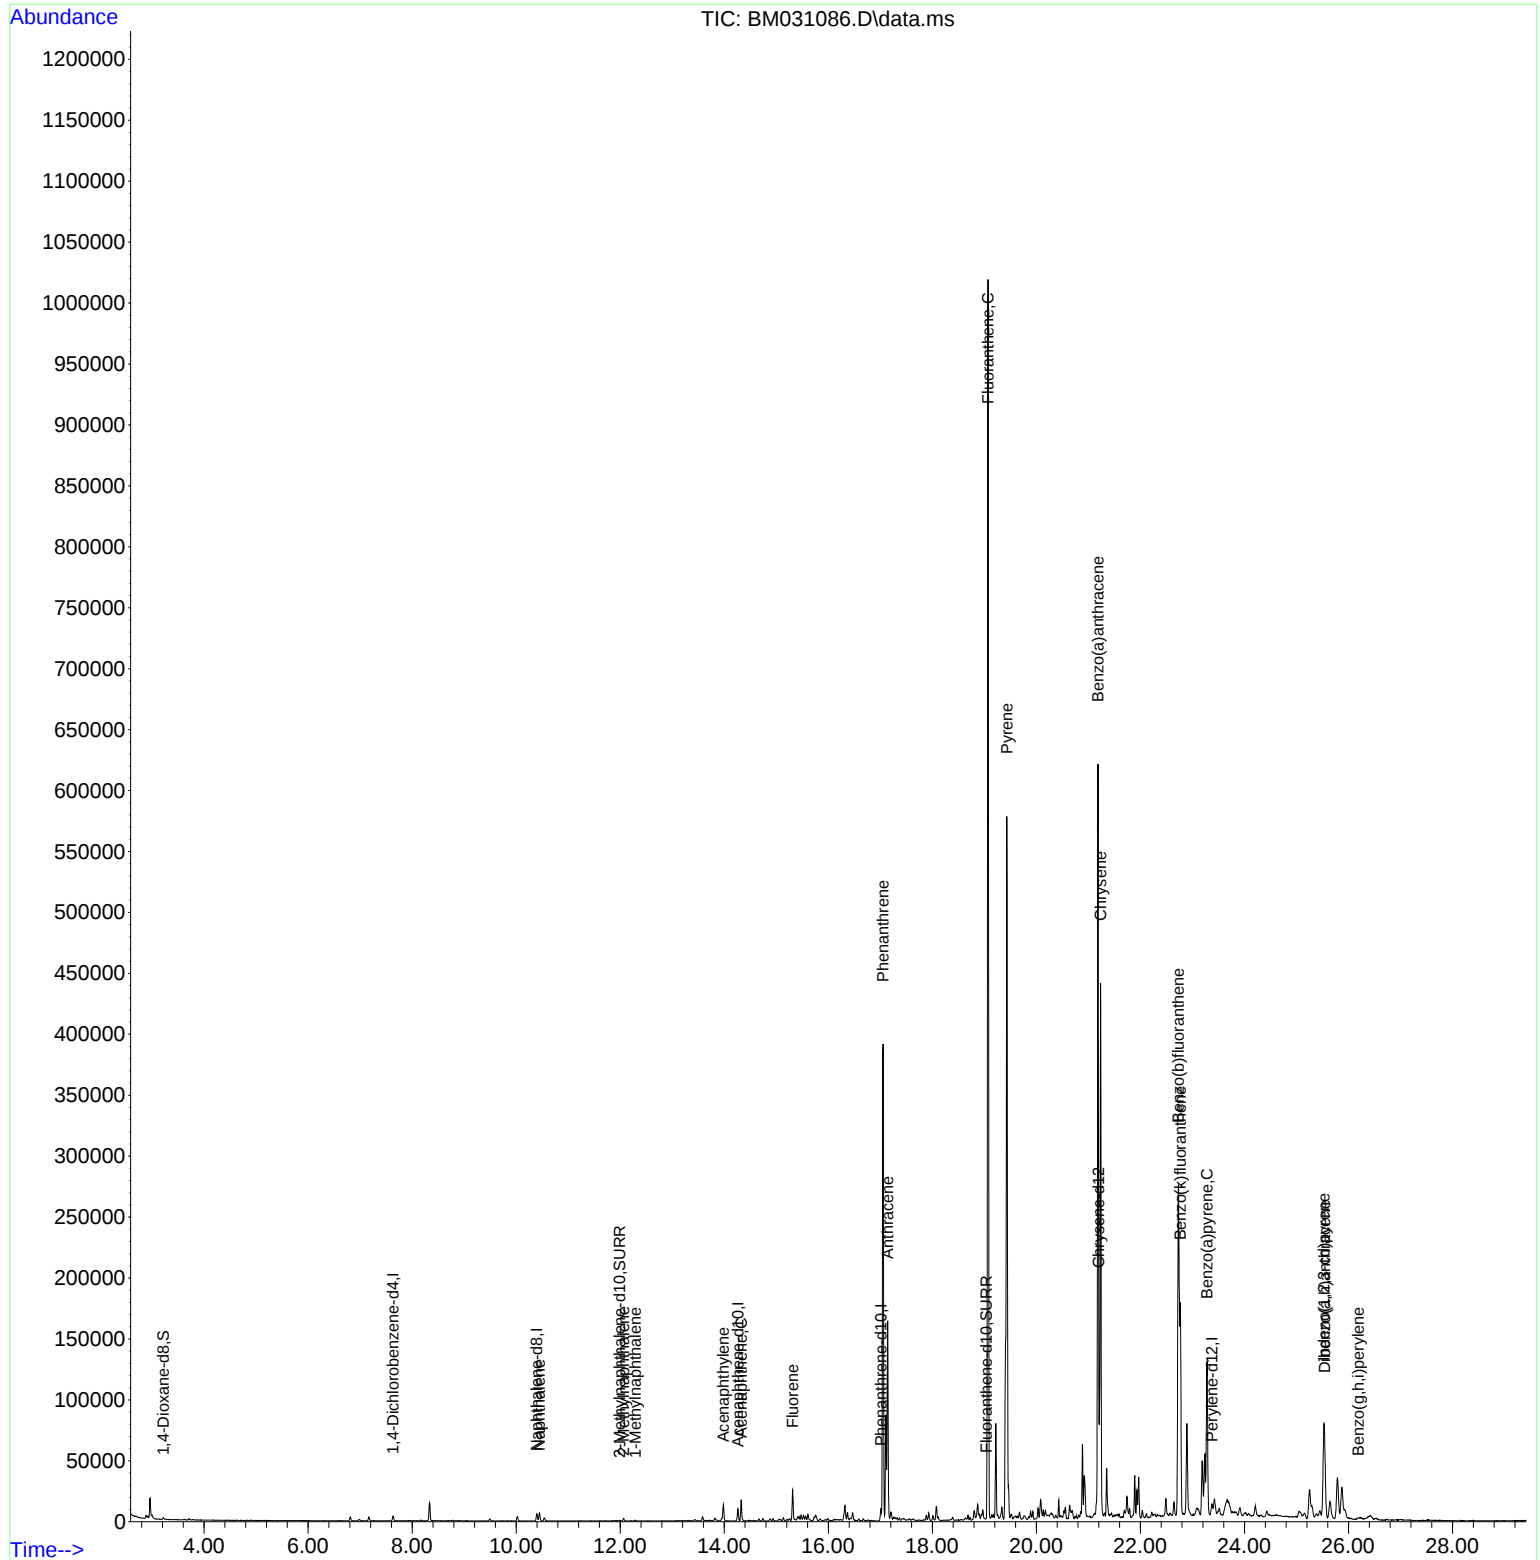







#5
Naphthalene
Concen: 0.374 ng/ul
RT: 10.446 min Scan# 2243
Delta R.T. -0.004 min
Lab File: BM031086.D
Acq: 23 Jul 2021 11:26

Tgt Ion:	128	Resp:	8931
Ion Ratio	Lower	Upper	
128	100		
129	11.9	10.2	15.4
127	14.0	11.8	17.8

Instrument :
BNA_M
ClientSampleId :
BGE17DL




Manual Integrations
APPROVED


mohammad
7/26/2021 7:59:52 AM

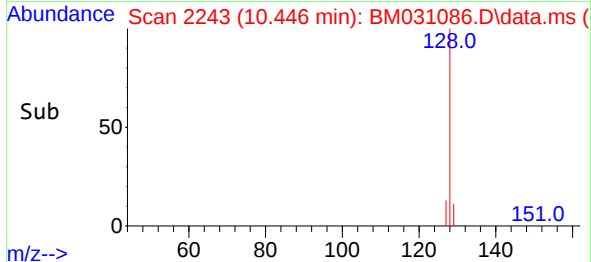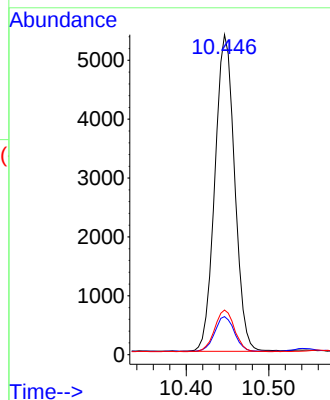

#7
2-Methylnaphthalene
Concen: 0.083 ng/ul
RT: 12.065 min Scan# 2603
Delta R.T. -0.004 min
Lab File: BM031086.D
Acq: 23 Jul 2021 11:26

Tgt Ion:	142	Resp:	1430
Ion Ratio	Lower	Upper	
142	100		
141	90.6	71.5	107.3

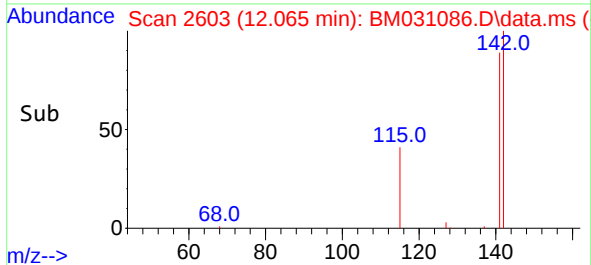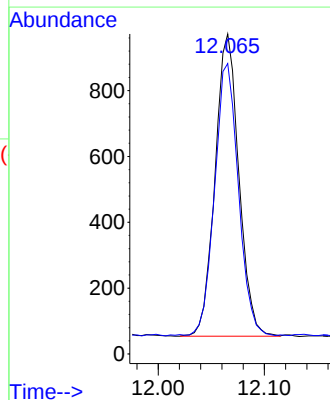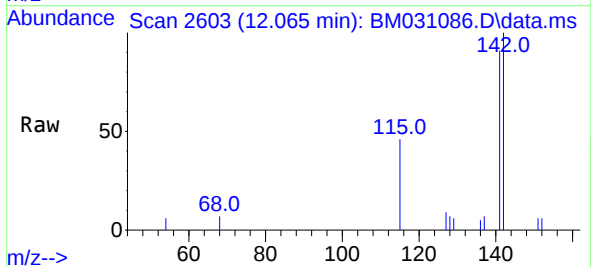







#8
1-Methylnaphthalene
Concen: 0.022 ng/ul
RT: 12.286 min Scan# 2652
Delta R.T. -0.004 min
Lab File: BM031086.D
Acq: 23 Jul 2021 11:26

Tgt Ion:142 Resp: 375
Ion Ratio Lower Upper
142 100
141 93.1 74.2 111.4

Instrument :
BNA_M
ClientSampled :
BGE17DL




Manual Integrations
APPROVED


mohammad
7/26/2021 7:59:52 AM

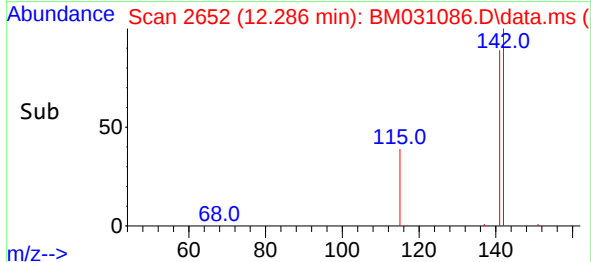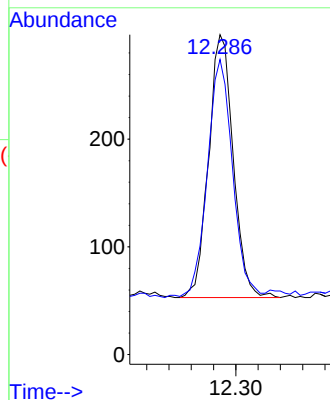

#10
Acenaphthylene
Concen: 0.629 ng/ul
RT: 13.981 min Scan# 3029
Delta R.T. -0.004 min
Lab File: BM031086.D
Acq: 23 Jul 2021 11:26


Tgt Ion:152 Resp: 13944
Ion Ratio Lower Upper
152 100
151 20.4 17.5 26.3
153 0.0 0.0 0.0

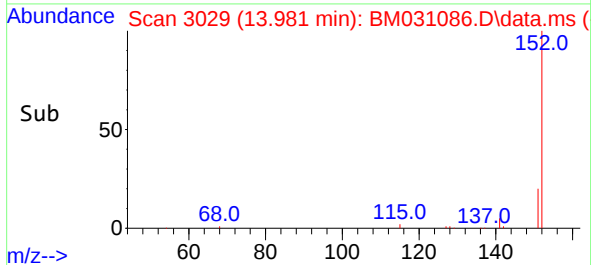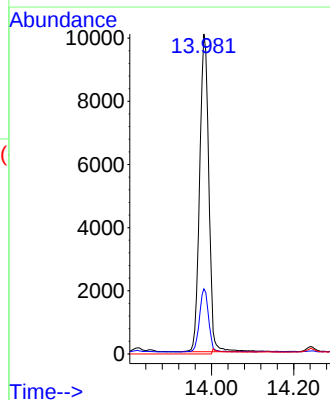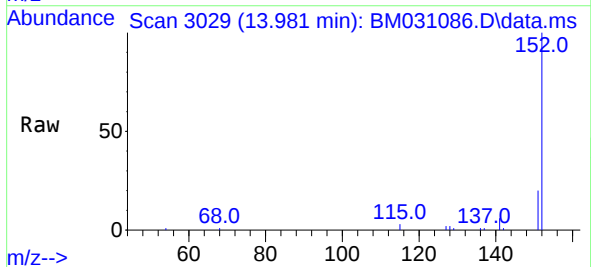



#11
Acenaphthene
Concen: 0.502 ng/ul
RT: 14.326 min Scan# 3119
Delta R.T. 0.000 min
Lab File: BM031086.D
Acq: 23 Jul 2021 11:26




Instrument :
BNA_M
ClientSampled :
BGE17DL




Tgt Ion:153 Resp: 9836
Ion Ratio Lower Upper
153 100
152 48.8 39.4 59.2
154 87.4 68.2 102.4

Manual Integrations
APPROVED



mohammad
7/26/2021 7:59:52 AM

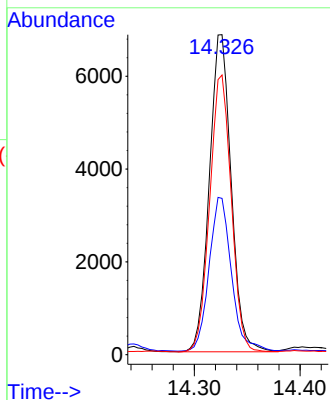


#12
Fluorene
Concen: 0.667 ng/ul
RT: 15.316 min Scan# 3380
Delta R.T. 0.000 min
Lab File: BM031086.D
Acq: 23 Jul 2021 11:26

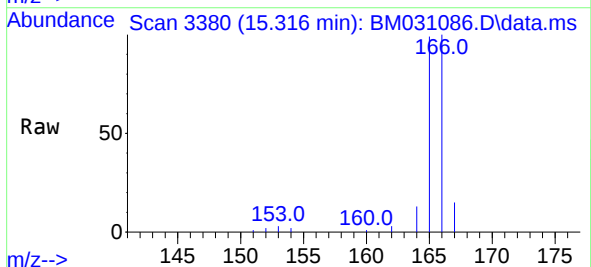


Tgt Ion:166 Resp: 15390
Ion Ratio Lower Upper
166 100
165 99.1 78.2 117.2
167 15.3 12.3 18.5

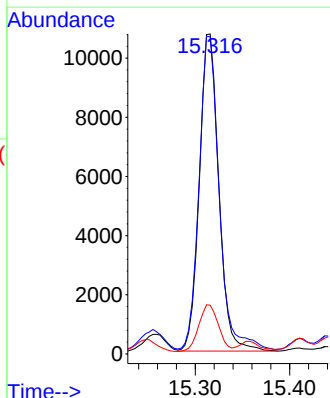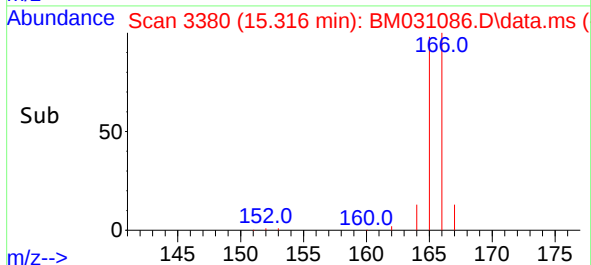



#15
Phenanthrene
Concen: 10.775 ng/ul
RT: 17.051 min Scan# 3851
Delta R.T. 0.000 min
Lab File: BM031086.D
Acq: 23 Jul 2021 11:26




Instrument :
BNA_M
ClientSampled :
BGE17DL



Tgt Ion:178 Resp: 407813
Ion Ratio Lower Upper
178 100
179 15.5 13.3 19.9
176 19.2 15.4 23.2




Manual Integrations
APPROVED


mohammad
7/26/2021 7:59:52 AM

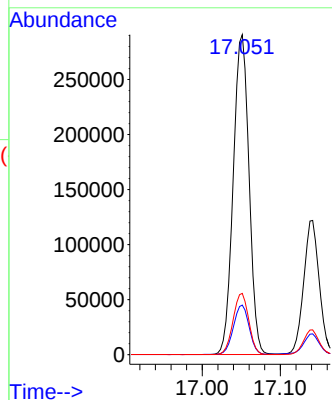

#16
Anthracene
Concen: 4.711 ng/ul
RT: 17.141 min Scan# 3877
Delta R.T. 0.000 min
Lab File: BM031086.D
Acq: 23 Jul 2021 11:26

Tgt Ion:178 Resp: 167047
Ion Ratio Lower Upper
178 100
179 15.6 13.8 20.8
176 18.4 15.7 23.5

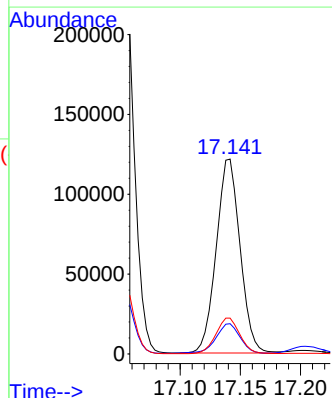







#19
Fluoranthene
Concen: 17.952 ng/u1
RT: 19.070 min Scan# 4418
Delta R.T. 0.000 min
Lab File: BM031086.D
Acq: 23 Jul 2021 11:26

Tgt Ion:202 Resp: 865722
Ion Ratio Lower Upper
202 100
101 9.0 6.0 9.0
100 6.9 4.8 7.2

Instrument :
BNA_M
ClientSampled :
BGE17DL




Manual Integrations
APPROVED


mohammad
7/26/2021 7:59:52 AM

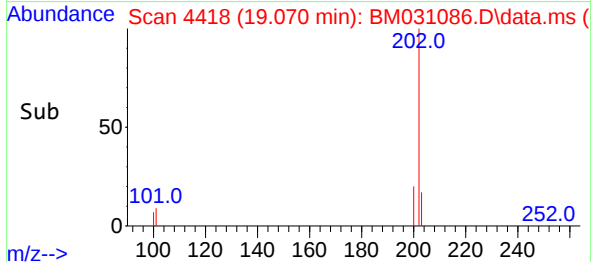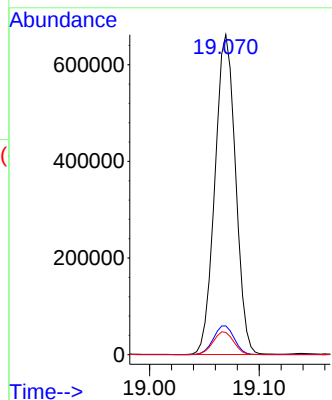

#20
Pyrene
Concen: 10.237 ng/u1
RT: 19.432 min Scan# 4513
Delta R.T. 0.000 min
Lab File: BM031086.D
Acq: 23 Jul 2021 11:26

Tgt Ion:202 Resp: 503991
Ion Ratio Lower Upper
202 100
101 10.5 7.4 11.0
100 8.8 6.0 9.0

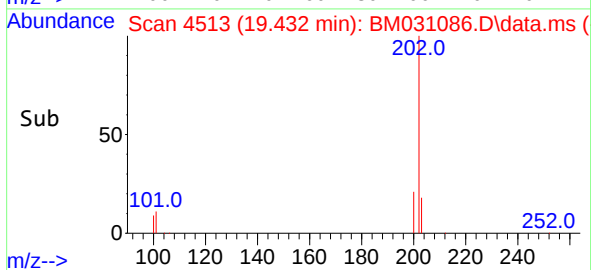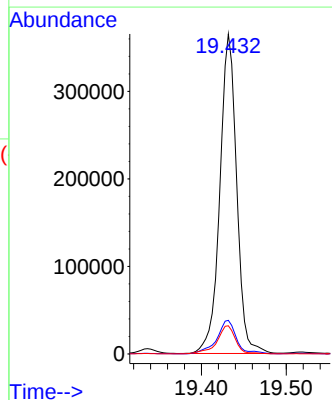







#21
Benzo(a)anthracene
Concen: 10.358 ng/ul
RT: 21.183 min Scan# 5075
Delta R.T. 0.000 min
Lab File: BM031086.D
Acq: 23 Jul 2021 11:26

Tgt Ion:228 Resp: 495568
Ion Ratio Lower Upper
228 100
229 20.3 16.0 24.0
226 30.4 21.4 32.2

Instrument :
BNA_M
ClientSampled :
BGE17DL




Manual Integrations
APPROVED


mohammad
7/26/2021 7:59:52 AM

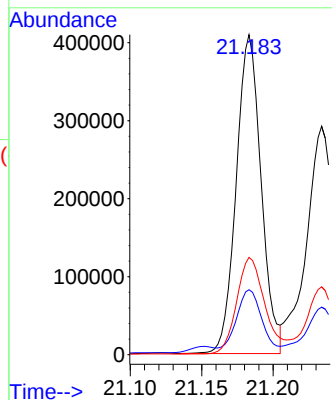


#22
Chrysene
Concen: 7.540 ng/ul
RT: 21.234 min Scan# 5096
Delta R.T. 0.000 min
Lab File: BM031086.D
Acq: 23 Jul 2021 11:26

Tgt Ion:228 Resp: 390440
Ion Ratio Lower Upper
228 100
226 29.7 24.5 36.7
229 20.8 15.8 23.8

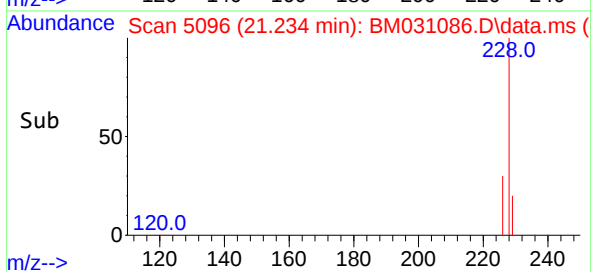

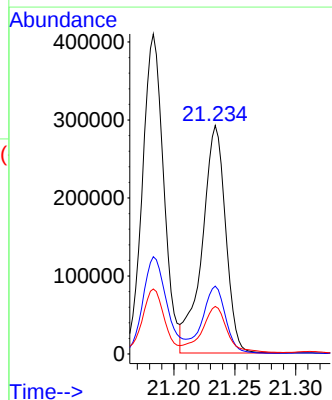





#24
Benzo(b)fluoranthene
Concen: 7.943 ng/ul m
RT: 22.730 min Scan# 5714
Delta R.T. 0.005 min
Lab File: BM031086.D
Acq: 23 Jul 2021 11:26





Tgt Ion:252 Resp: 442295
Ion Ratio Lower Upper
252 100
253 22.5 0.0 52.8
125 9.7 0.0 20.2

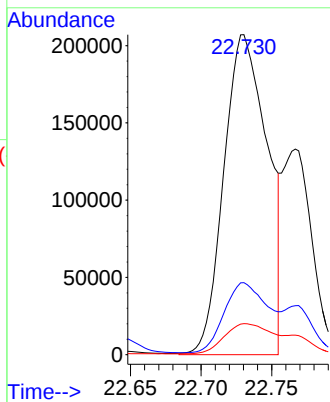

#25
Benzo(k)fluoranthene
Concen: 3.441 ng/ul m
RT: 22.767 min Scan# 5729
Delta R.T. -0.002 min
Lab File: BM031086.D
Acq: 23 Jul 2021 11:26

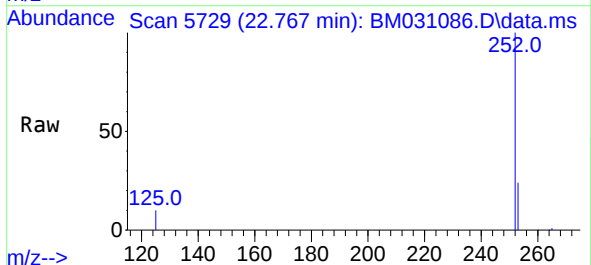


Tgt Ion:252 Resp: 194413
Ion Ratio Lower Upper
252 100
253 23.9 21.6 32.4
125 9.5 8.6 13.0

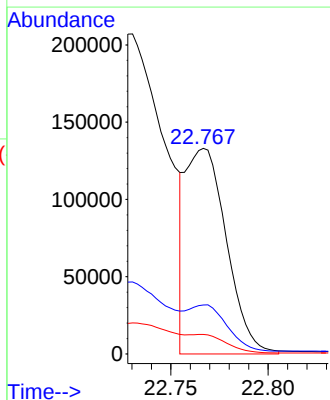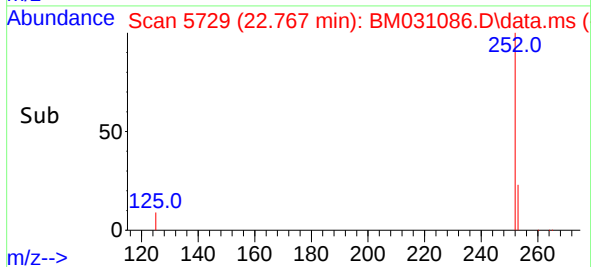

Instrument :
BNA_M
ClientSampled :
BGE17DL

Manual Integrations
APPROVED

mohammad
7/26/2021 7:59:52 AM







#26
Benzo(a)pyrene
Concen: 3.501 ng/ul
RT: 23.280 min Scan# 5941
Delta R.T. 0.000 min
Lab File: BM031086.D
Acq: 23 Jul 2021 11:26

Tgt Ion:252 Resp: 168532
Ion Ratio Lower Upper
252 100
253 23.9 23.1 34.7
125 10.4 10.7 16.1#

Instrument :
BNA_M
ClientSampled :
BGE17DL




Manual Integrations
APPROVED


mohammad
7/26/2021 7:59:52 AM

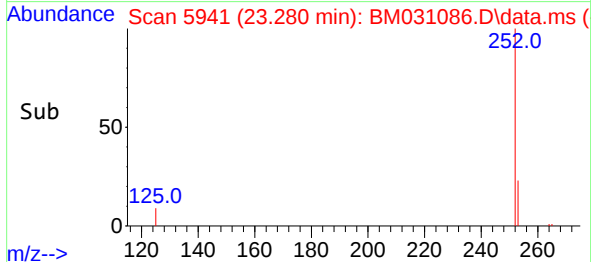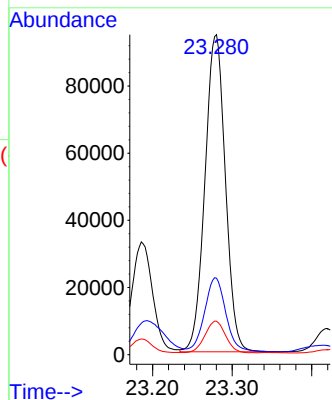

#27
Indeno(1,2,3-cd)pyrene
Concen: 1.696 ng/ul
RT: 25.529 min Scan# 6869
Delta R.T. -0.007 min
Lab File: BM031086.D
Acq: 23 Jul 2021 11:26

Tgt Ion:276 Resp: 106954
Ion Ratio Lower Upper
276 100
138 20.7 15.4 23.0
227 0.0 0.0 0.0

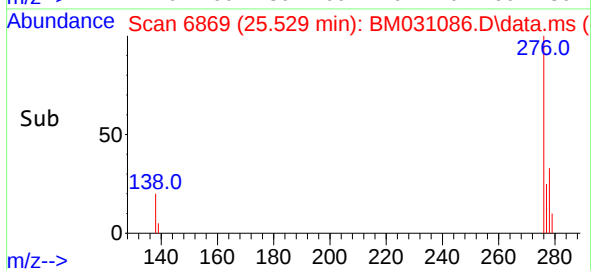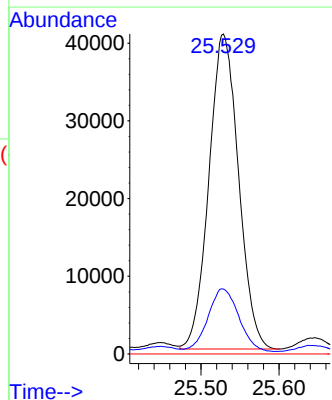







#28
Dibenzo(a,h)anthracene
Concen: 0.928 ng/ul
RT: 25.541 min Scan# 6874
Delta R.T. -0.010 min
Lab File: BM031086.D
Acq: 23 Jul 2021 11:26

Tgt Ion:278 Resp: 46973
Ion Ratio Lower Upper
278 100
139 16.4 12.6 18.8
279 29.3 22.6 34.0

Instrument :
BNA_M
ClientSampled :
BGE17DL




Manual Integrations
APPROVED

mohammad
7/26/2021 7:59:52 AM

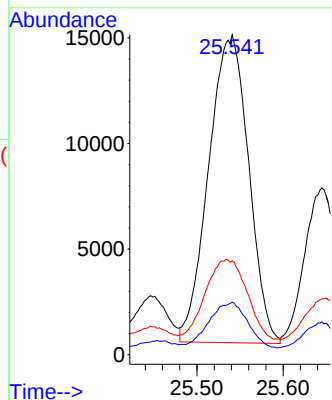

#29
Benzo(g,h,i)perylene
Concen: 0.069 ng/ul
RT: 26.185 min Scan# 7140
Delta R.T. -0.007 min
Lab File: BM031086.D
Acq: 23 Jul 2021 11:26

Tgt Ion:276 Resp: 3678
Ion Ratio Lower Upper
276 100
138 32.8 14.0 21.0#
277 42.2 19.9 29.9#

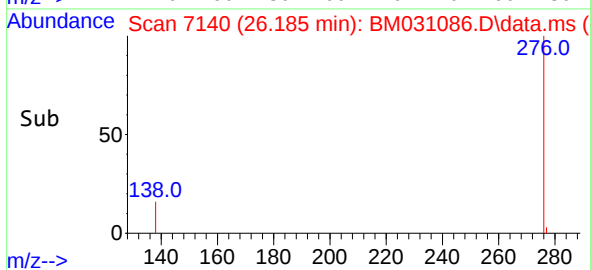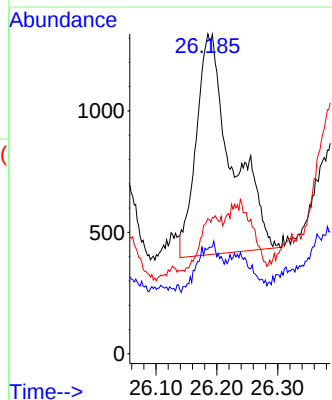


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM072221\
Data File : BM031086.D
Acq On : 23 Jul 2021 11:26
Operator : CG/JU
Sample : M2970-16DL 5X
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGE17DL

Manual Integrations
APPROVED

mohammad
7/26/2021 7:59:52 AM

Quant Time: Jul 23 11:59:47 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM072221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 22 11:33:47 2021
Response via : Initial Calibration

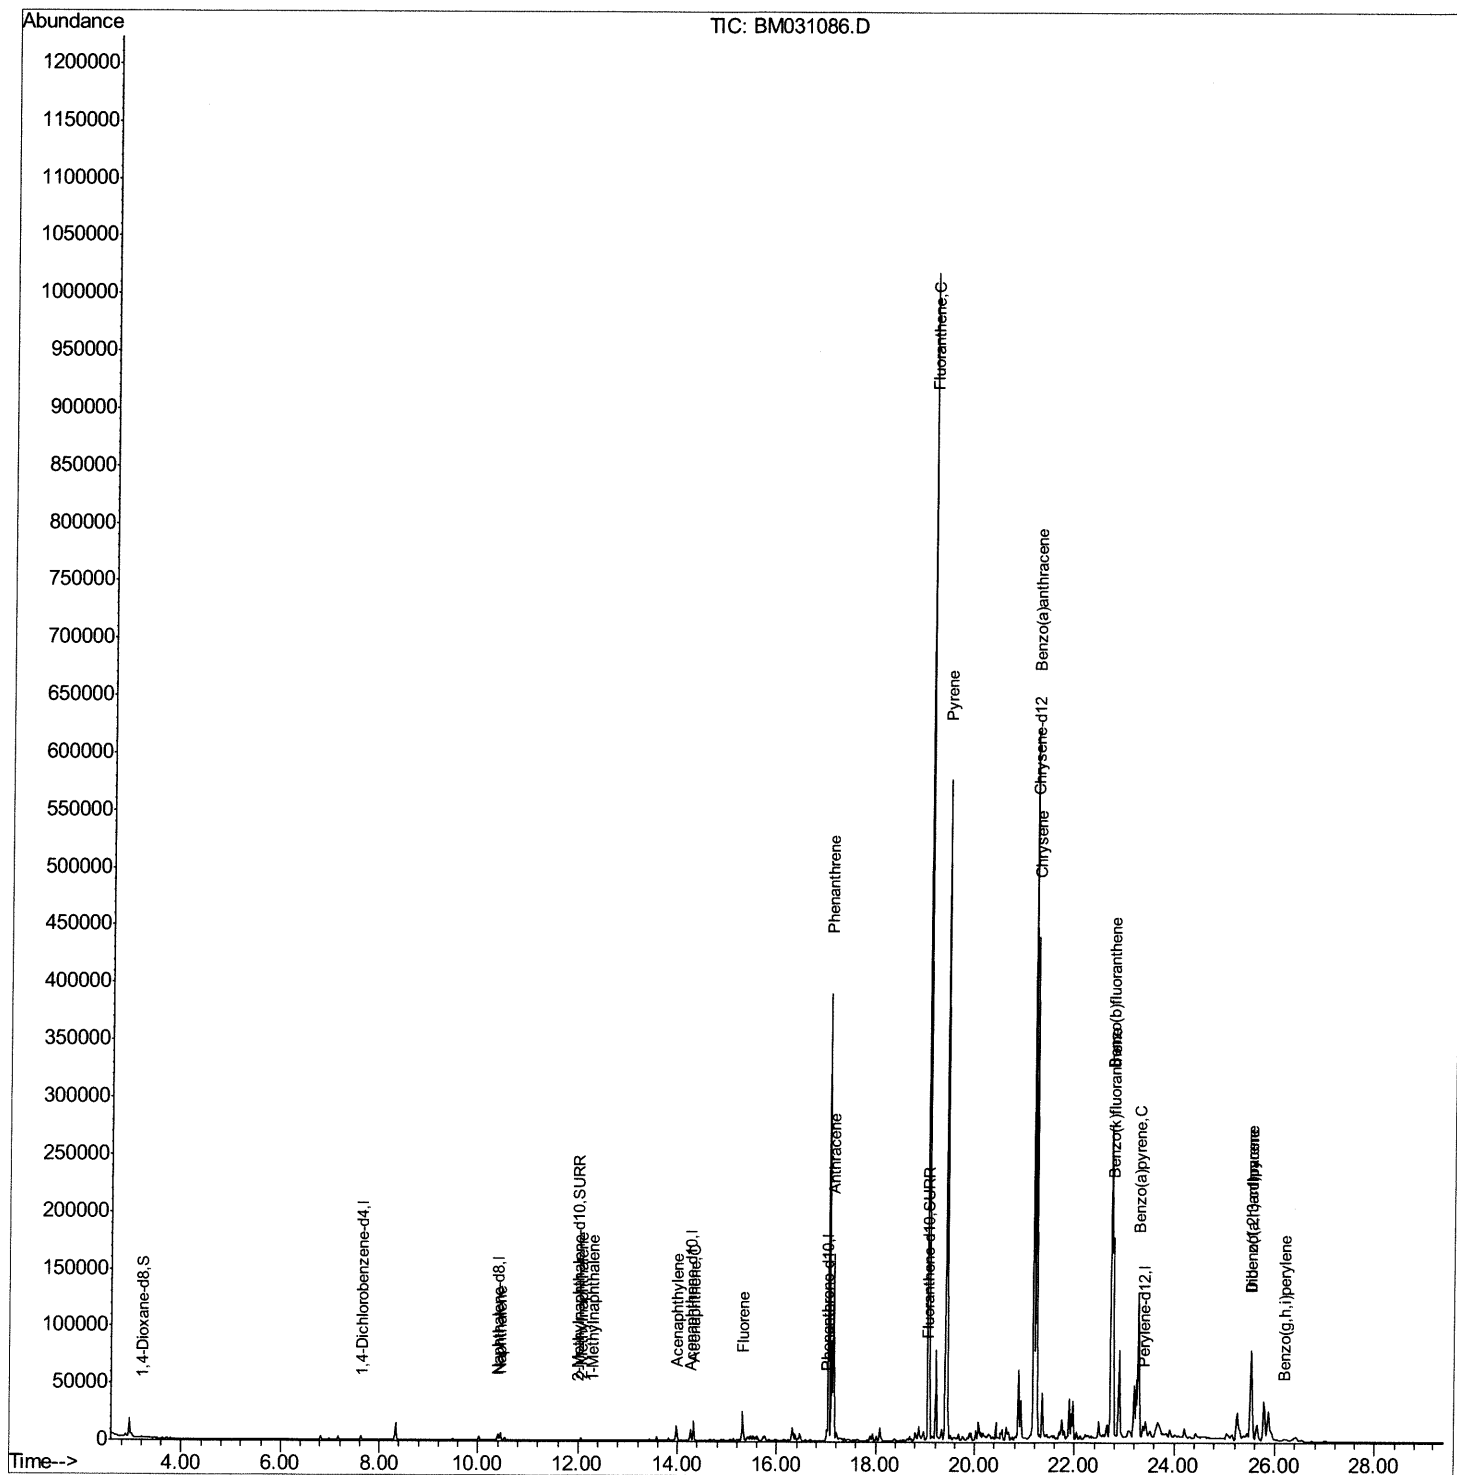

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM072221\
 Data File : BM031086.D
 Acq On : 23 Jul 2021 11:26
 Operator : CG/JU
 Sample : M2970-16DL 5X
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_M
ClientSampleId :
 BGE17DL

Manual Integrations
APPROVED

mohammad
 7/26/2021 7:59:52 AM

Quant Time: Jul 23 11:57:34 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM072221.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 22 11:33:47 2021
 Response via : Initial Calibration

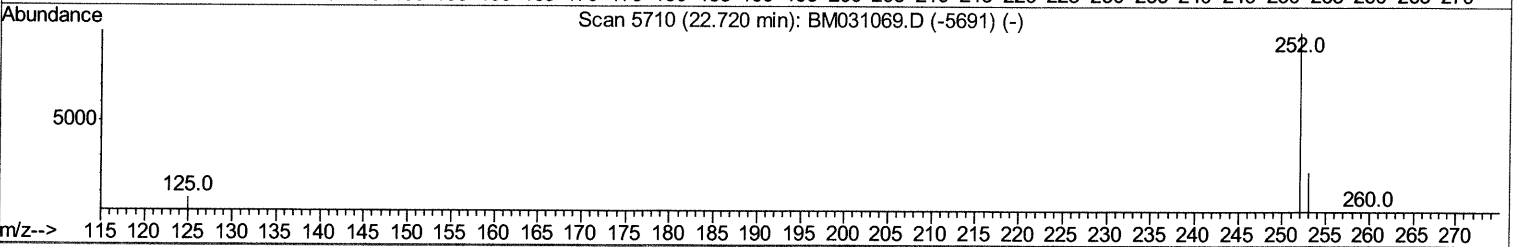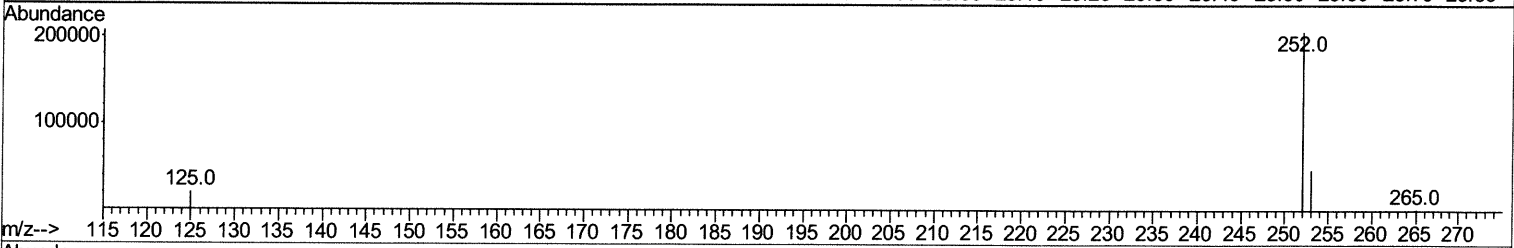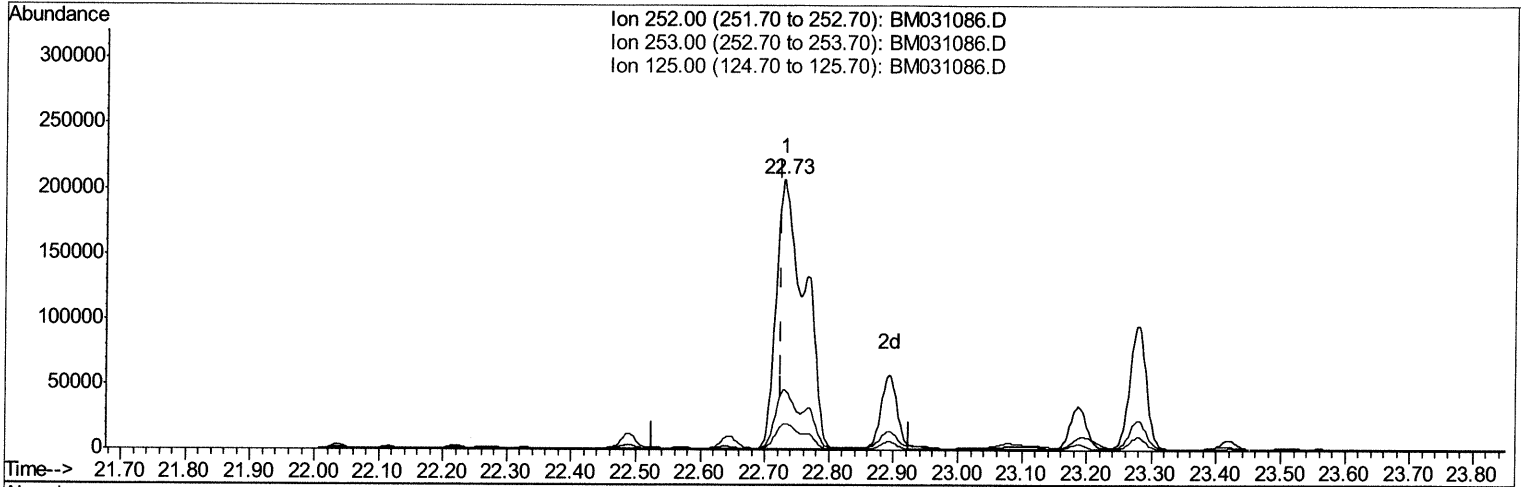

TIC: BM031086.D

(24) Benzo(b)fluoranthene

22.730min (+0.005) 11.36ng/ul

response 632793

Ion	Exp%	Act%
252.00	100	100
253.00	26.40	22.49
125.00	10.10	9.70
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM072221\
 Data File : BM031086.D
 Acq On : 23 Jul 2021 11:26
 Operator : CG/JU
 Sample : M2970-16DL 5X
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGE17DL

Manual Integrations
 APPROVED

mohammad
 7/26/2021 7:59:52 AM

Quant Time: Jul 23 11:57:34 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM072221.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 22 11:33:47 2021
 Response via : Initial Calibration

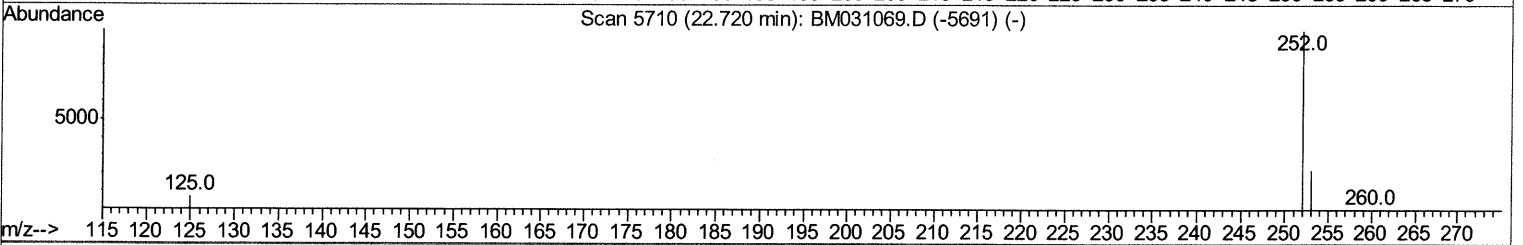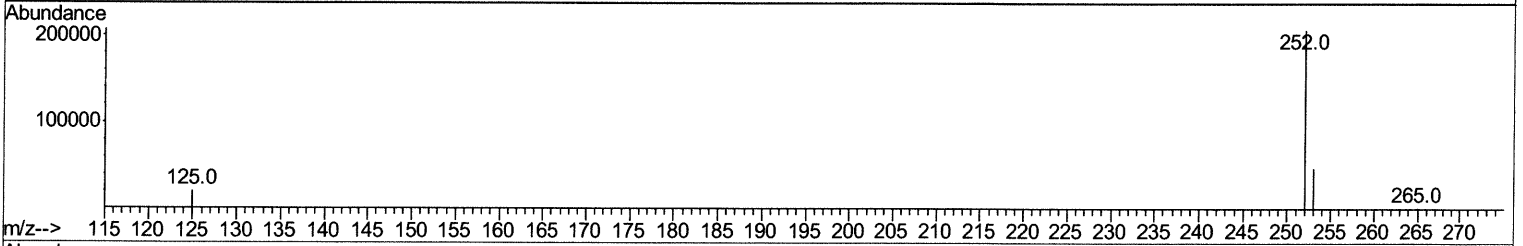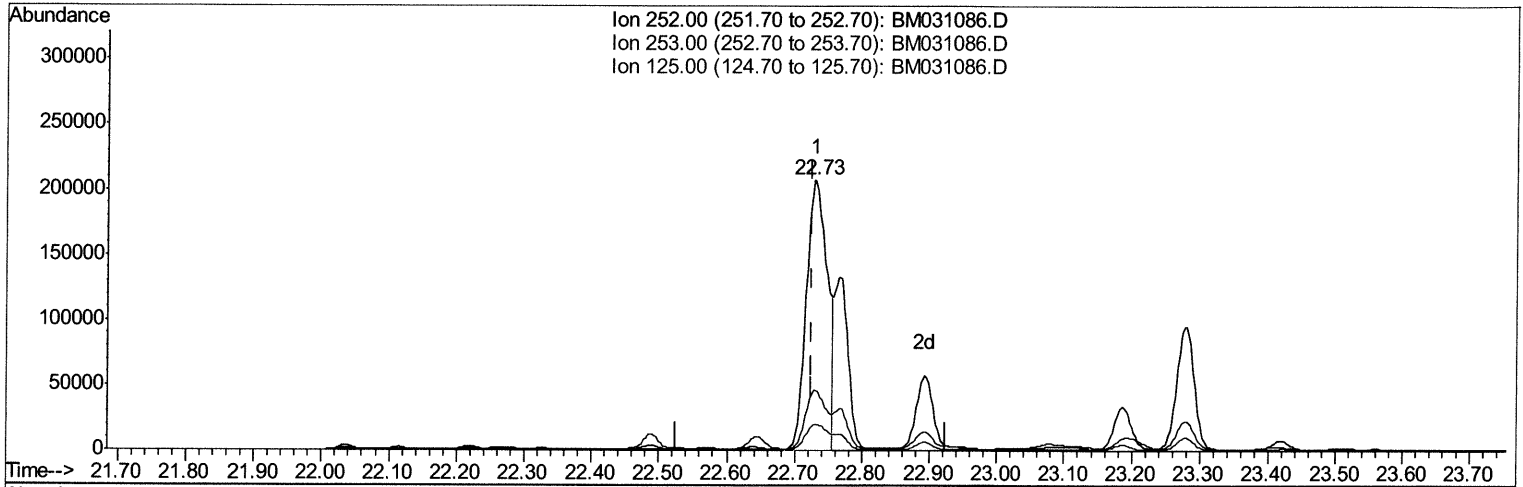

TIC: BM031086.D

(24) Benzo(b)fluoranthene

22.730min (+0.005) 7.94ng/ul m

07/26/21 JU

response 442295

Ion	Exp%	Act%
252.00	100	100
253.00	26.40	22.49
125.00	10.10	9.70
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM072221\
 Data File : BM031086.D
 Acq On : 23 Jul 2021 11:26
 Operator : CG/JU
 Sample : M2970-16DL 5X
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_M
ClientSampleId :
 BGE17DL

Manual Integrations
APPROVED

mohammad
 7/26/2021 7:59:52 AM

Quant Time: Jul 23 11:57:34 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM072221.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 22 11:33:47 2021
 Response via : Initial Calibration

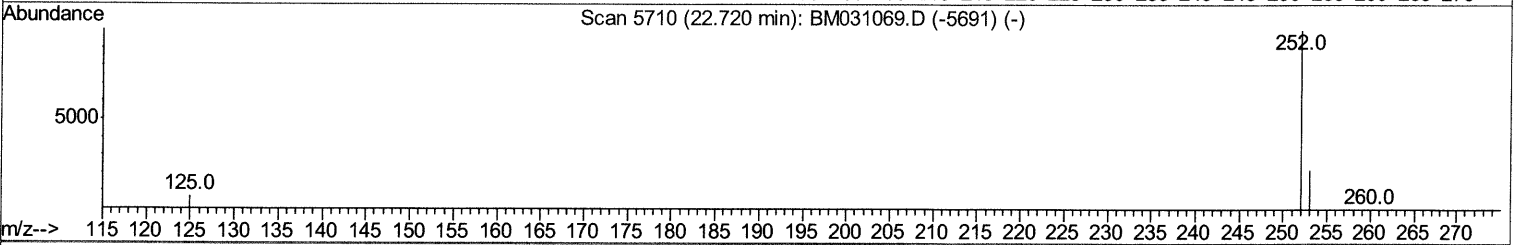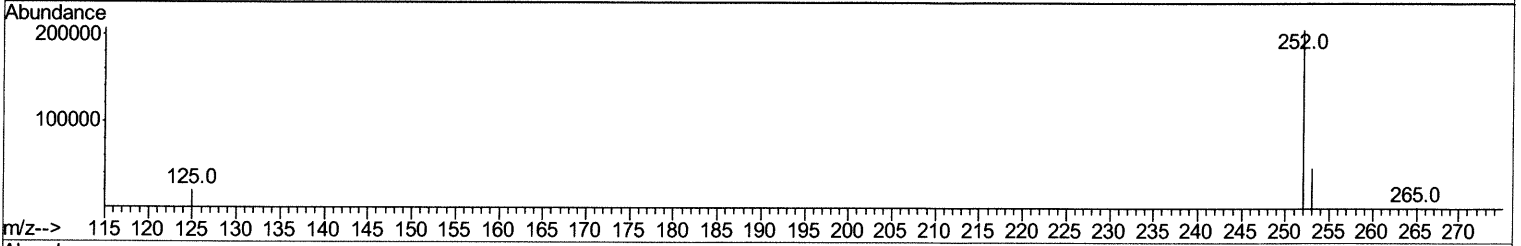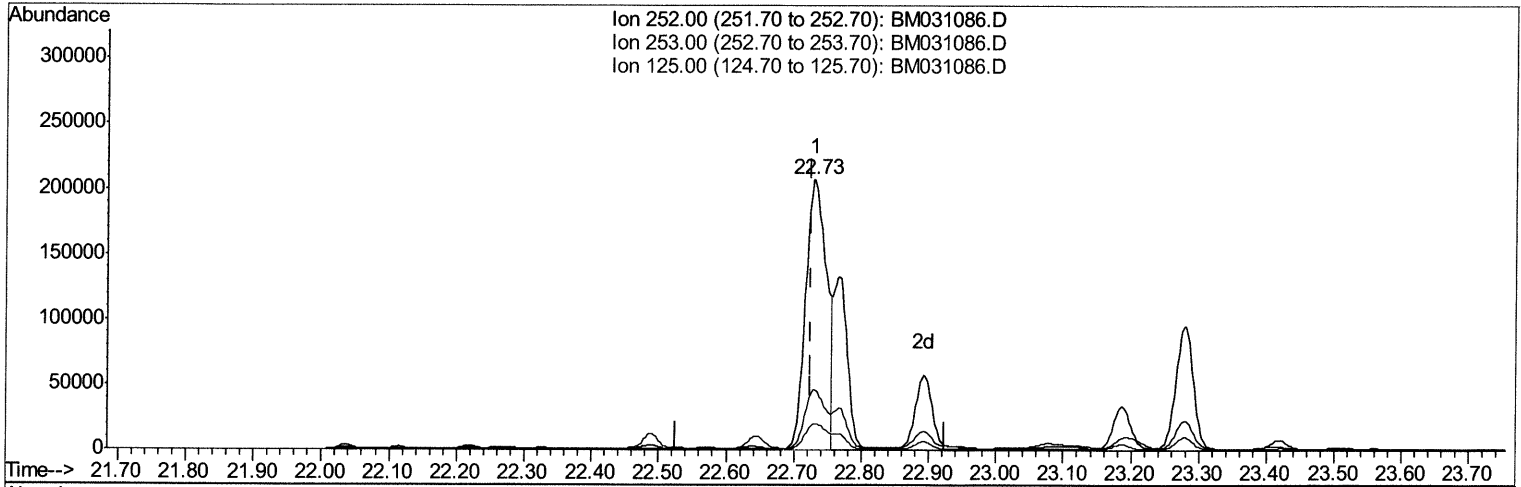

TIC: BM031086.D

(24) Benzo(b)fluoranthene

22.730min (+0.005) 7.94ng/ul m 07/26/21 JU

response 442295

Ion	Exp%	Act%
252.00	100	100
253.00	26.40	22.49
125.00	10.10	9.70
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM072221\
 Data File : BM031086.D
 Acq On : 23 Jul 2021 11:26
 Operator : CG/JU
 Sample : M2970-16DL 5X
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_M
ClientSampleId :
 BGE17DL

Manual Integrations
APPROVED

mohammad
 7/26/2021 7:59:52 AM

Quant Time: Jul 23 11:57:34 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM072221.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 22 11:33:47 2021
 Response via : Initial Calibration

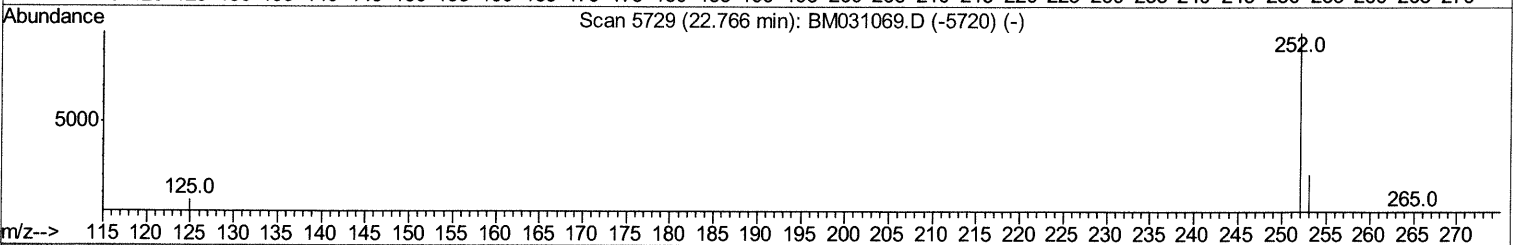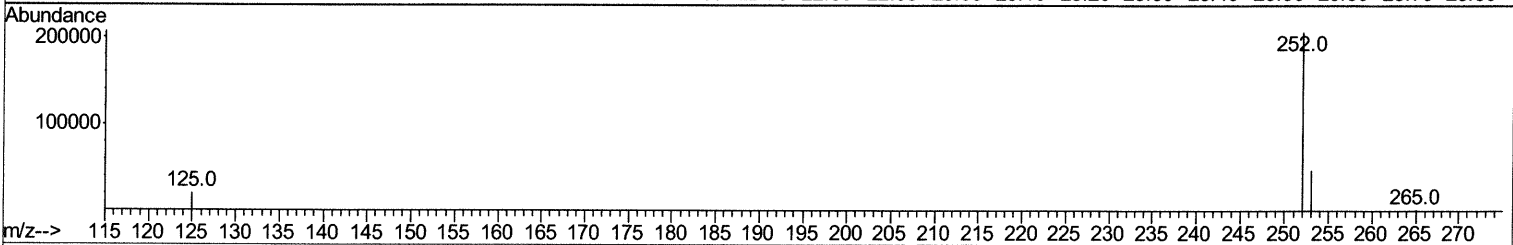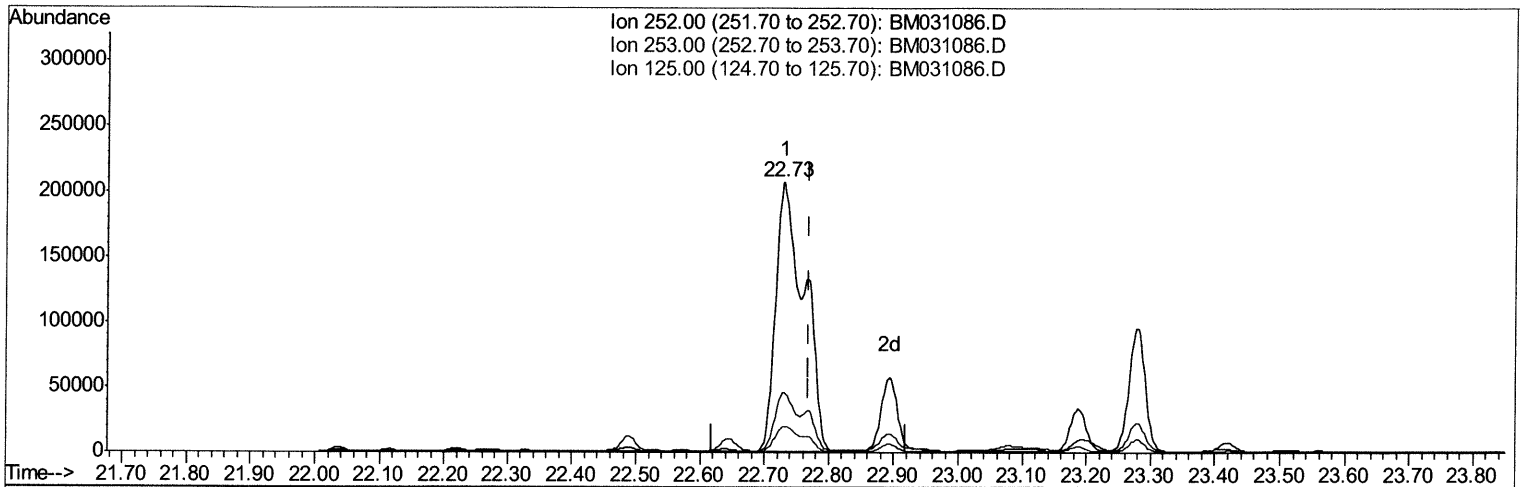

TIC: BM031086.D

(25) Benzo(k)fluoranthene
 22.730min (-0.039) 11.20ng/ul
 response 632793

Ion	Exp%	Act%
252.00	100	100
253.00	27.00	22.49
125.00	10.80	9.70
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM072221\
 Data File : BM031086.D
 Acq On : 23 Jul 2021 11:26
 Operator : CG/JU
 Sample : M2970-16DL 5X
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGE17DL

Manual Integrations
 APPROVED

mohammad
 7/26/2021 7:59:52 AM

Quant Time: Jul 23 11:57:34 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM072221.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 22 11:33:47 2021
 Response via : Initial Calibration

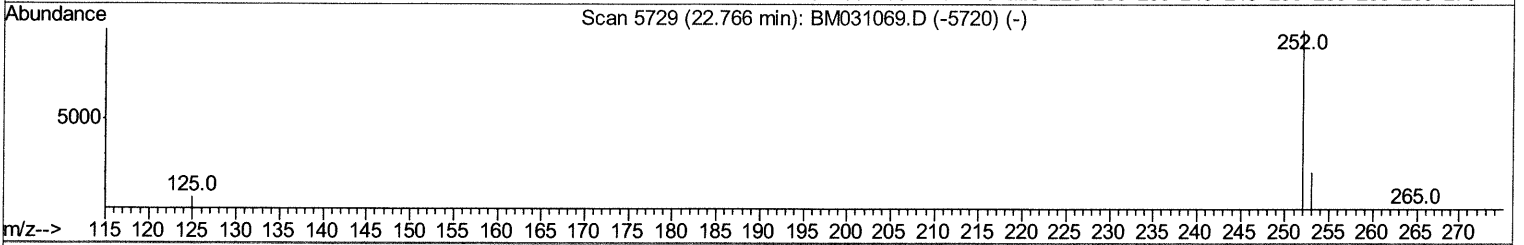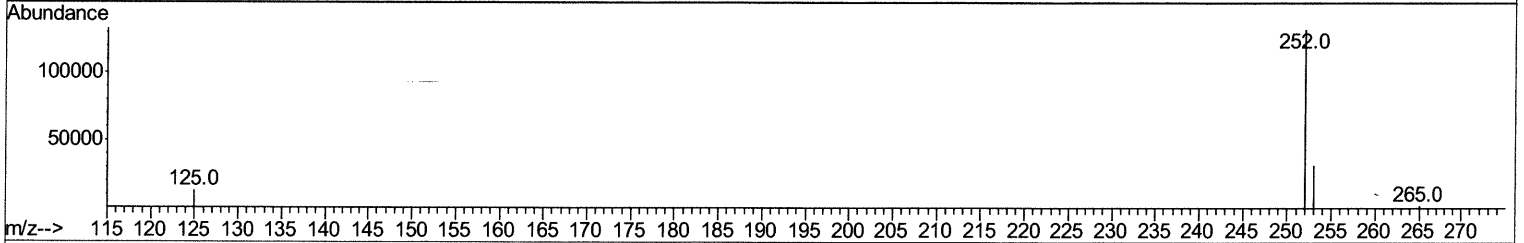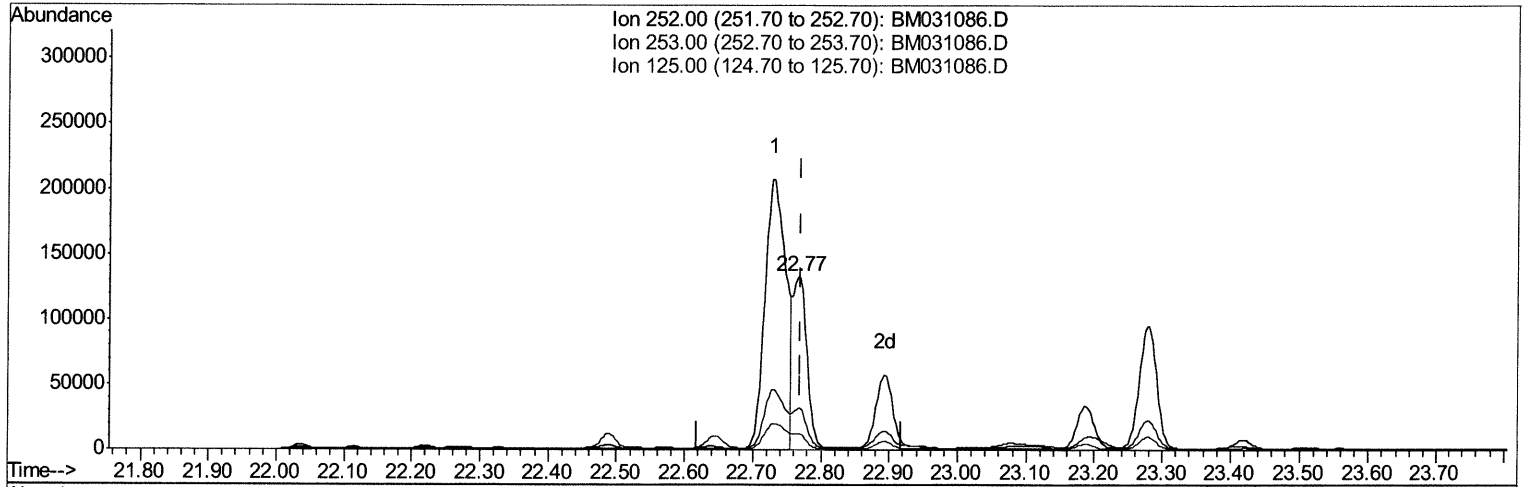

TIC: BM031086.D

(25) Benzo(k)fluoranthene

22.767min (-0.002) 3.44ng/ul m 07/26/21 JU

response 194413

Ion	Exp%	Act%
252.00	100	100
253.00	27.00	23.85
125.00	10.80	9.50
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM072221\
 Data File : BM031086.D
 Acq On : 23 Jul 2021 11:26
 Operator : CG/JU
 Sample : M2970-16DL 5X
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGE17DL

Manual Integrations
 APPROVED

mohammad
 7/26/2021 7:59:52 AM

Quant Time: Jul 23 11:59:47 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM072221.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 22 11:33:47 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	1966	0.40	ng/ul	0.00
4) Naphthalene-d8	10.40	136	7997	0.40	ng/ul	0.00
9) Acenaphthene-d10	14.26	164	5424	0.40	ng/ul	0.00
13) Phenanthrene-d10	17.01	188	11917	0.40	ng/ul	0.00
17) Chrysene-d12	21.20	240	11979	0.40	ng/ul	0.00
23) Perylene-d12	23.37	264	11844	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.21	96	1130	0.55	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.99	152	582	0.04	ng/ul	0.00
18) Fluoranthene-d10	19.04	212	1554	0.04	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
5) Naphthalene	10.45	128	8931	0.374	ng/ul	98
7) 2-Methylnaphthalene	12.07	142	1430	0.083	ng/ul	99
8) 1-Methylnaphthalene	12.29	142	375	0.022	ng/ul	100
10) Acenaphthylene	13.98	152	13944	0.629	ng/ul	97
11) Acenaphthene	14.33	153	9836	0.502	ng/ul	98
12) Fluorene	15.32	166	15390	0.667	ng/ul	99
15) Phenanthrene	17.05	178	407813	10.775	ng/ul	99
16) Anthracene	17.14	178	167047	4.711	ng/ul	97
19) Fluoranthene	19.07	202	865722	17.952	ng/ul	96
20) Pyrene	19.43	202	503991	10.237	ng/ul	96
21) Benzo(a)anthracene	21.18	228	495568	10.358	ng/ul	96
22) Chrysene	21.23	228	390440	7.540	ng/ul	98
24) Benzo(b)fluoranthene	22.73	252	442295m	7.943	ng/ul	98
25) Benzo(k)fluoranthene	22.77	252	194413m	3.441	ng/ul	98
26) Benzo(a)pyrene	23.28	252	168532	3.501	ng/ul#	91
27) Indeno(1,2,3-cd)pyrene	25.53	276	106954	1.696	ng/ul#	97
28) Dibenzo(a,h)anthracene	25.54	278	46973	0.928	ng/ul	98
29) Benzo(a,h,i)perylene	26.19	276	3678	0.069	ng/ul#	65

(#) = qualifier out of range (m) = manual integration (+) = signals summed