


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM072318\
 Data File : BM016019.D
 Acq On : 23 Jul 2018 11:01
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM072318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jul 23 16:08:38 2018

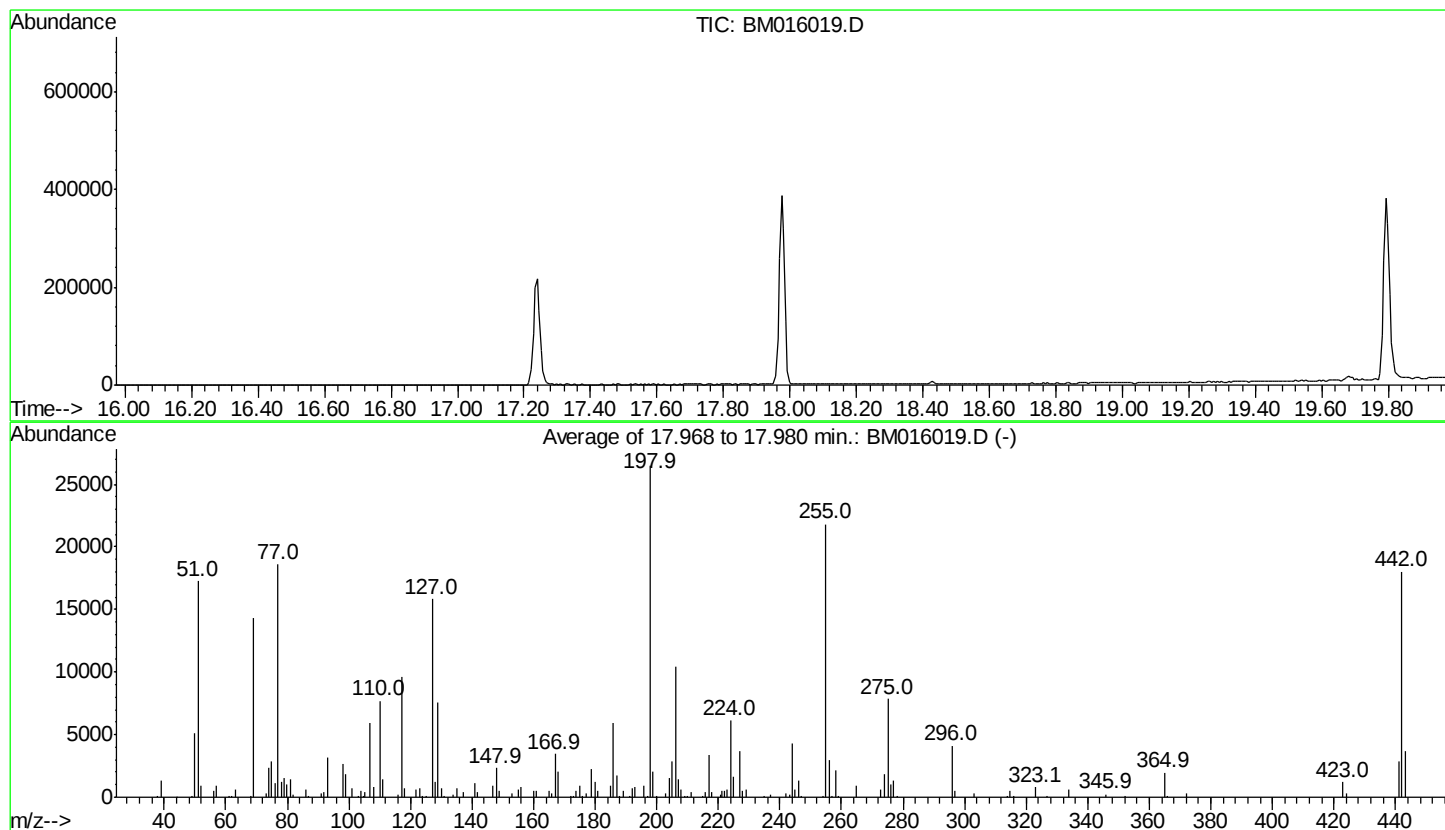

AutoFind: Scans 2496, 2497, 2498; Background Corrected with Scan 2490

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	65.1	17233	PASS
68	69	0.00	2	0.8	112	PASS
69	198	0.00	100	53.9	14276	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	59.8	15835	PASS
197	198	0.00	2	0.4	108	PASS
198	198	100	100	100.0	26488	PASS
199	198	5	9	7.6	2004	PASS
275	198	10	60	29.7	7855	PASS
365	198	1	100	7.4	1968	PASS
441	198	0.01	100	10.8	2859	PASS
442	198	50	100	68.1	18030	PASS
443	442	15	24	20.5	3689	PASS