


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM072318\
 Data File : BM016028.D
 Acq On : 23 Jul 2018 16:32
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM072318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jul 23 16:08:38 2018

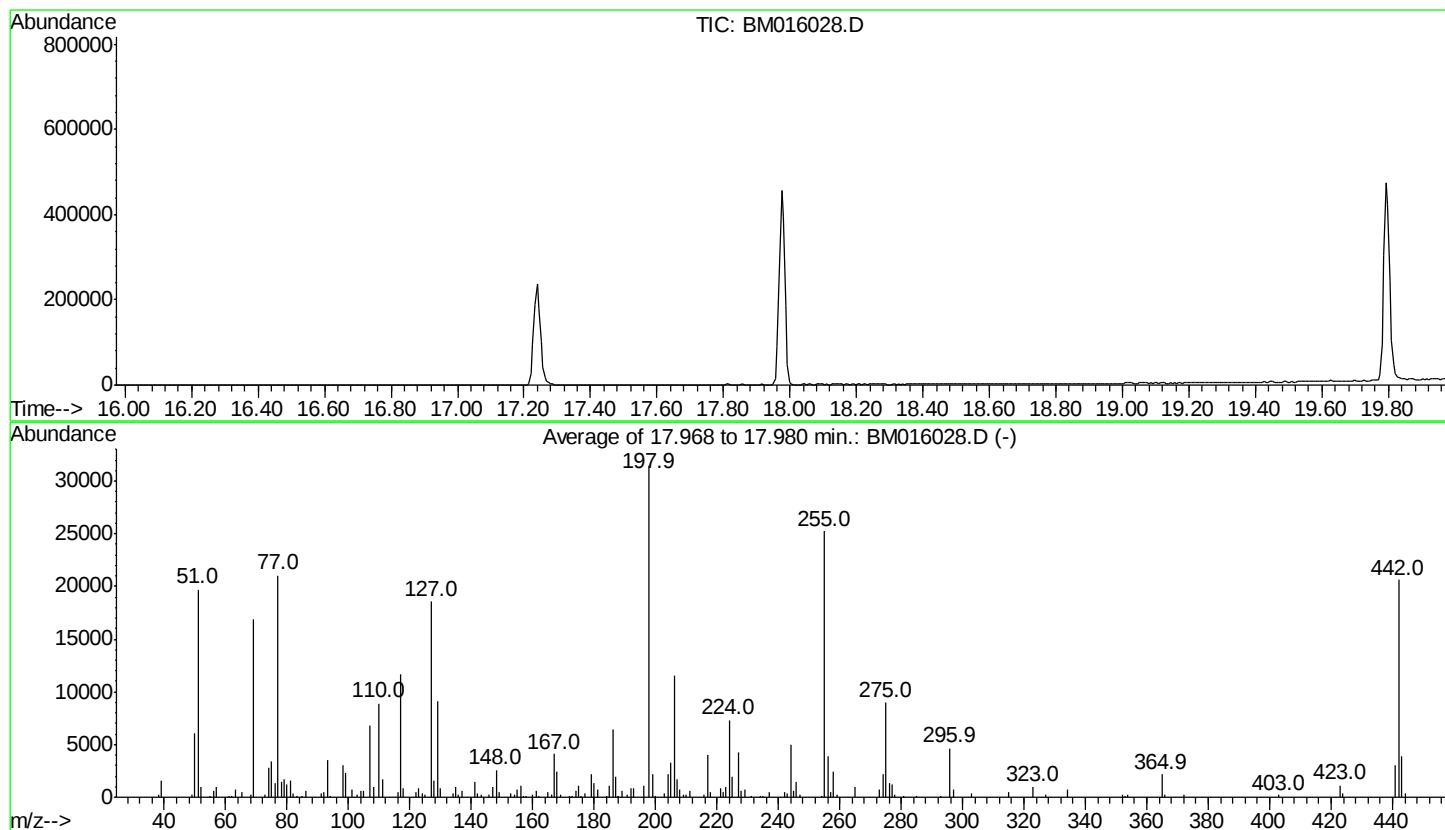

AutoFind: Scans 2496, 2497, 2498; Background Corrected with Scan 2491

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	62.7	19725	PASS
68	69	0.00	2	1.3	228	PASS
69	198	0.00	100	53.8	16933	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	58.9	18534	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	31464	PASS
199	198	5	9	7.1	2224	PASS
275	198	10	60	28.5	8974	PASS
365	198	1	100	6.8	2133	PASS
441	198	0.01	100	9.8	3070	PASS
442	198	50	100	65.6	20631	PASS
443	442	15	24	19.0	3920	PASS