


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM072318\
 Data File : BM016047.D
 Acq On : 24 Jul 2018 04:13
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM072318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jul 23 16:08:38 2018

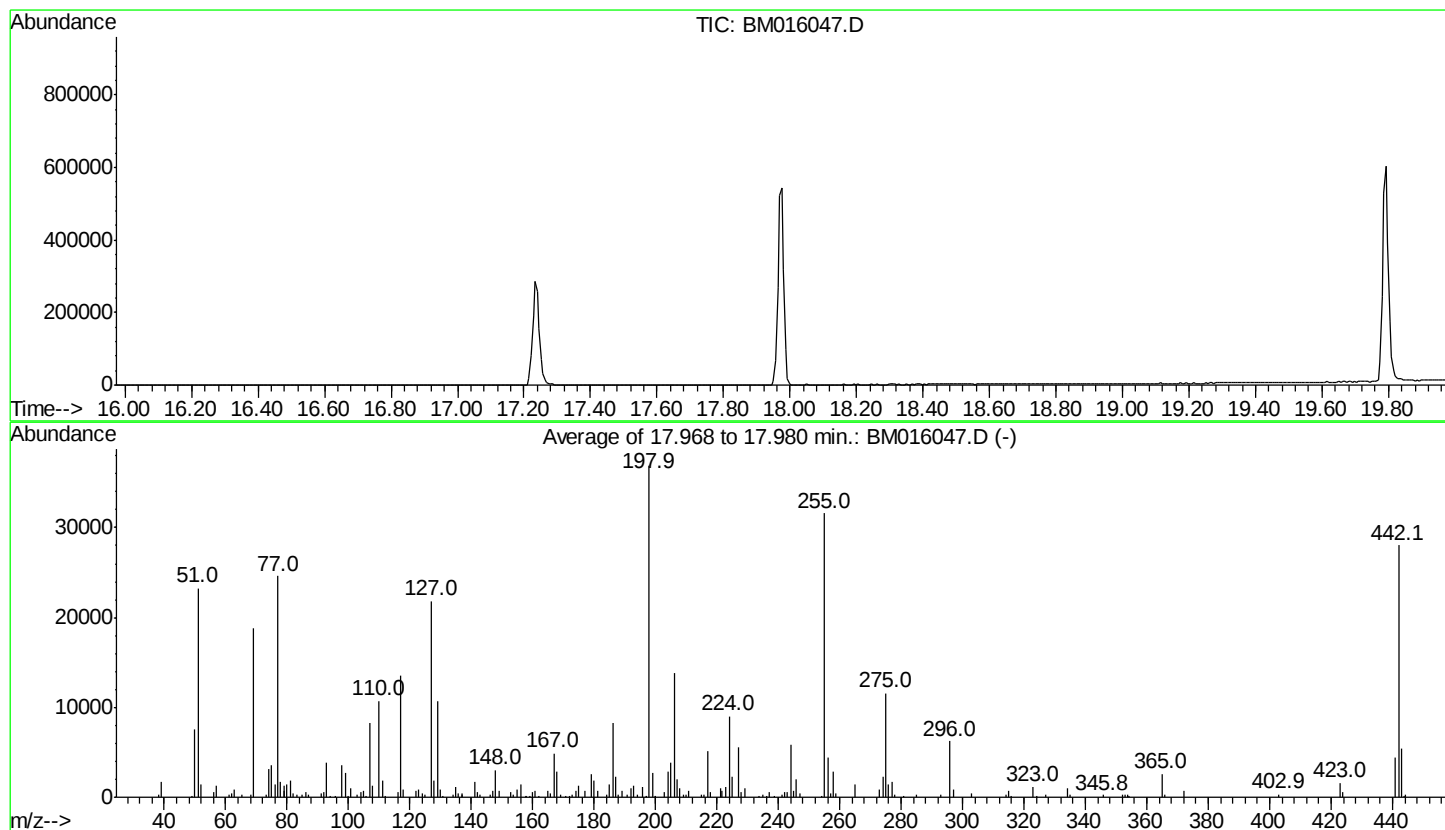

AutoFind: Scans 2496, 2497, 2498; Background Corrected with Scan 2490

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	62.9	23224	PASS
68	69	0.00	2	1.8	345	PASS
69	198	0.00	100	51.1	18840	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	59.1	21807	PASS
197	198	0.00	2	0.4	160	PASS
198	198	100	100	100.0	36901	PASS
199	198	5	9	7.3	2711	PASS
275	198	10	60	31.3	11548	PASS
365	198	1	100	7.1	2606	PASS
441	198	0.01	100	11.8	4364	PASS
442	198	50	100	76.0	28050	PASS
443	442	15	24	19.3	5402	PASS