

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM072319\
 Data File : BM021616.D
 Acq On : 23 Jul 2019 18:23
 Operator : HP/JU
 Sample : K3890-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A52Q7

Quant Time: Jul 24 01:24:27 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM072319MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 24 01:21:49 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.70	152	85287	20.00	ng/ul	0.00
18) Naphthalene-d8	10.49	136	389746	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.35	164	281516	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.10	188	683274	20.00	ng/ul	0.00
77) Chrysene-d12	21.29	240	800670	20.00	ng/ul	0.00
85) Perylene-d12	23.54	264	981576	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.25	96	13991	8.94	ng/uL	0.00
5) Phenol-d5	6.88	99	66027	9.13	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.05	67	159673	38.05	ng/ul	0.00
9) 2-Chlorophenol-d4	7.23	132	180650	31.84	ng/ul	0.00
13) 4-Methylphenol-d8	8.41	113	130292	21.09	ng/ul	0.00
19) Nitrobenzene-d5	8.87	128	121571	42.14	ng/ul	0.00
22) 2-Nitrophenol-d4	9.58	143	131160	42.38	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.12	165	253318	36.70	ng/ul	0.00
29) 4-Chloroaniline-d4	10.66	131	28438	4.25	ng/ul	0.02
43) Dimethylphthalate-d6	13.76	166	1026648	42.56	ng/ul	0.00
46) Acenaphthylene-d8	14.04	160	1122479	38.26	ng/ul	0.00
51) 4-Nitrophenol-d4	14.59	143	18715	4.52	ng/ul	0.02
57) Fluorene-d10	15.35	176	903255	41.50	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.48	200	121706	28.44	ng/ul	0.00
70) Anthracene-d10	17.20	188	1558082	46.35	ng/ul	0.00
78) Pyrene-d10	19.50	212	1932308	49.45	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.40	264	2424142	46.25	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	13.81	163	92457	3.993	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM072319\
Data File : BM021616.D
Acq On : 23 Jul 2019 18:23
Operator : HP/JU
Sample : K3890-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A52Q7

Quant Time: Jul 24 01:24:27 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM072319MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jul 24 01:21:49 2019
Response via : Initial Calibration

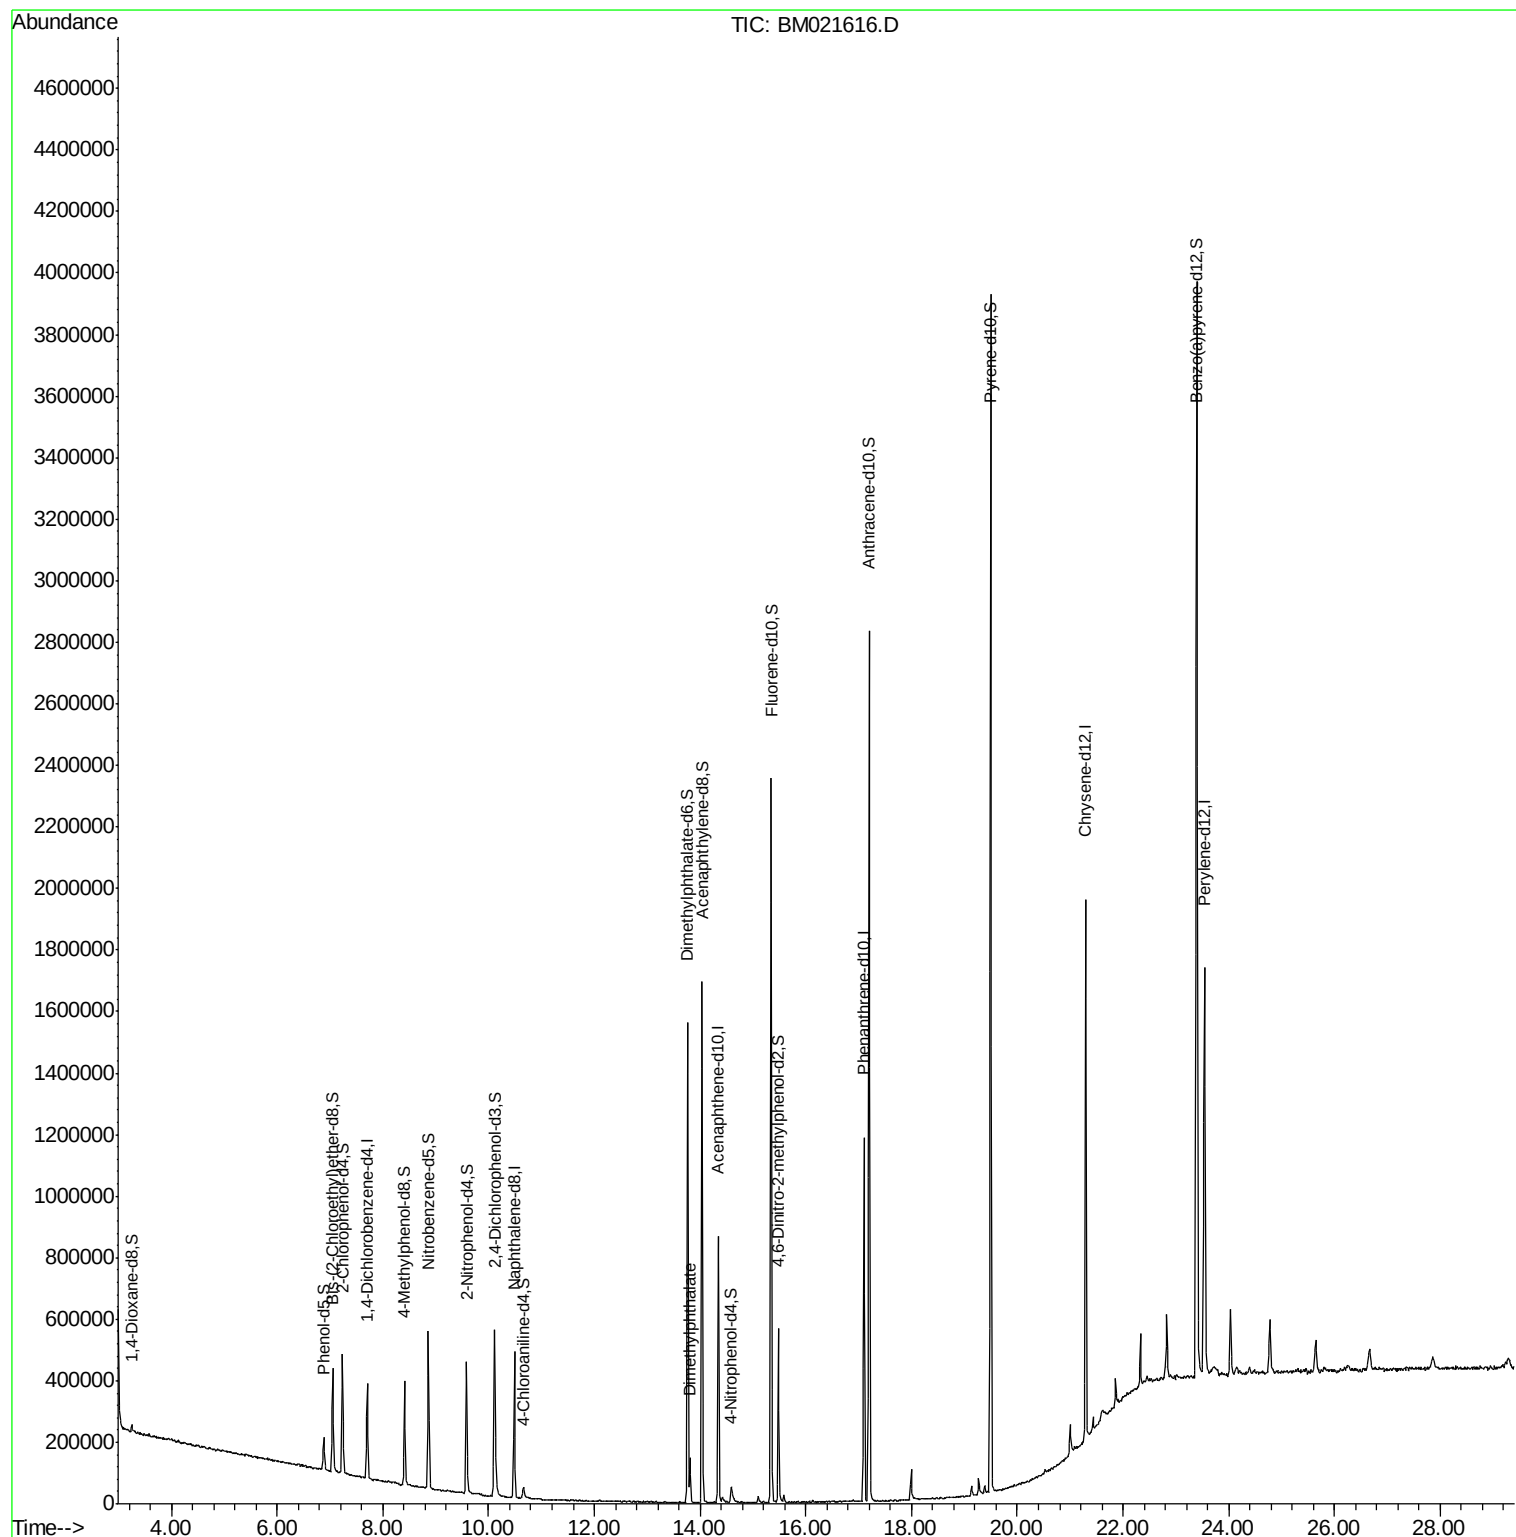

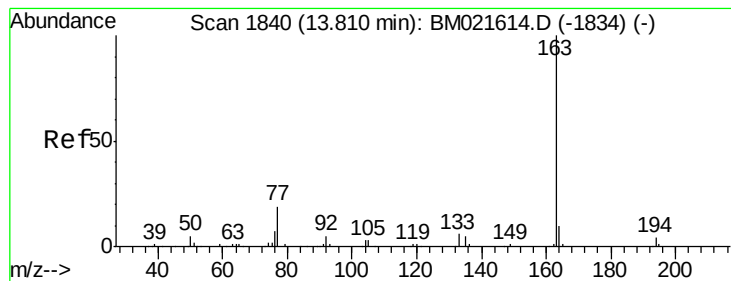

#44

Dimethylphthalate

Concen: 3.993 ng/ul

RT: 13.81 min Scan# 1840

Delta R.T. 0.00 min

Lab File: BM021616.D

Acq: 23 Jul 2019 18:23

Instrument :

BNA_M

ClientSampleId :

A52Q7


Tgt Ion:163 Resp: 92457

Ion Ratio Lower Upper

163 100

194 4.0 3.2 4.8

164 10.8 8.2 12.4

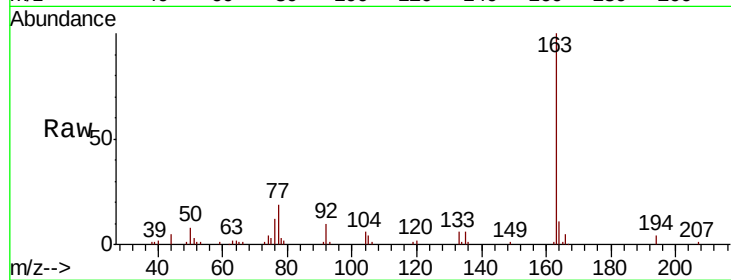

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

