
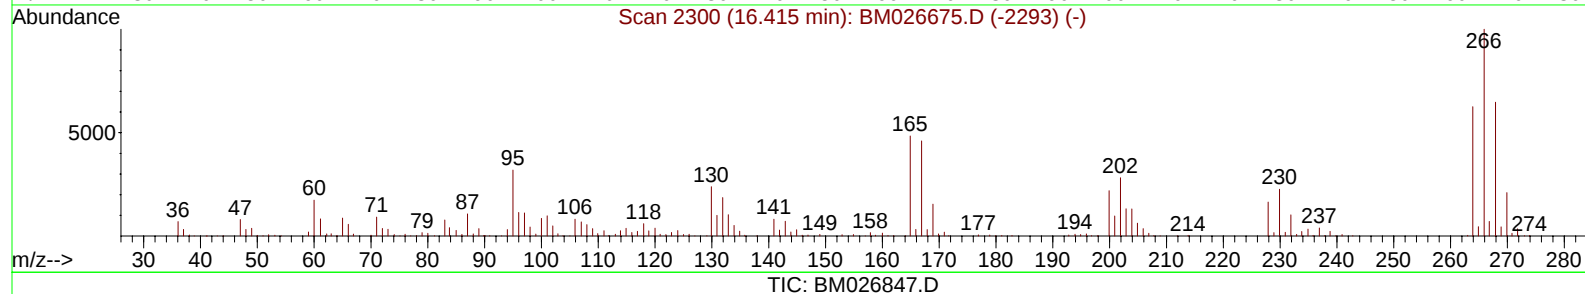
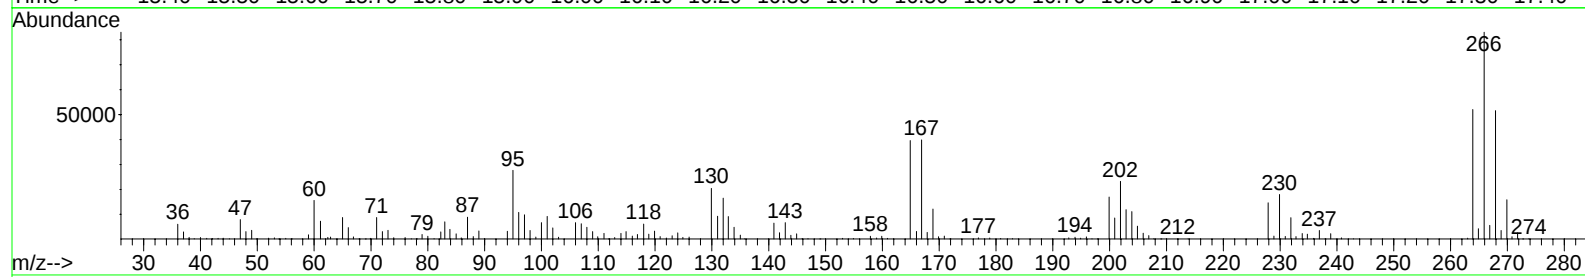


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM072320\
 Data File : BM026847.D
 Acq On : 23 Jul 2020 11:59
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 23 18:55:19 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM070820.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 22 14:16:10 2020
 Response via : Initial Calibration

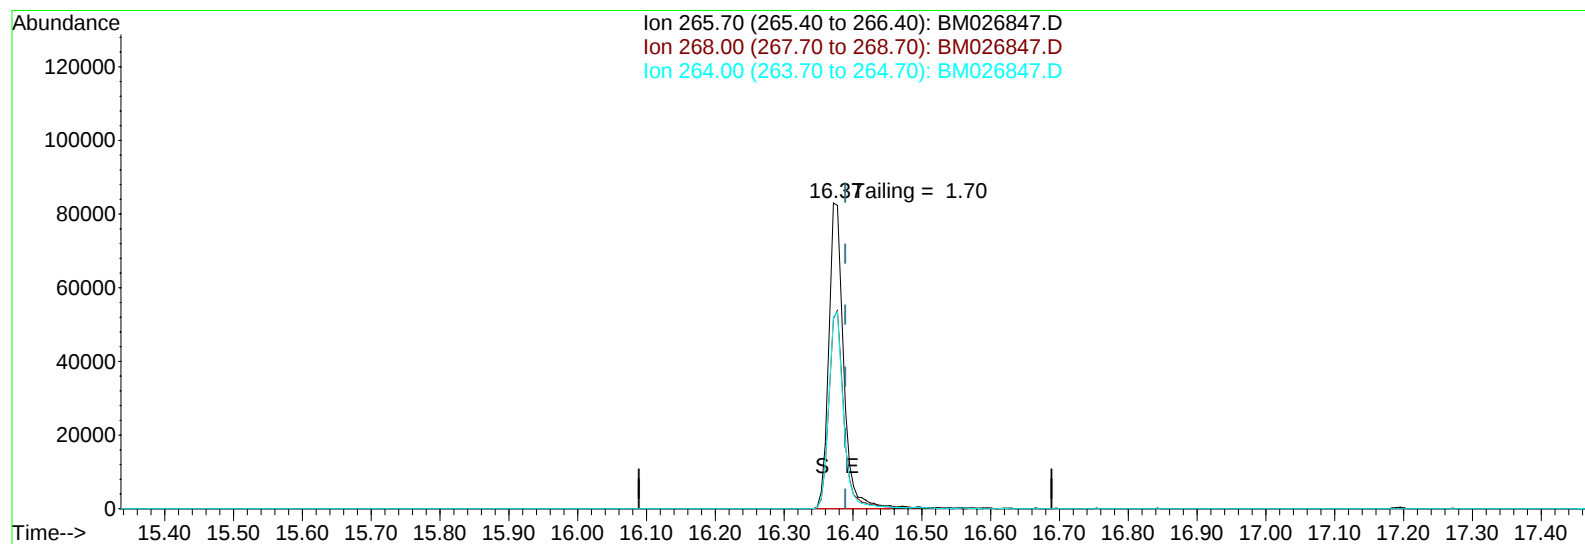

(70) Pentachlorophenol (C)




16.372min (-0.017) 285610.87ng

response 124884

Ion	Exp%	Act%
265.70	100	100
268.00	64.70	62.12
264.00	62.60	62.71
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM072320\
 Data File : BM026847.D
 Acq On : 23 Jul 2020 11:59
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 23 18:55:19 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM070820.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 22 14:16:10 2020
 Response via : Initial Calibration

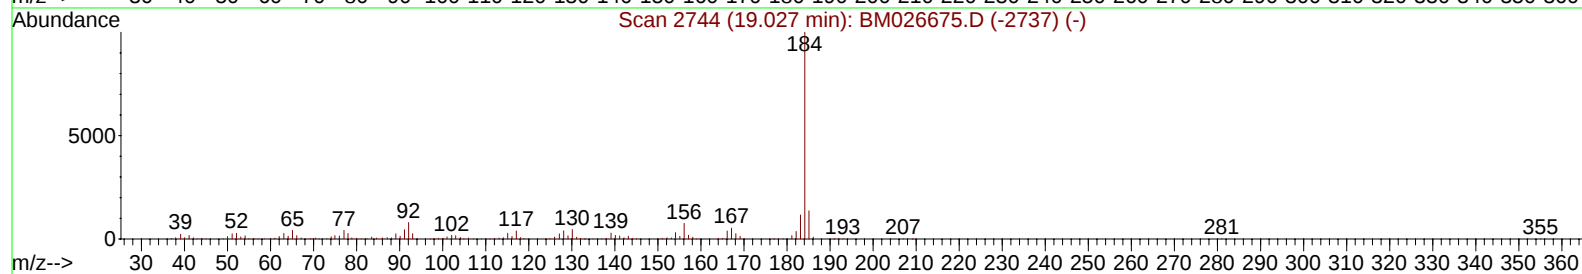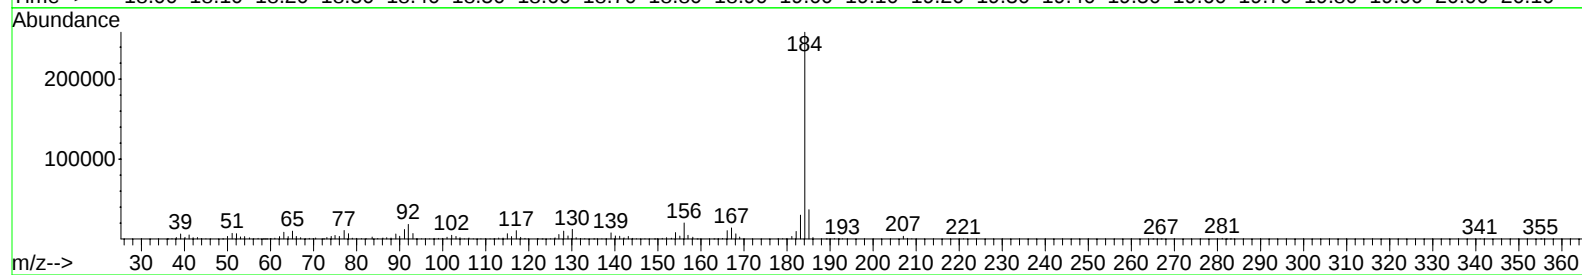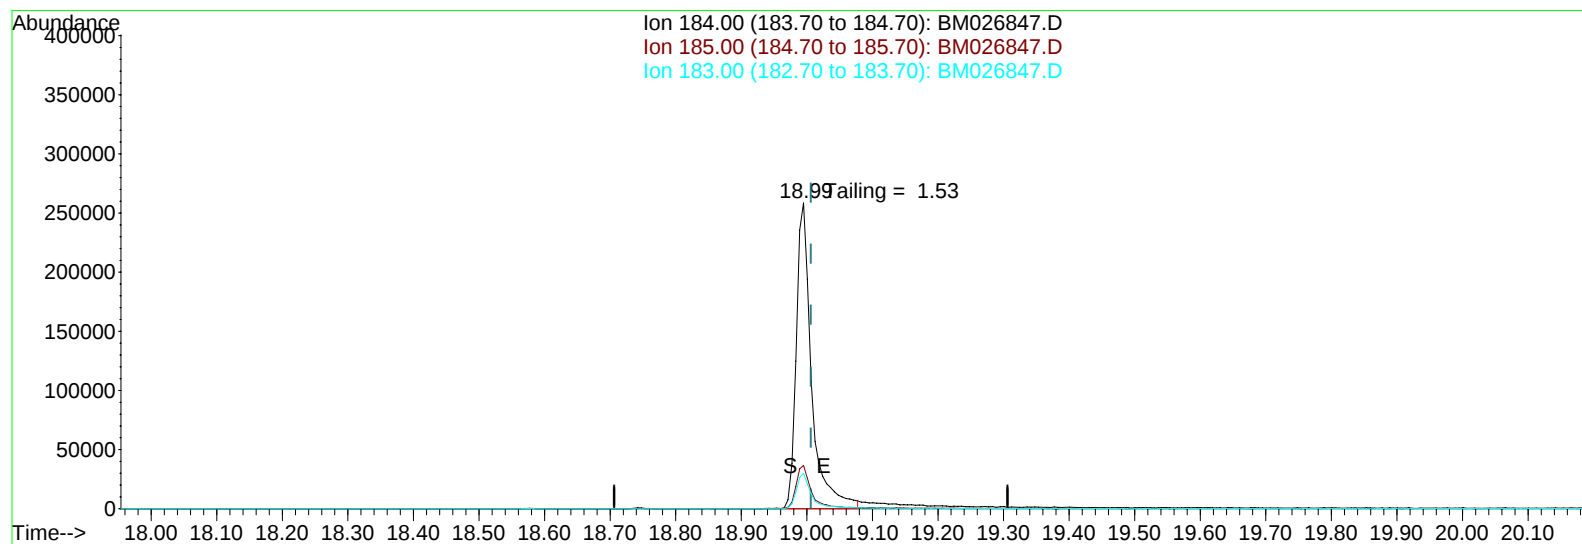

TIC: BM026847.D

(77) Benzidine

18.995min (-0.011) 30940.61ng

response 448345

Ion	Exp%	Act%
184.00	100	100
185.00	13.60	14.20
183.00	11.60	11.58
0.00	0.00	0.00